

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
 Data File : P0061975.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Oct 2019 20:59
 Operator : HP/AJ
 Sample : K5350-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-209

Manual Integrations
 APPROVED

Ankita
 10/15/2019 9:02:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:08:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.325	3.486	1274520	879405	20.608m	20.508
2)	SA Decachlor...	9.954	8.340	917819	436148	16.403	14.865

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061975.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Oct 2019 20:59
Operator : HP/AJ
Sample : K5350-01
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-209


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:08:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

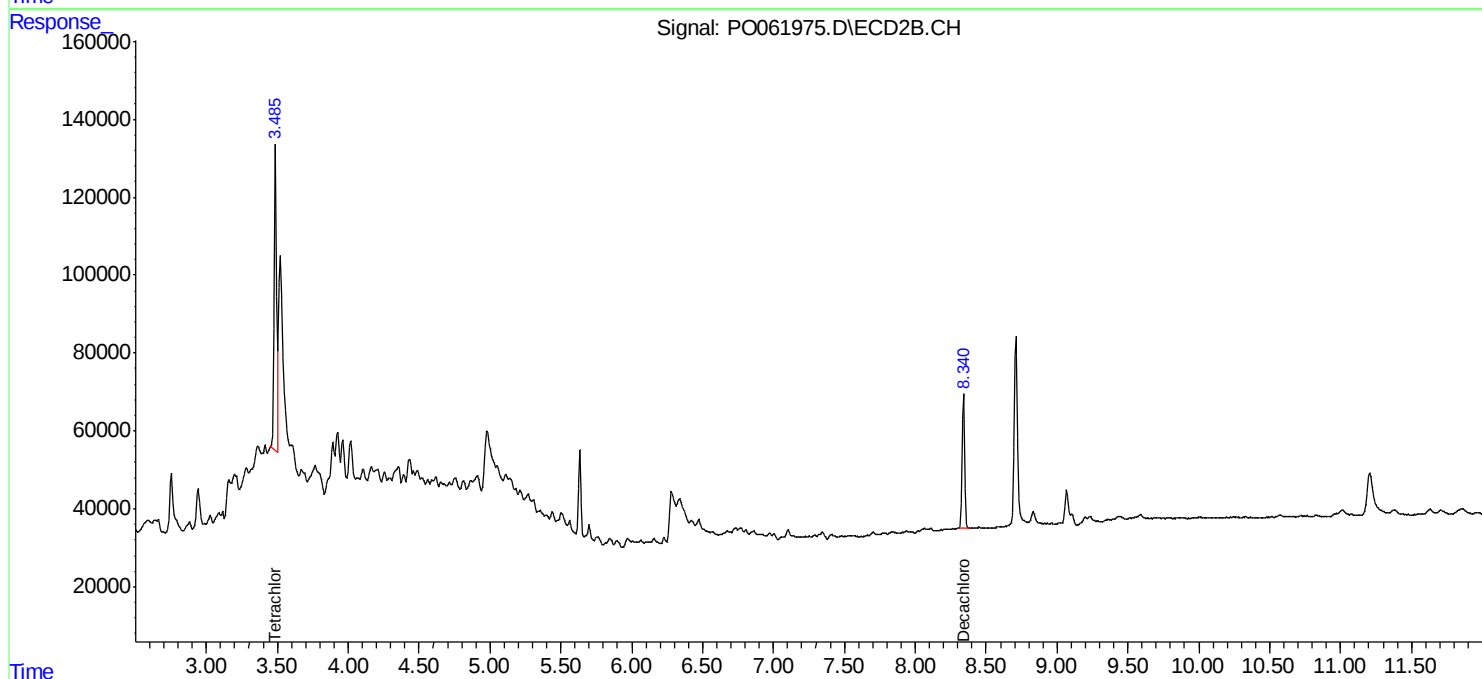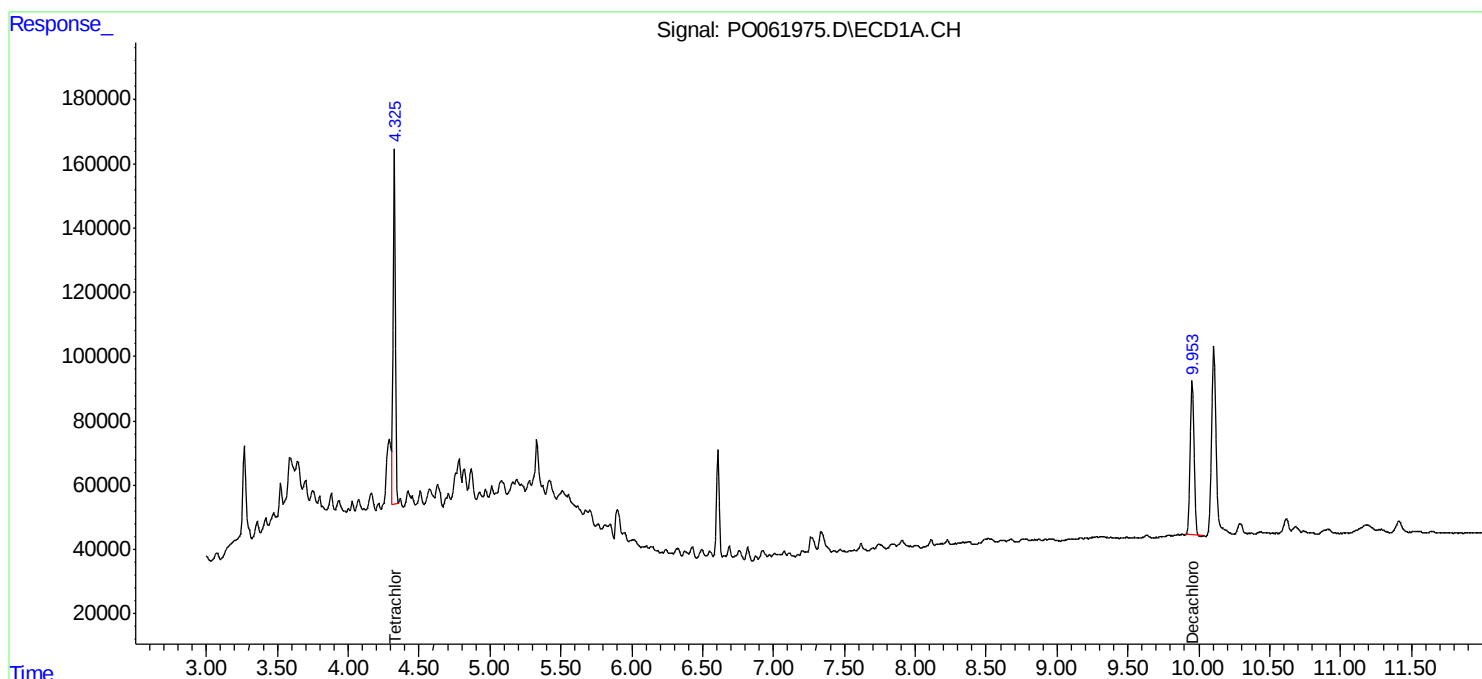

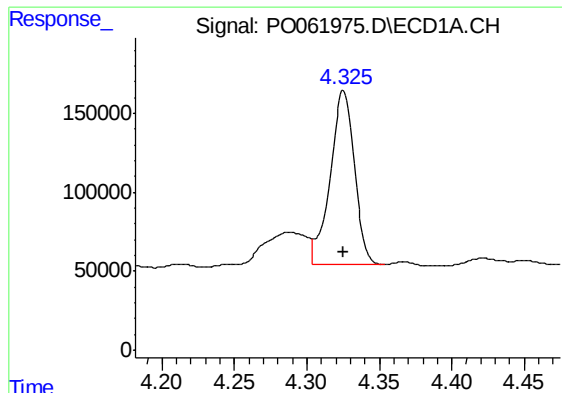


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 1274520
Conc: 20.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VNJ-209


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:25 AM

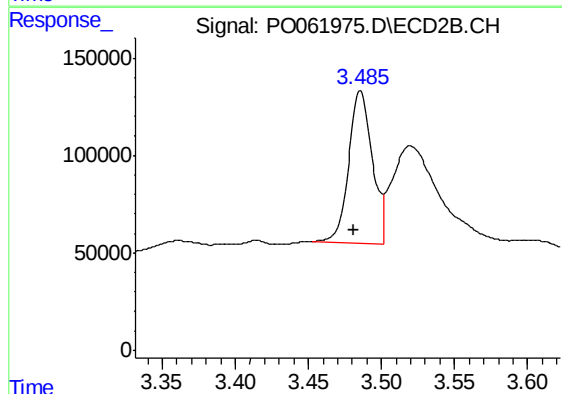


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: 0.004 min
Response: 879405
Conc: 20.51 ng/ml

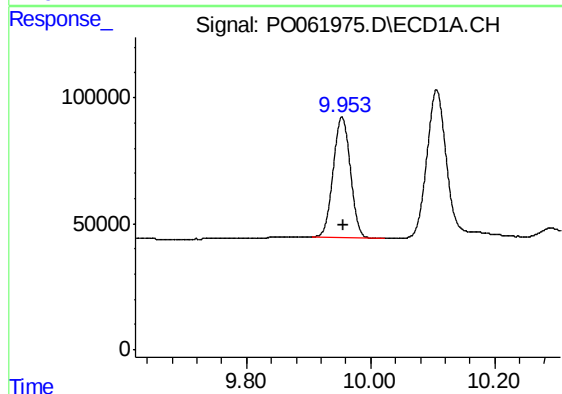

#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.003 min
Response: 917819
Conc: 16.40 ng/ml

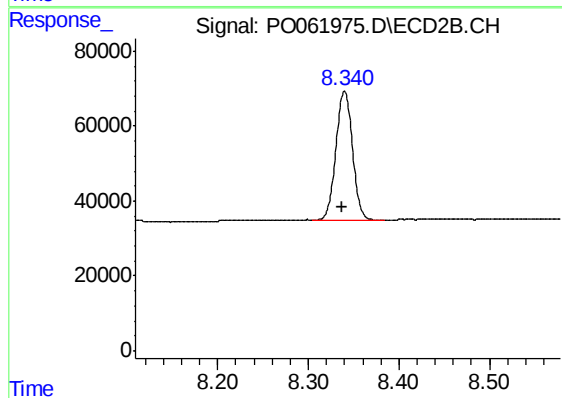

#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.002 min
Response: 436148
Conc: 14.86 ng/ml