

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
 Data File : P0061976.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Oct 2019 21:15
 Operator : HP/AJ
 Sample : K5350-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-230

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:09:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.484	1327368	967845	21.462	22.570
2)	SA Decachlor...	9.953	8.339	1068568	527938	19.098	17.993
Target Compounds							
21)	L5 AR-1248-1	5.484	4.527	30082	20787	20.989m	21.173m
22)	L5 AR-1248-2	5.757	4.757	40430	31048	20.194	24.507
23)	L5 AR-1248-3	5.958	4.796	35835	27719	16.225m	20.881 #
24)	L5 AR-1248-4	6.362	4.962	187228	34881	73.289	22.044 #
25)	L5 AR-1248-5	6.399	5.343	319451	44972	130.647	29.221 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Ankita

10/15/2019 9:02:27 AM



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061976.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Oct 2019 21:15
Operator : HP/AJ
Sample : K5350-05
Misc :
ALS Vial : 37 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
VNJ-230

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:09:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

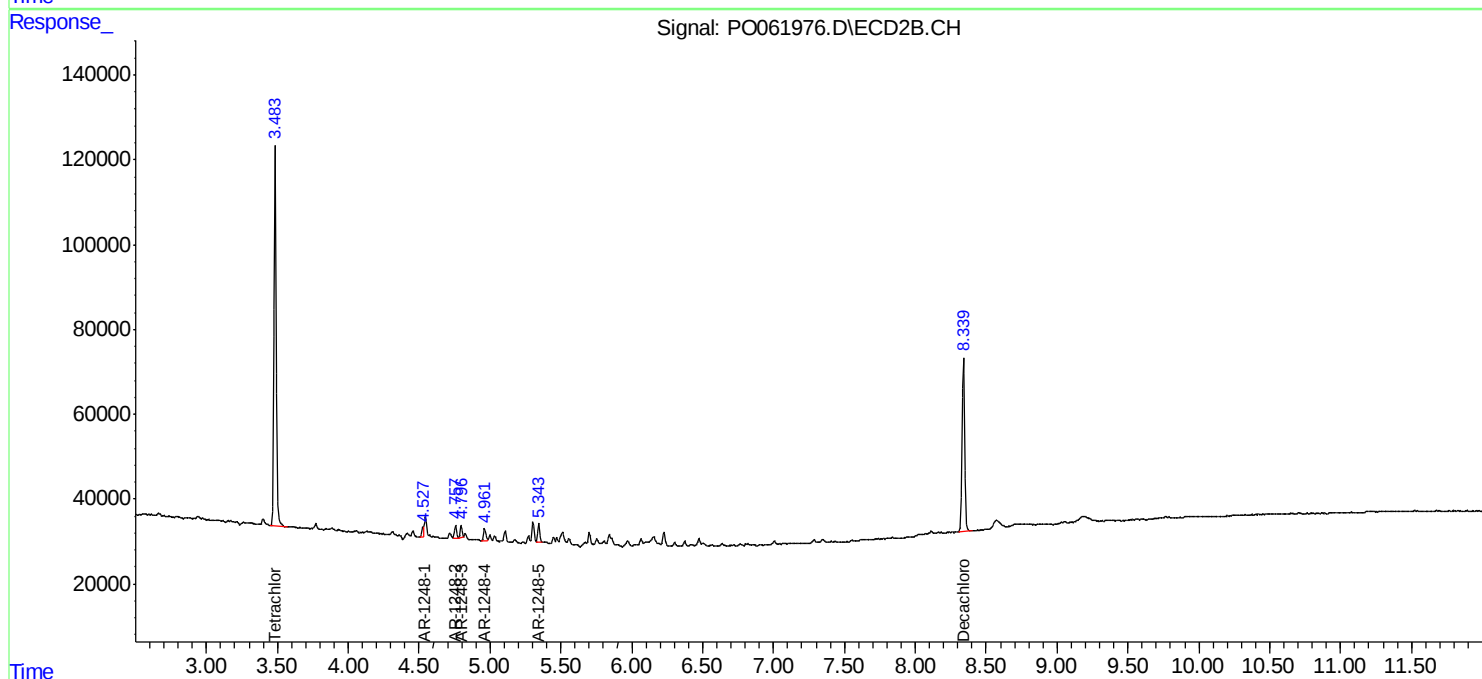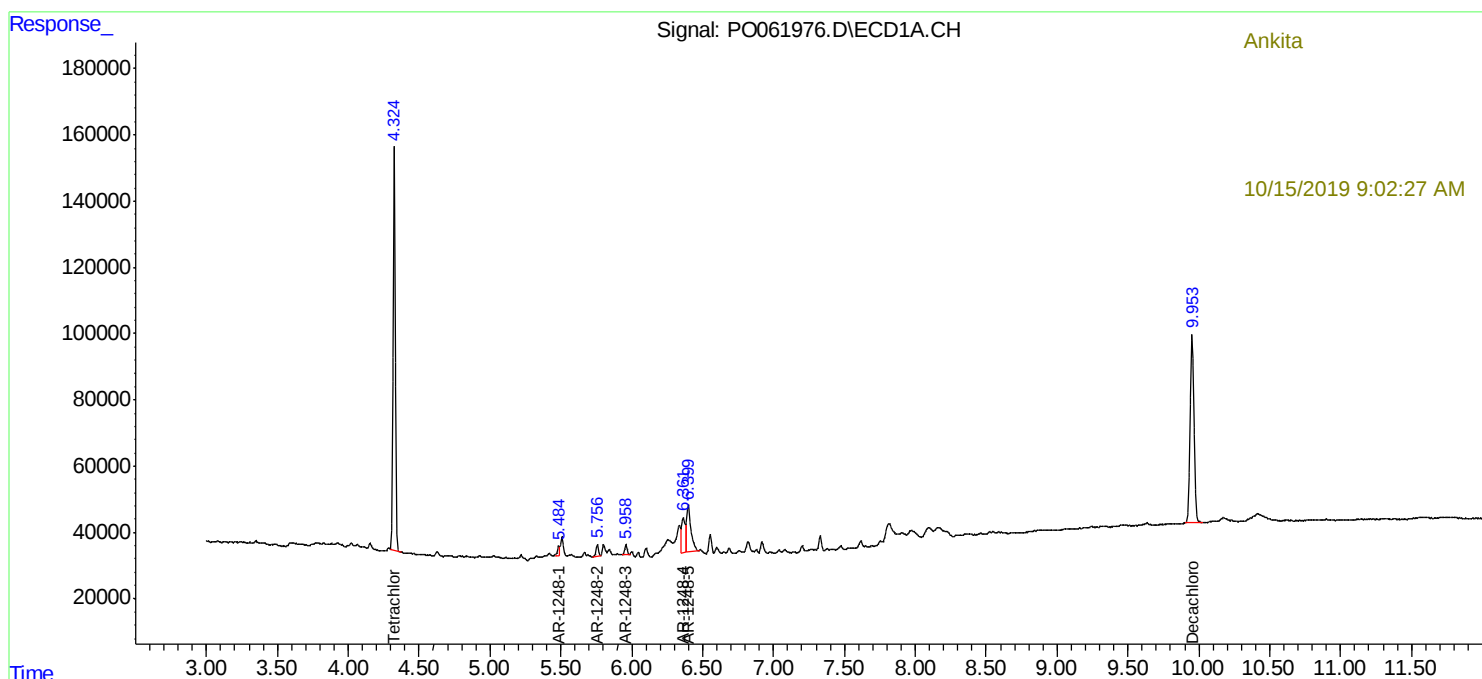

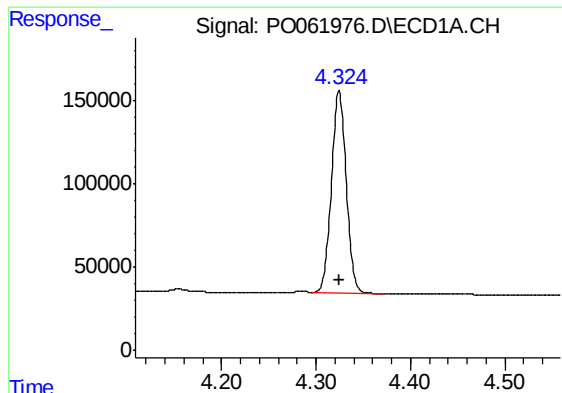


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: 0.000 min
Response: 1327368
Conc: 21.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-230


Manual Integrations
APPROVED

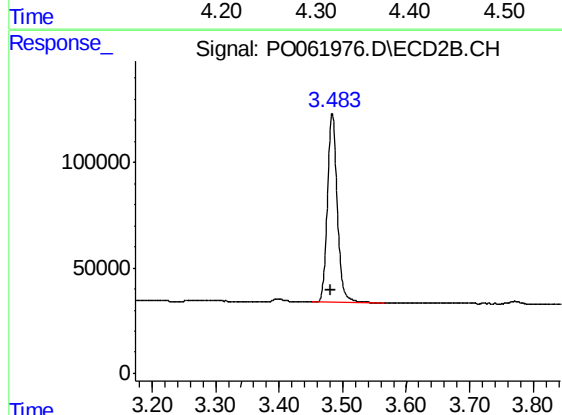

#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.002 min
Response: 967845
Conc: 22.57 ng/ml


Ankita

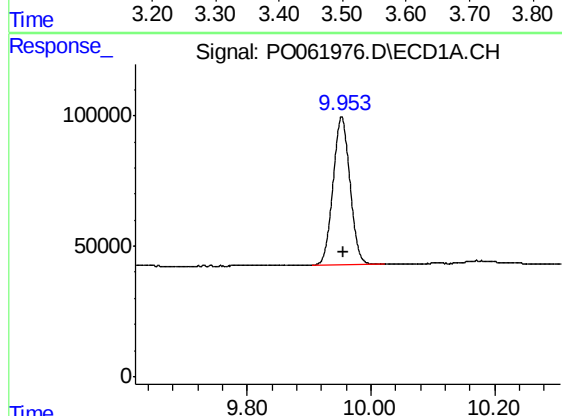

#2 Decachlorobiphenyl


R.T.: 9.953 min
Delta R.T.: -0.004 min
Response: 1068568
Conc: 19.10 ng/ml

10/15/2019 9:02:27 AM

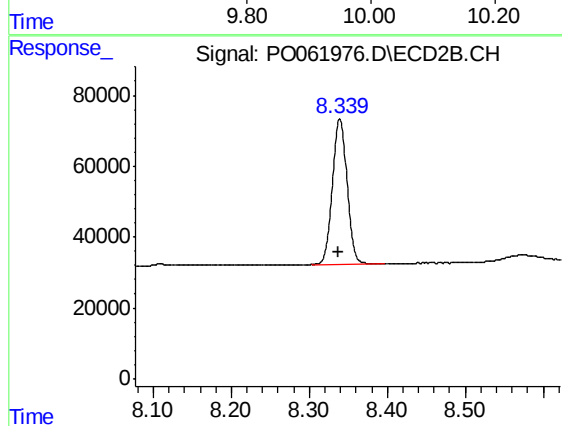

#2 Decachlorobiphenyl

R.T.: 8.339 min
Delta R.T.: 0.001 min
Response: 527938
Conc: 17.99 ng/ml

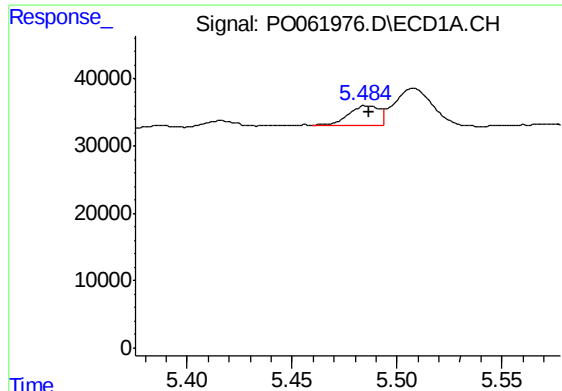


#21 AR-1248-1

R.T.: 5.484 min
Delta R.T.: -0.003 min
Response: 30082
Conc: 20.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VNJ-230


Manual Integrations
APPROVED

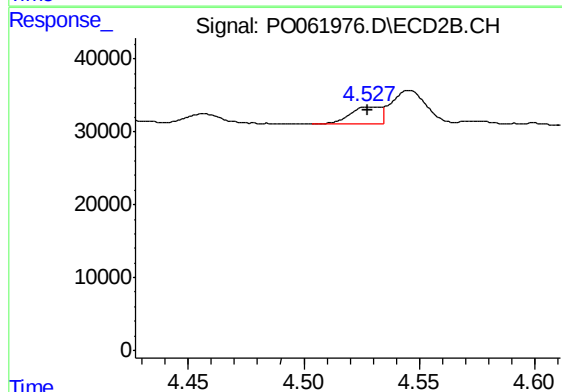

#21 AR-1248-1

R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 20787
Conc: 21.17 ng/ml m


Ankita

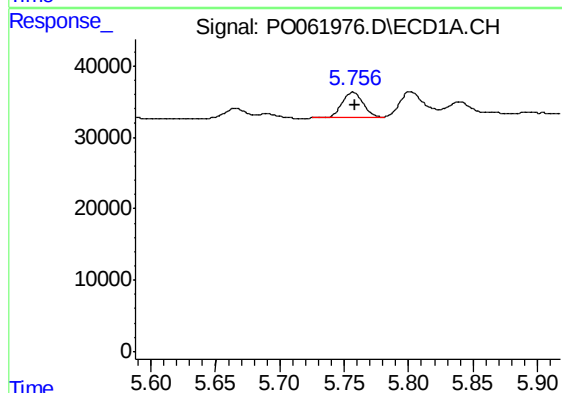

#22 AR-1248-2


R.T.: 5.757 min
Delta R.T.: -0.001 min
Response: 40430
Conc: 20.19 ng/ml

10/15/2019 9:02:27 AM

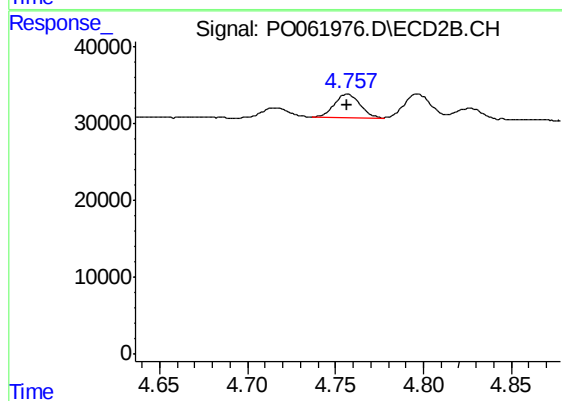

#22 AR-1248-2

R.T.: 4.757 min
Delta R.T.: 0.000 min
Response: 31048
Conc: 24.51 ng/ml

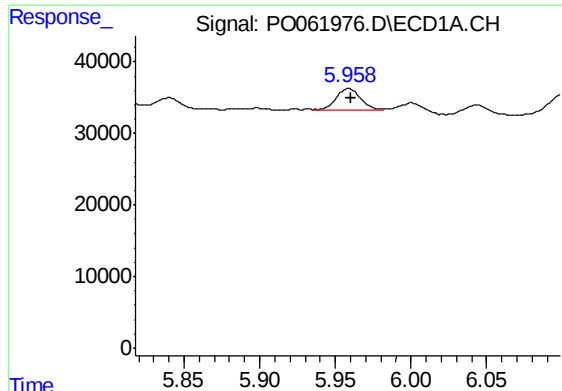


#23 AR-1248-3

R.T.: 5.958 min
Delta R.T.: -0.002 min
Response: 35835
Conc: 16.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VNJ-230


Manual Integrations
APPROVED

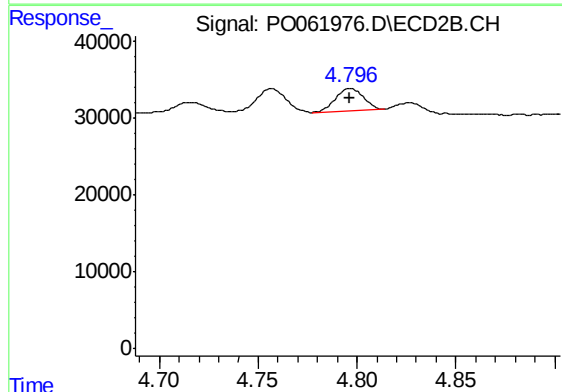

#23 AR-1248-3

R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 27719
Conc: 20.88 ng/ml


Ankita

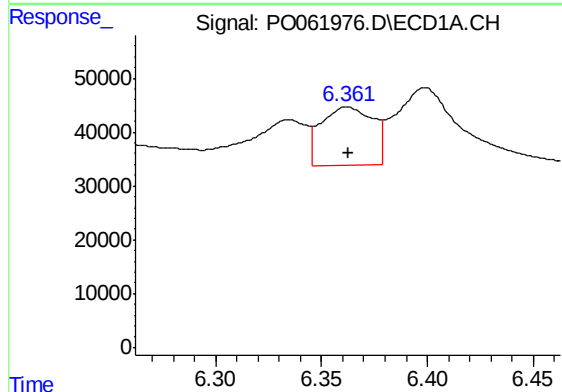

#24 AR-1248-4


R.T.: 6.362 min
Delta R.T.: 0.000 min
Response: 187228
Conc: 73.29 ng/ml

10/15/2019 9:02:27 AM

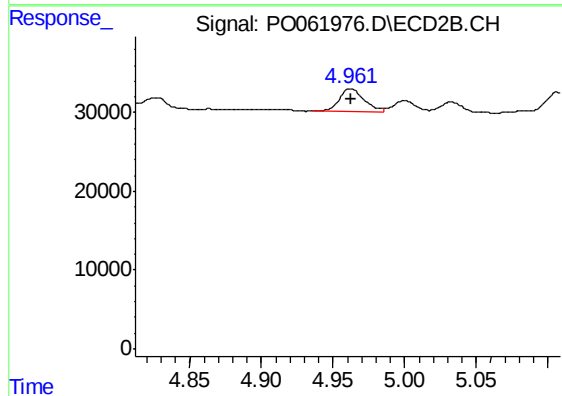

#24 AR-1248-4

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 34881
Conc: 22.04 ng/ml

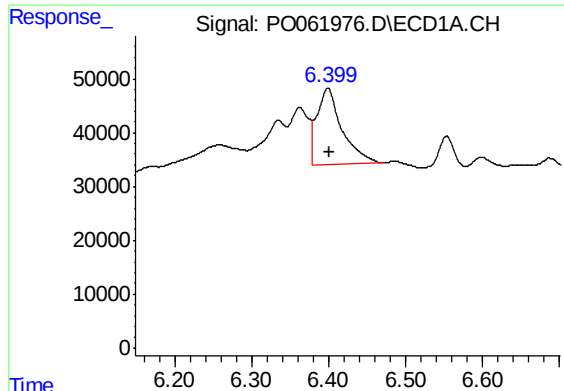


#25 AR-1248-5

R.T.: 6.399 min
Delta R.T.: -0.002 min
Response: 319451
Conc: 130.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-230

Manual Integrations
APPROVED

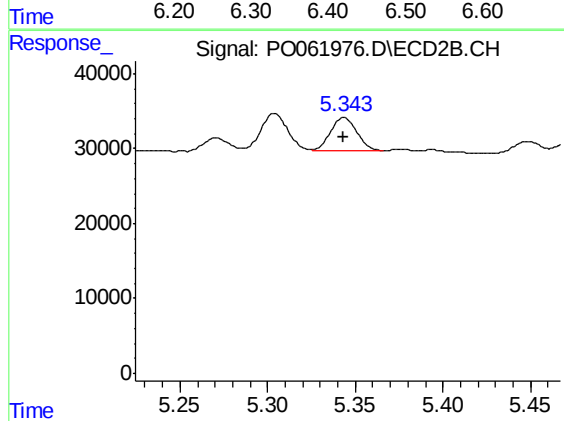

#25 AR-1248-5

R.T.: 5.343 min
Delta R.T.: 0.000 min
Response: 44972
Conc: 29.22 ng/ml

Ankita

10/15/2019 9:02:27 AM