

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
Data File : P0061984.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 00:32
Operator : HP/AJ
Sample : K5337-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HHT-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:11:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.484	1304636	892808	21.094	20.820
2)	SA Decachlor...	9.952	8.340	1135452	582924	20.293	19.867

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061984.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 00:32
Operator : HP/AJ
Sample : K5337-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HHT-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:11:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

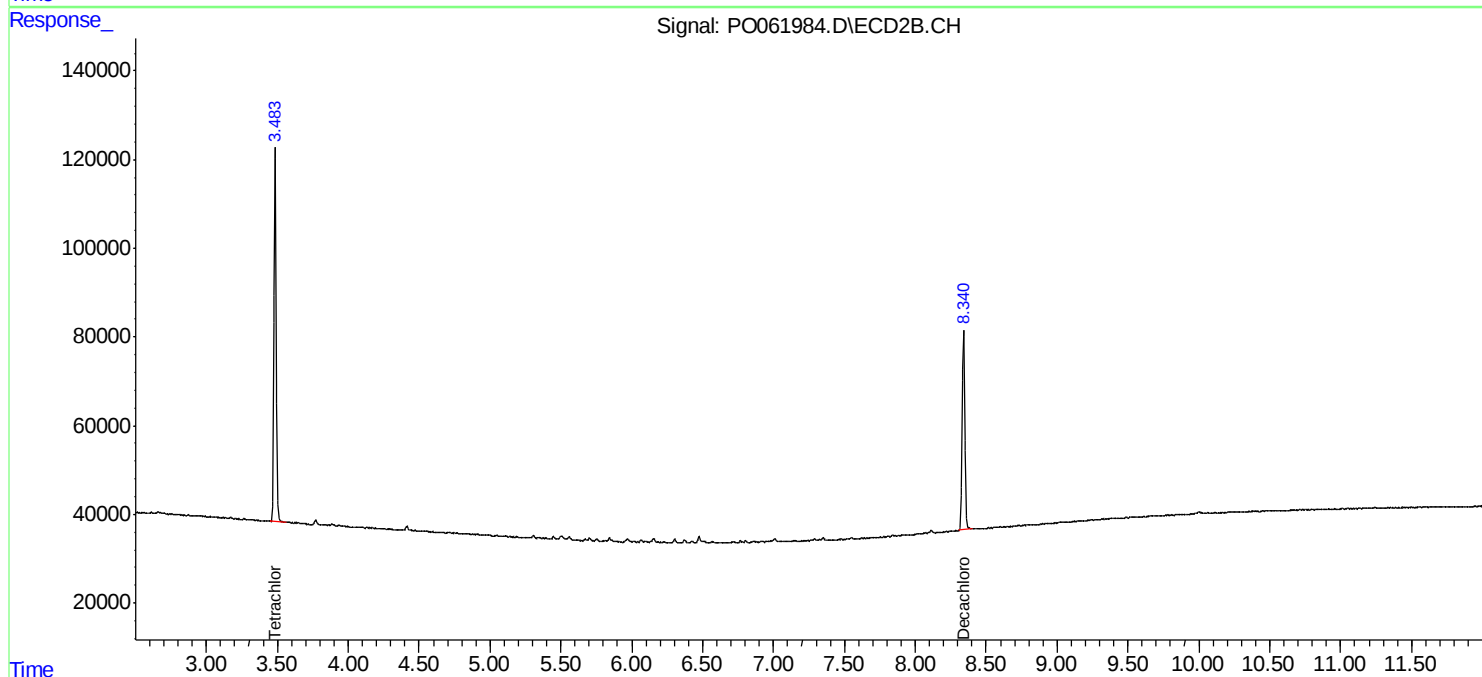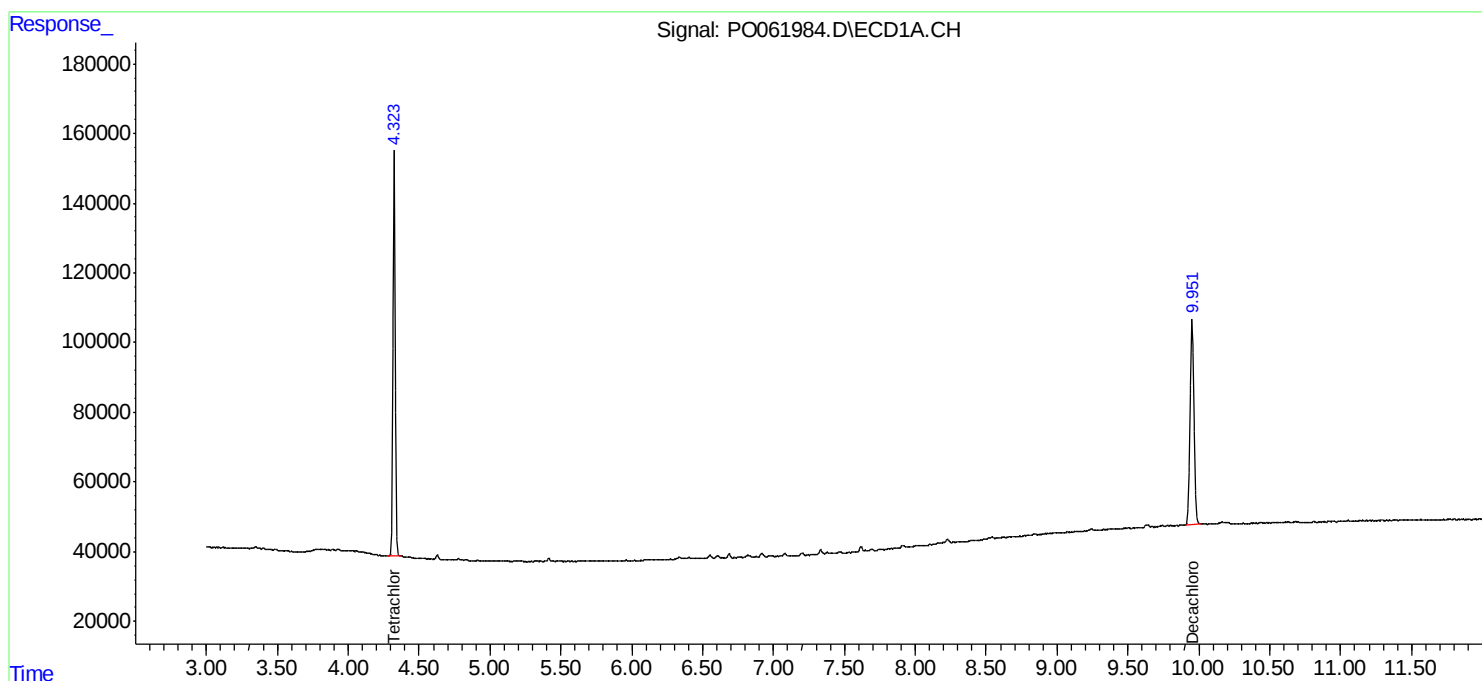


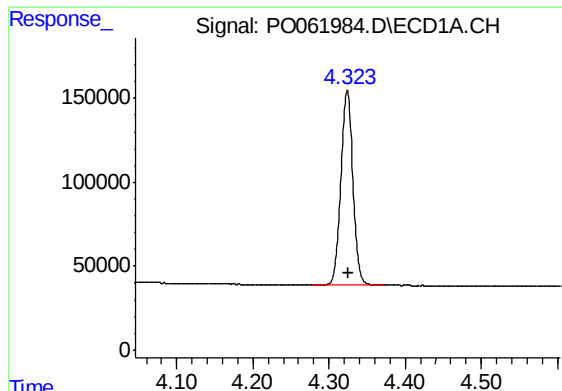

#1 Tetrachloro-m-xylene


R.T.: 4.324 min
Delta R.T.: -0.001 min
Response: 1304636
Conc: 21.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
HHT-WATER

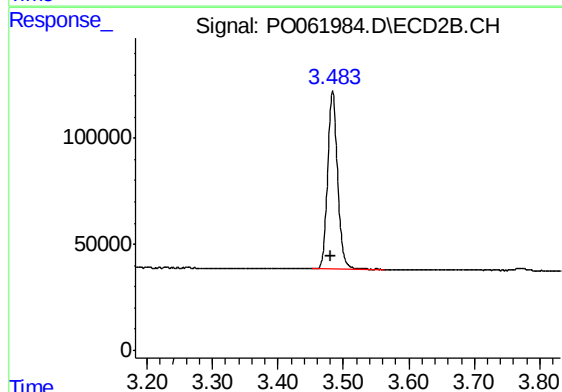


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.002 min
Response: 892808
Conc: 20.82 ng/ml

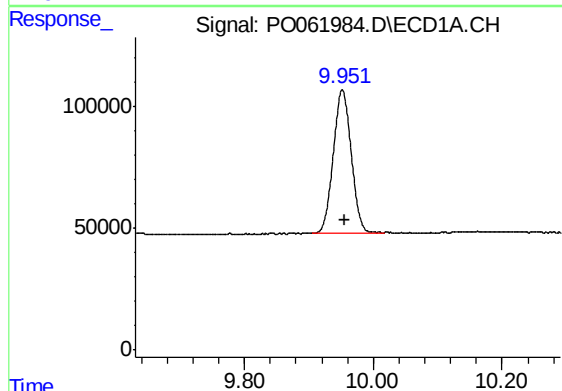

#2 Decachlorobiphenyl

R.T.: 9.952 min
Delta R.T.: -0.005 min
Response: 1135452
Conc: 20.29 ng/ml

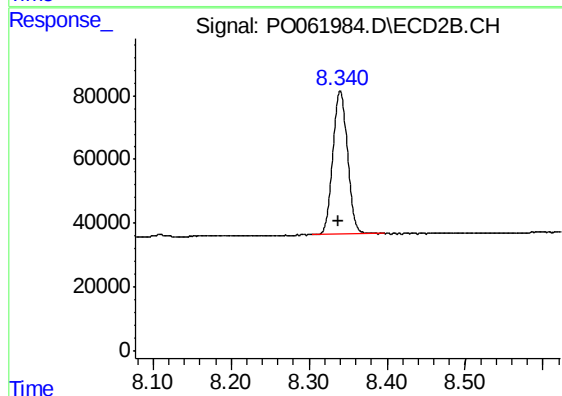

#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.002 min
Response: 582924
Conc: 19.87 ng/ml