

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
 Data File : P0061985.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2019 00:48
 Operator : HP/AJ
 Sample : K5352-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-20A-S

Manual Integrations
 APPROVED

Ankita
 10/15/2019 9:02:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:11:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.484	1266488	862094	20.478	20.104
2)	SA Decachlor...	9.951	8.339	959408	473459	17.147	16.136
Target Compounds							
26)	L6 AR-1254-1	6.333	5.304	32241	35225	12.095	14.402
27)	L6 AR-1254-2	6.550	5.448	57593	26856	14.087	12.681
28)	L6 AR-1254-3	6.915	5.839	86977	64085	20.788	19.669m
29)	L6 AR-1254-4	7.198	6.065	32648	19092	10.835m	9.885m
30)	L6 AR-1254-5	7.616	6.474	63575	69585	20.286	26.346 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 00:48
Operator : HP/AJ
Sample : K5352-07
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-20A-S


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:11:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

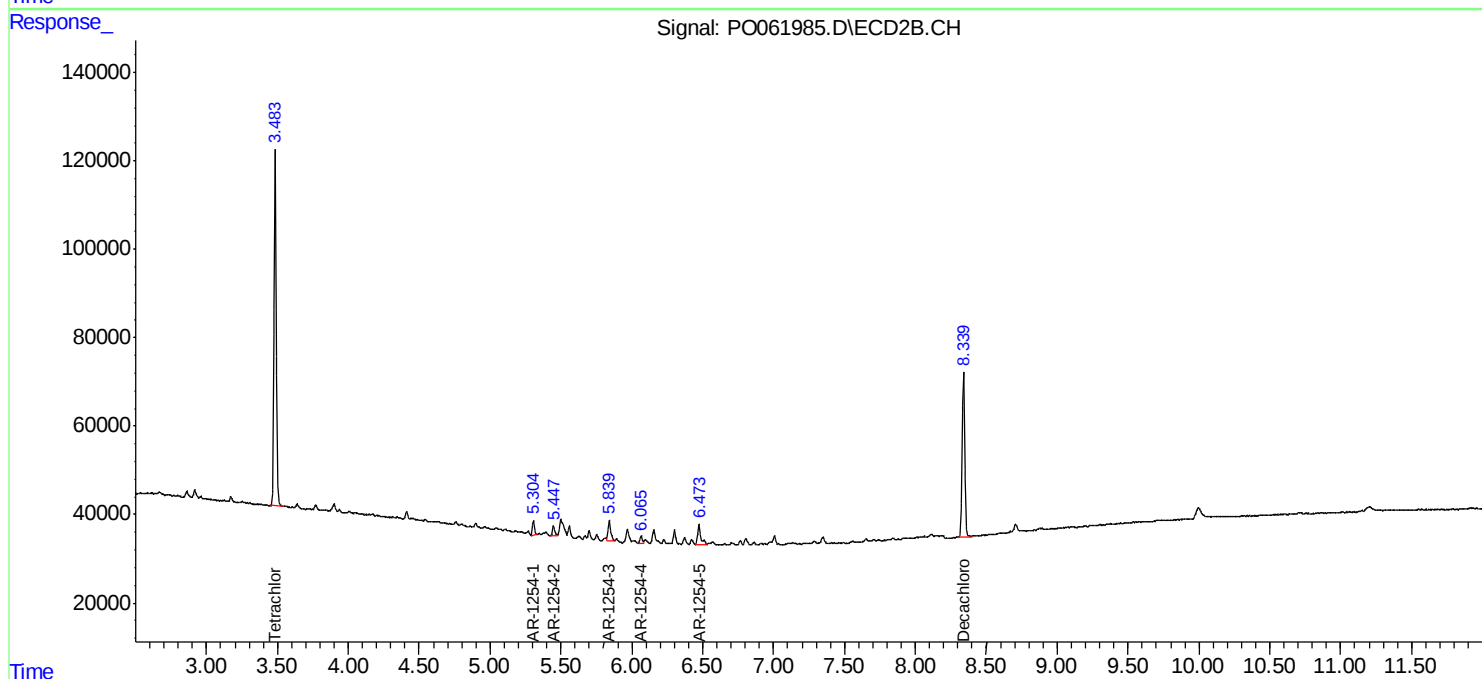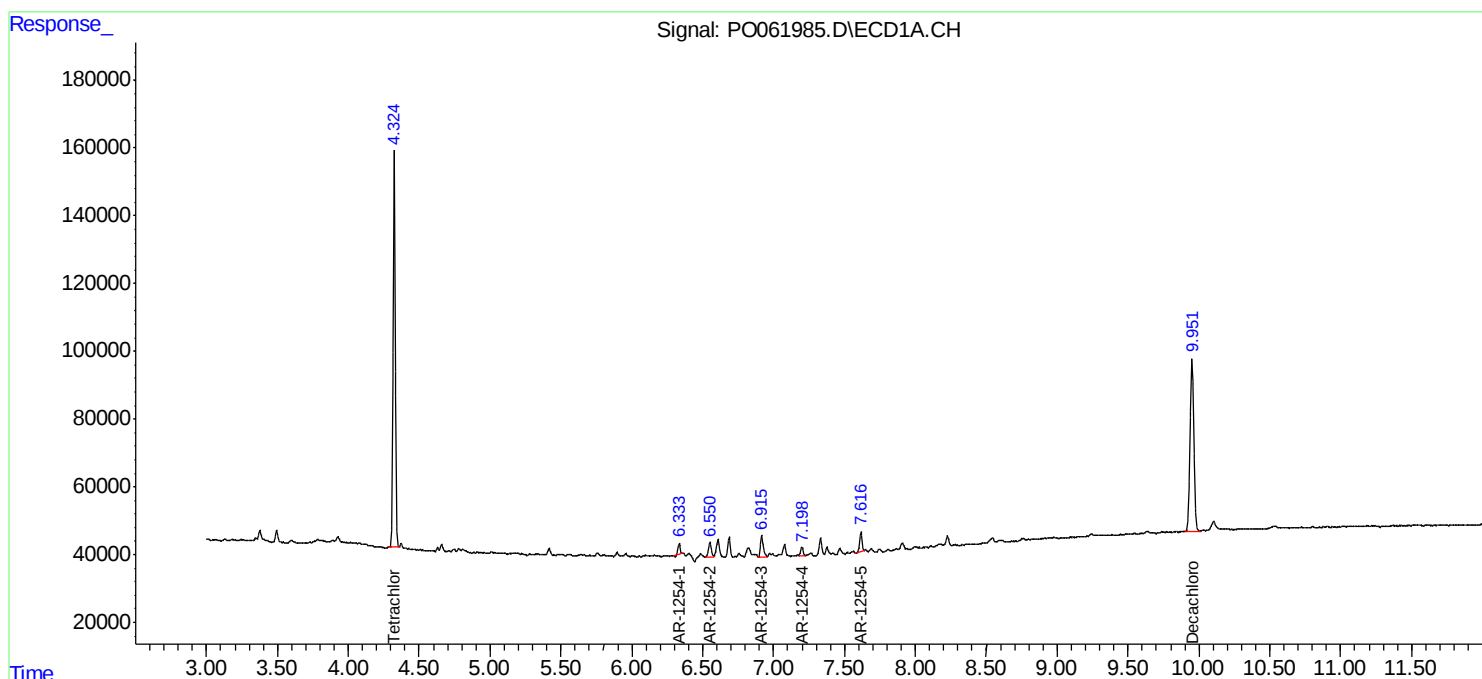

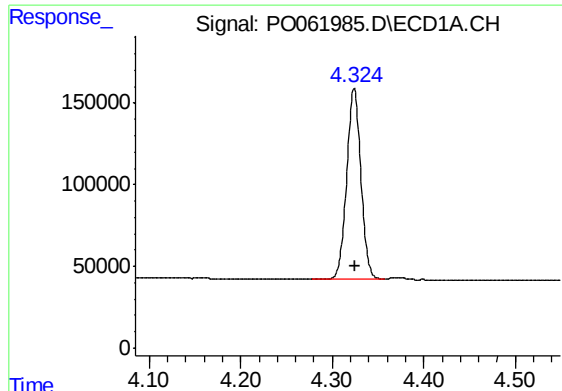


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.001 min
Response: 1266488
Conc: 20.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20A-S


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:39 AM

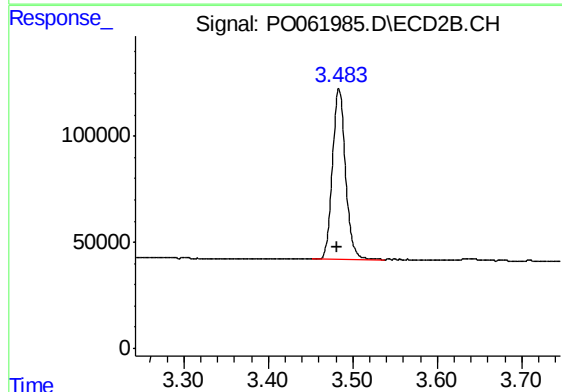


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.002 min
Response: 862094
Conc: 20.10 ng/ml

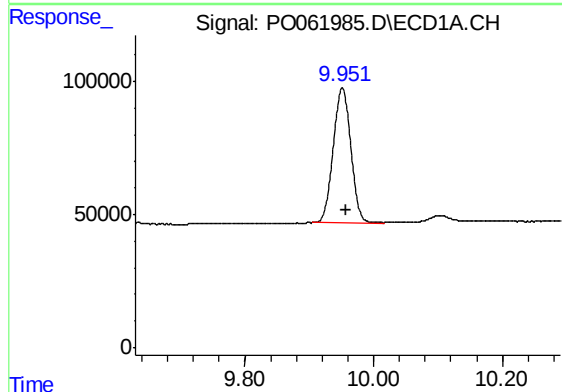


#2 Decachlorobiphenyl

R.T.: 9.951 min
Delta R.T.: -0.005 min
Response: 959408
Conc: 17.15 ng/ml

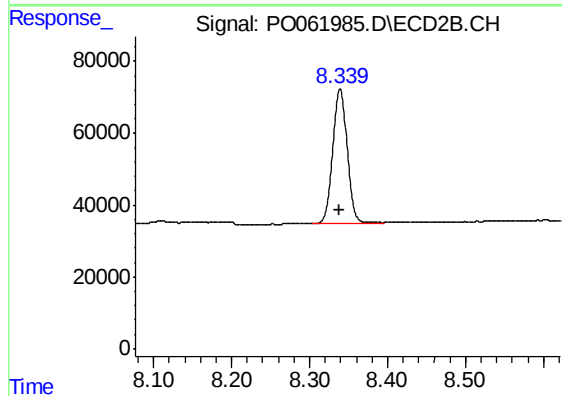

#2 Decachlorobiphenyl

R.T.: 8.339 min
Delta R.T.: 0.001 min
Response: 473459
Conc: 16.14 ng/ml

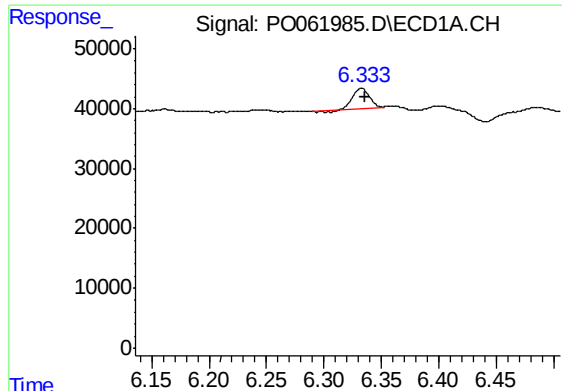


#26 AR-1254-1

R.T.: 6.333 min
Delta R.T.: -0.003 min
Response: 32241
Conc: 12.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20A-S


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:39 AM

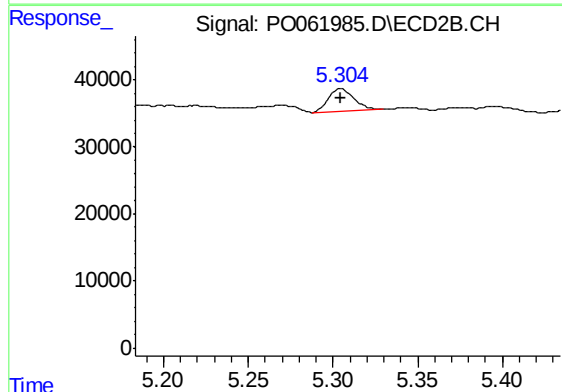


#26 AR-1254-1

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 35225
Conc: 14.40 ng/ml

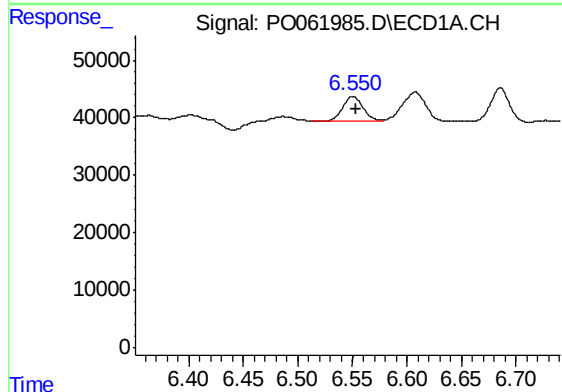


#27 AR-1254-2

R.T.: 6.550 min
Delta R.T.: -0.003 min
Response: 57593
Conc: 14.09 ng/ml

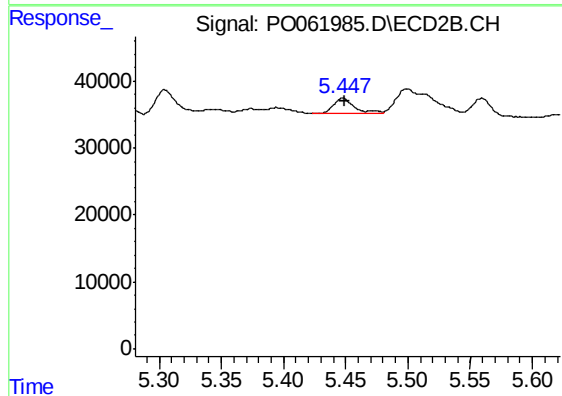

#27 AR-1254-2

R.T.: 5.448 min
Delta R.T.: -0.001 min
Response: 26856
Conc: 12.68 ng/ml

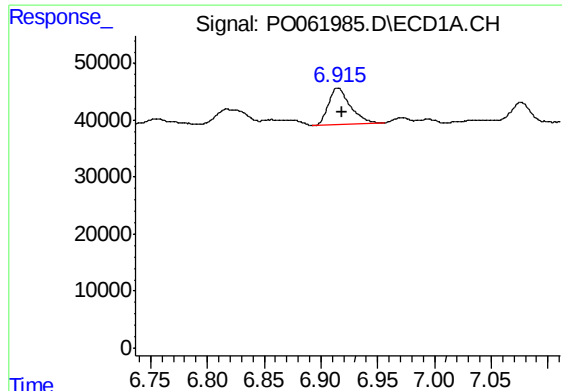


#28 AR-1254-3

R.T.: 6.915 min
Delta R.T.: -0.003 min
Response: 86977
Conc: 20.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20A-S


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:39 AM

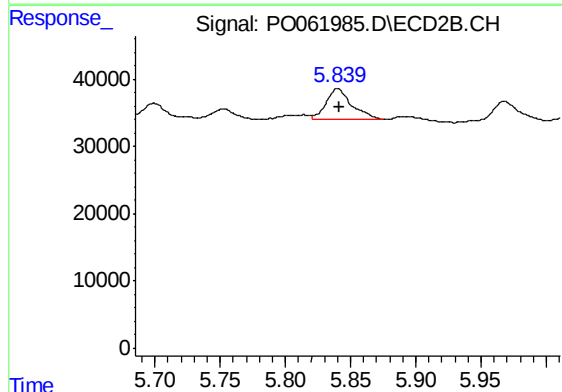


#28 AR-1254-3

R.T.: 5.839 min
Delta R.T.: -0.003 min
Response: 64085
Conc: 19.67 ng/ml m

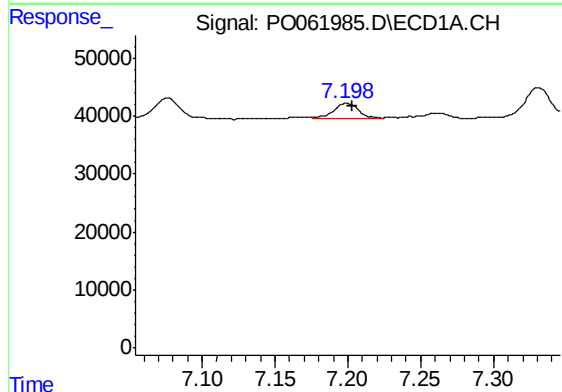


#29 AR-1254-4

R.T.: 7.198 min
Delta R.T.: -0.005 min
Response: 32648
Conc: 10.83 ng/ml m

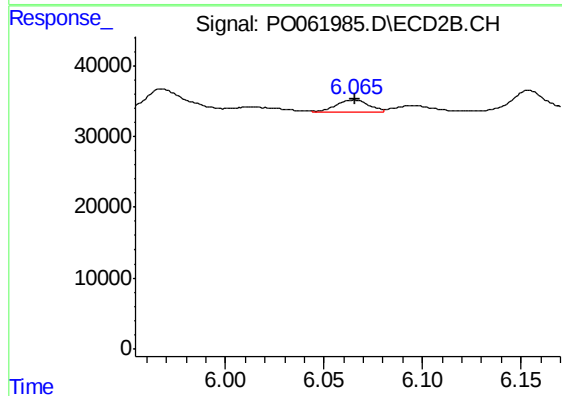

#29 AR-1254-4

R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 19092
Conc: 9.89 ng/ml m

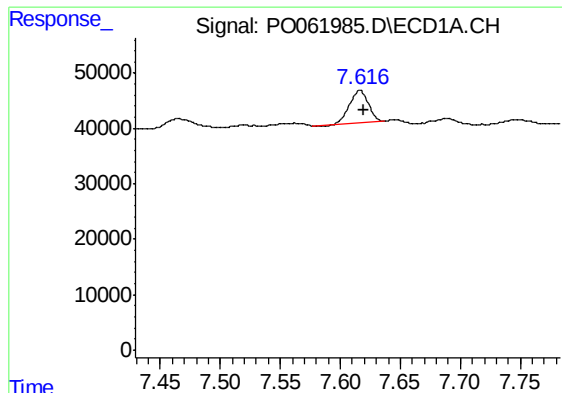


#30 AR-1254-5

R.T.: 7.616 min
Delta R.T.: -0.004 min
Response: 63575
Conc: 20.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20A-S

Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:39 AM

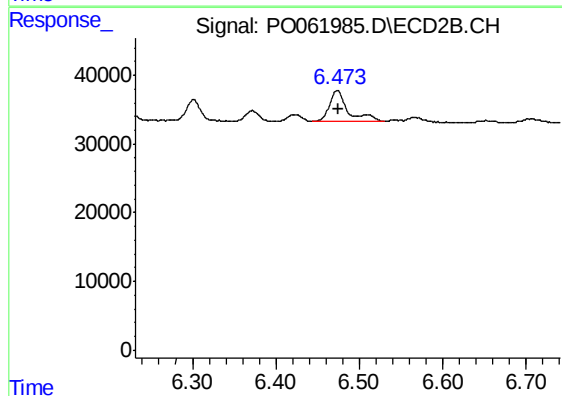

#30 AR-1254-5

R.T.: 6.474 min
Delta R.T.: -0.002 min
Response: 69585
Conc: 26.35 ng/ml