

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101419\
 Data File : P0061989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2019 1:54
 Operator : HP/AJ
 Sample : K5334-02
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-2-PIT-COMPOSITE

Manual Integrations
 APPROVED

Ankita
 10/15/2019 9:02:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 07:07:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.329	3.477	993595	3067050	16.065	71.524m#
2)	SA Decachlor...	9.974	8.350	504802	460693	9.022	15.701m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101419\
Data File : PO061989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 1:54
Operator : HP/AJ
Sample : K5334-02
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S-2-PIT-COMPOSITE


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 07:07:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

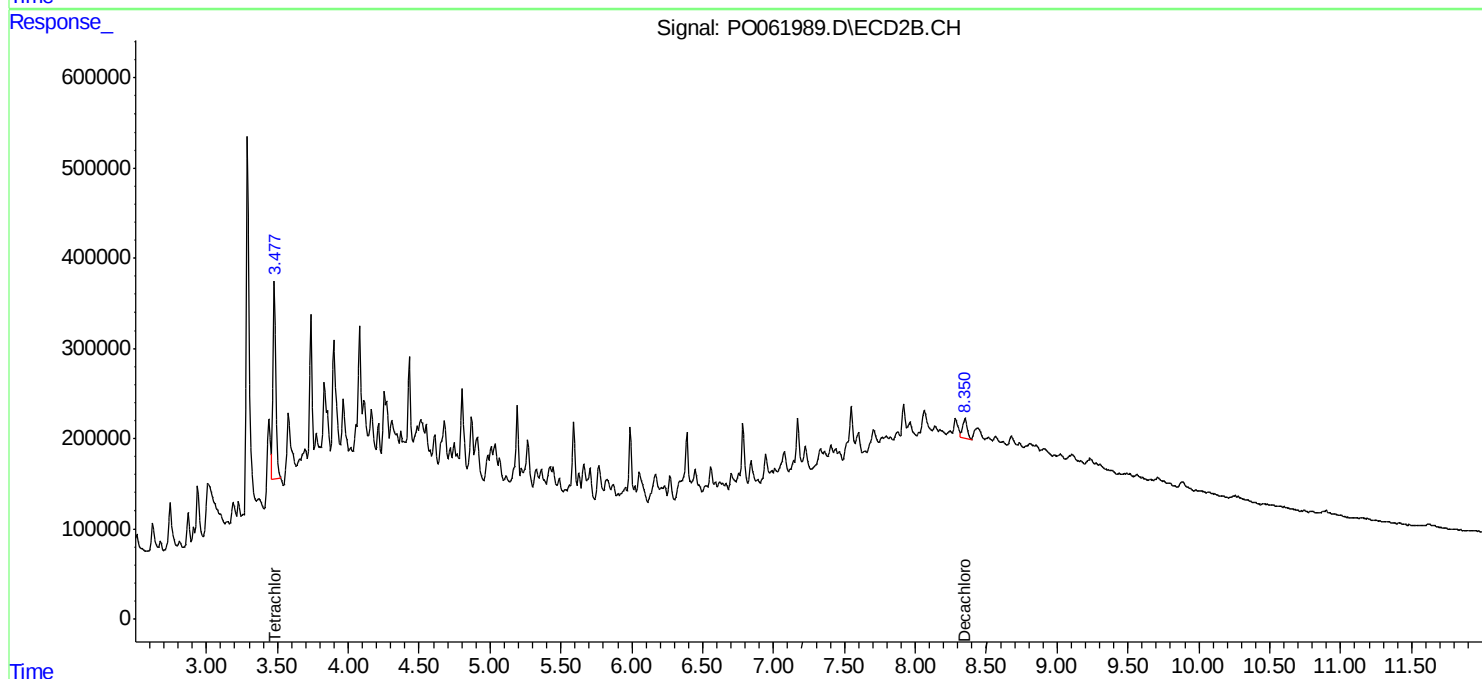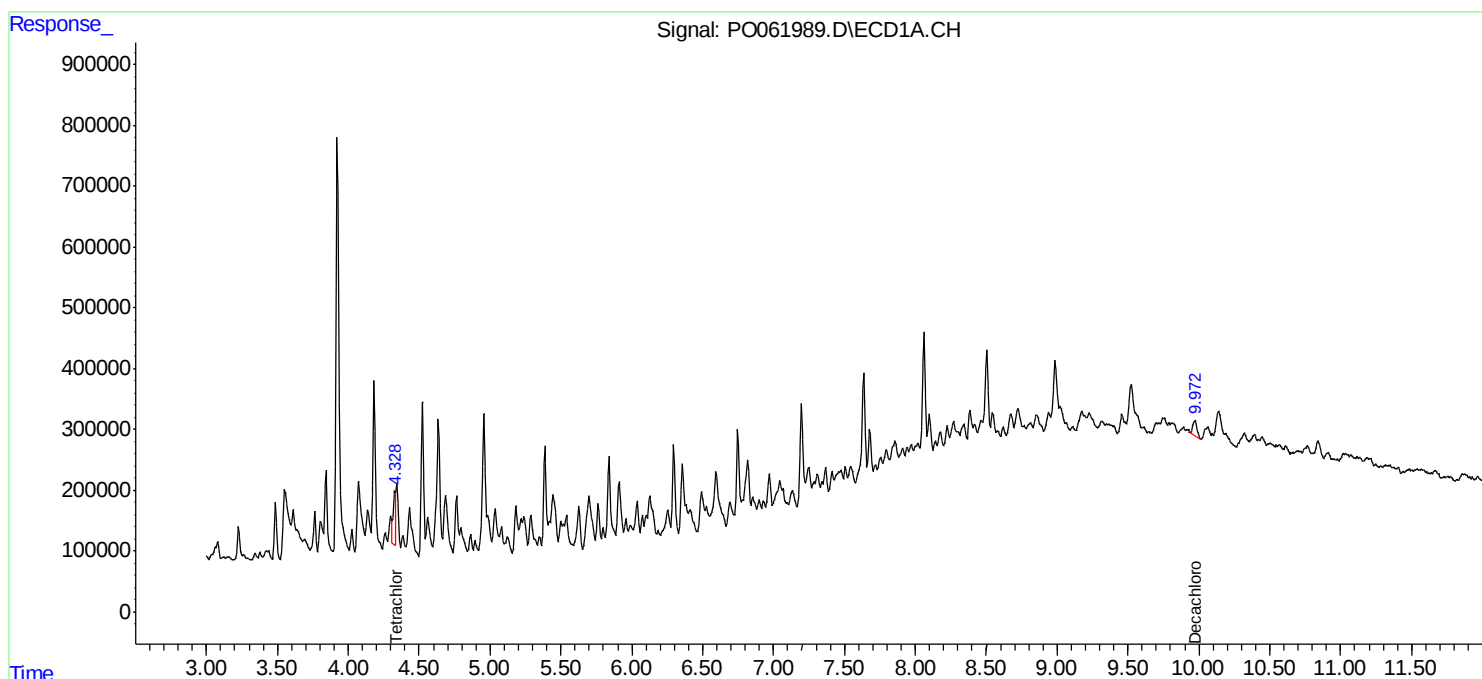

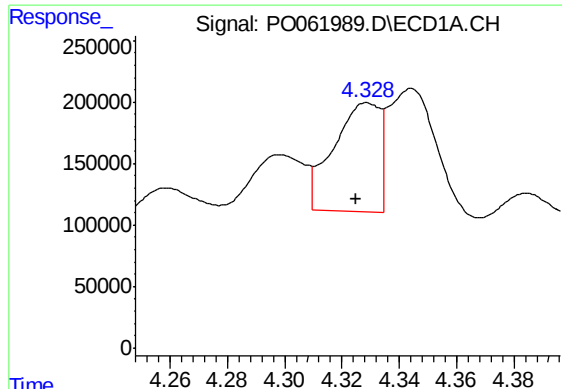


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: 0.004 min
Response: 993595
Conc: 16.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-2-PIT-COMPOSITE


Manual Integrations
APPROVED

Ankita
10/15/2019 9:02:41 AM

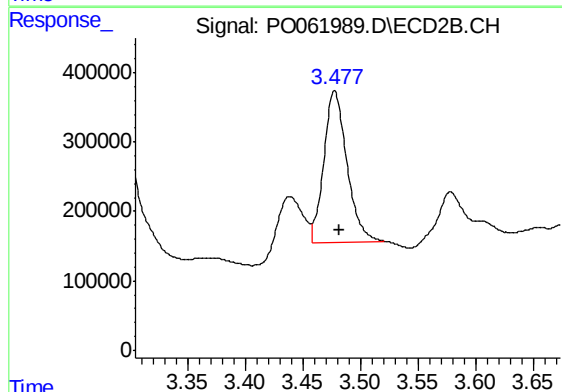


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.004 min
Response: 3067050
Conc: 71.52 ng/ml m

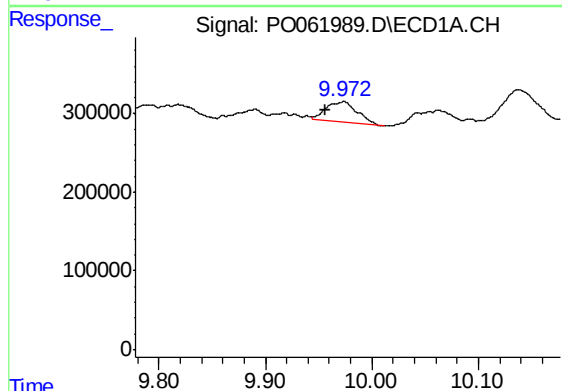

#2 Decachlorobiphenyl

R.T.: 9.974 min
Delta R.T.: 0.017 min
Response: 504802
Conc: 9.02 ng/ml

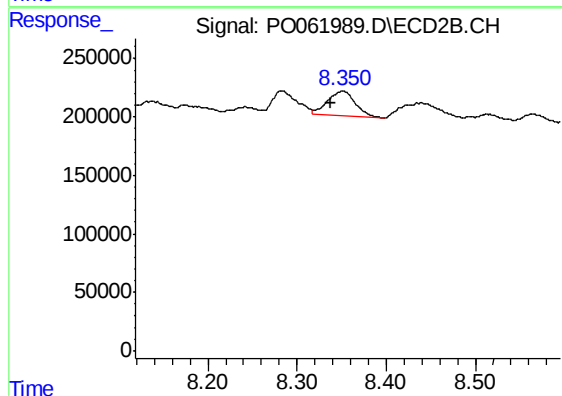

#2 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: 0.012 min
Response: 460693
Conc: 15.70 ng/ml m