

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
 Data File : PO050025.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2018 15:59
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 16:15:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 15:23:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.364	5334811	4025448	21.656	20.546
2) SA Decachlor...	10.068	8.126	-440609	3576184	N.D.	20.796

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050025.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2018 15:59
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 16:15:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 15:23:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

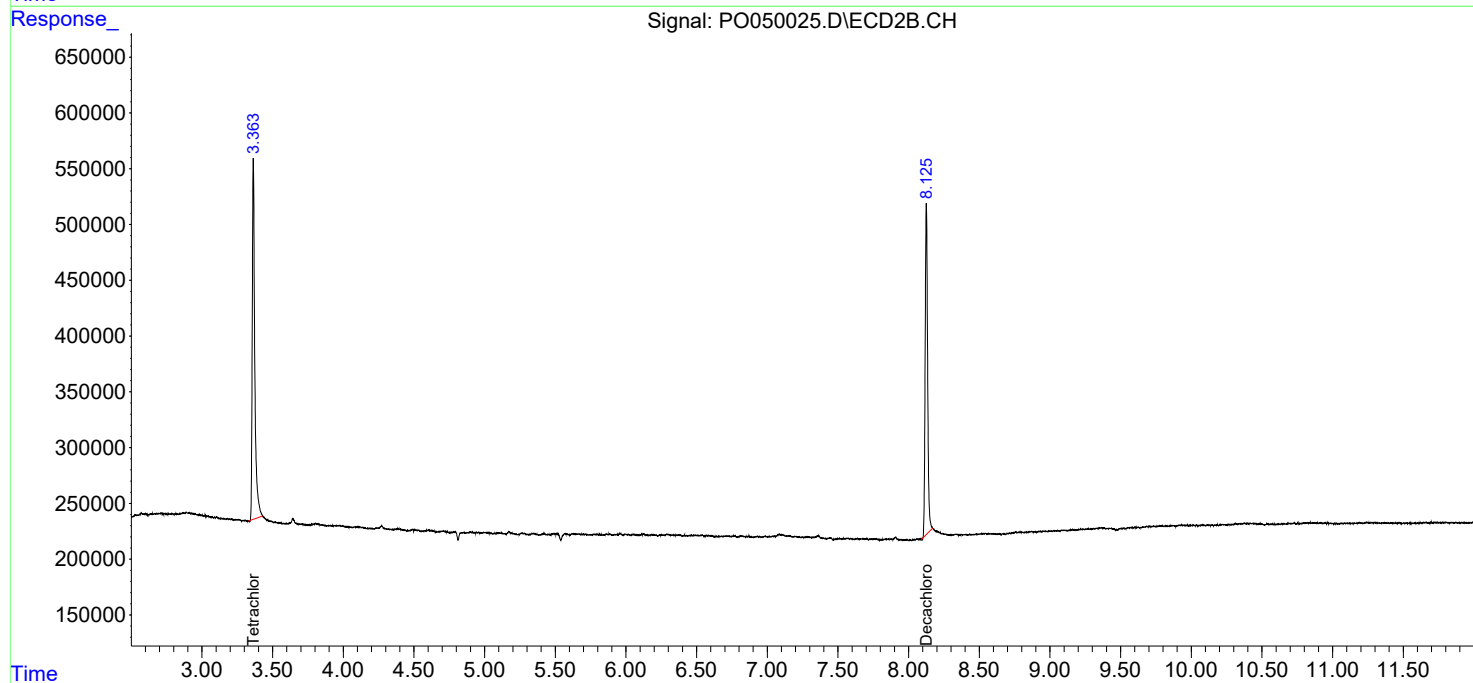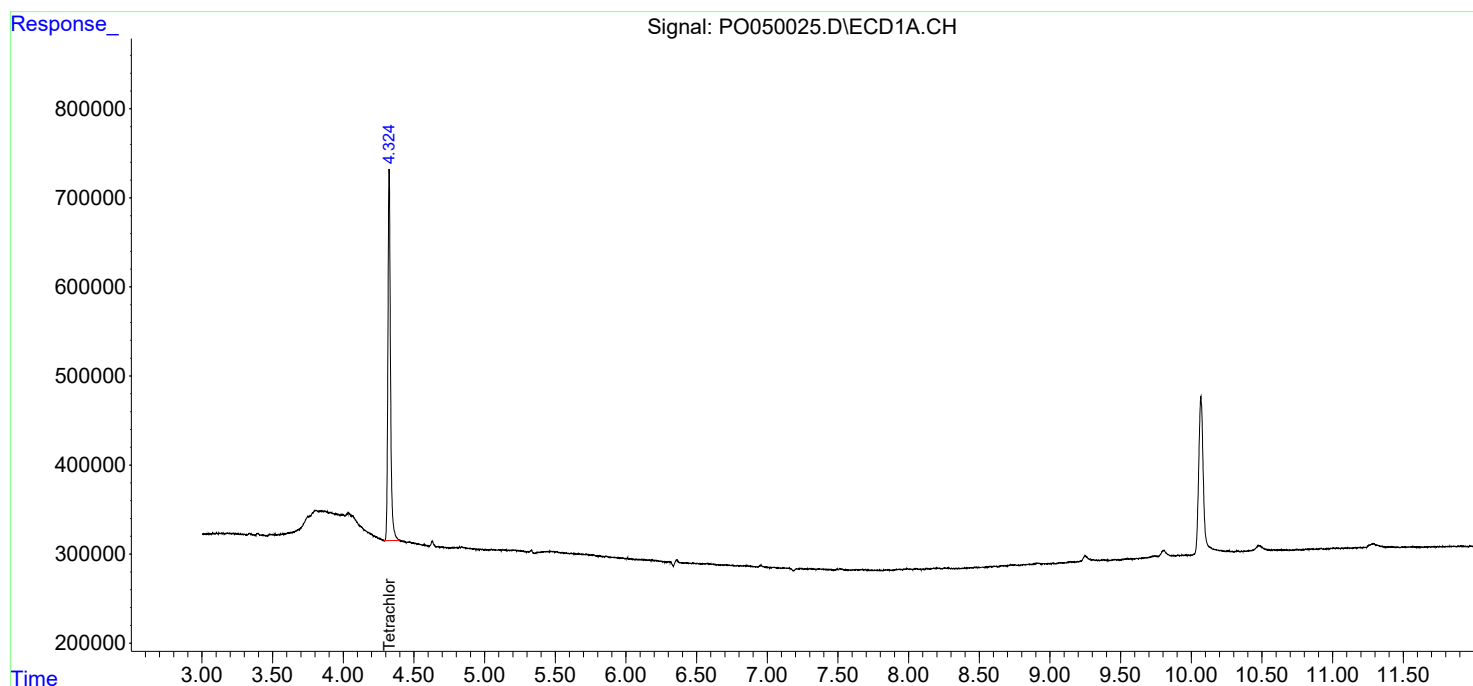


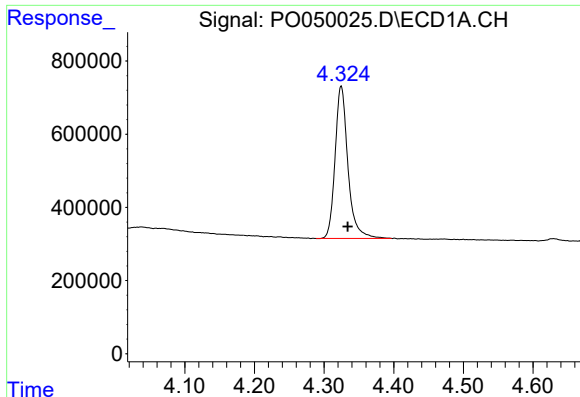

#1 Tetrachloro-m-xylene


R.T.: 4.325 min
Delta R.T.: -0.009 min
Response: 5334811
Conc: 21.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

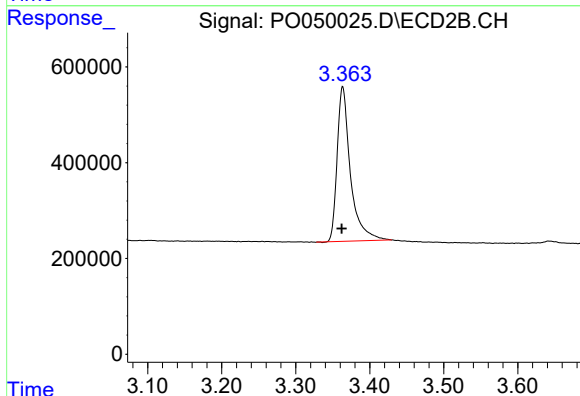


#1 Tetrachloro-m-xylene

R.T.: 3.364 min
Delta R.T.: 0.001 min
Response: 4025448
Conc: 20.55 ng/ml

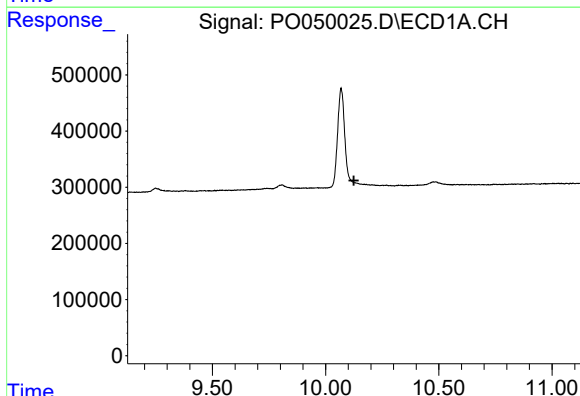

#2 Decachlorobiphenyl

R.T.: 10.068 min
Delta R.T.: -0.057 min
Response: -440609
Conc: N.D.

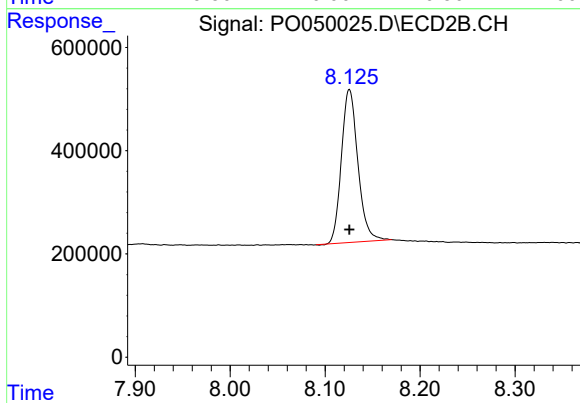

#2 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 3576184
Conc: 20.80 ng/ml