

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
 Data File : PO050056.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2018 3:29
 Operator : SM/SJ
 Sample : J5456-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-FRAC-TANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 10:08:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.366	4837551	3713411	19.637	18.953
2) SA Decachlor...	0.000	8.128	0	2625827	N.D.	15.270 #
Target Compounds						
10) L2 AR-1221-3	0.000	3.768	0	363967	N.D.	73.617 #
11) L3 AR-1232-1	0.000	3.768	0	363967	N.D.	101.978 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : P0050056.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2018 3:29
Operator : SM/SJ
Sample : J5456-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-FRAC-TANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 10:08:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

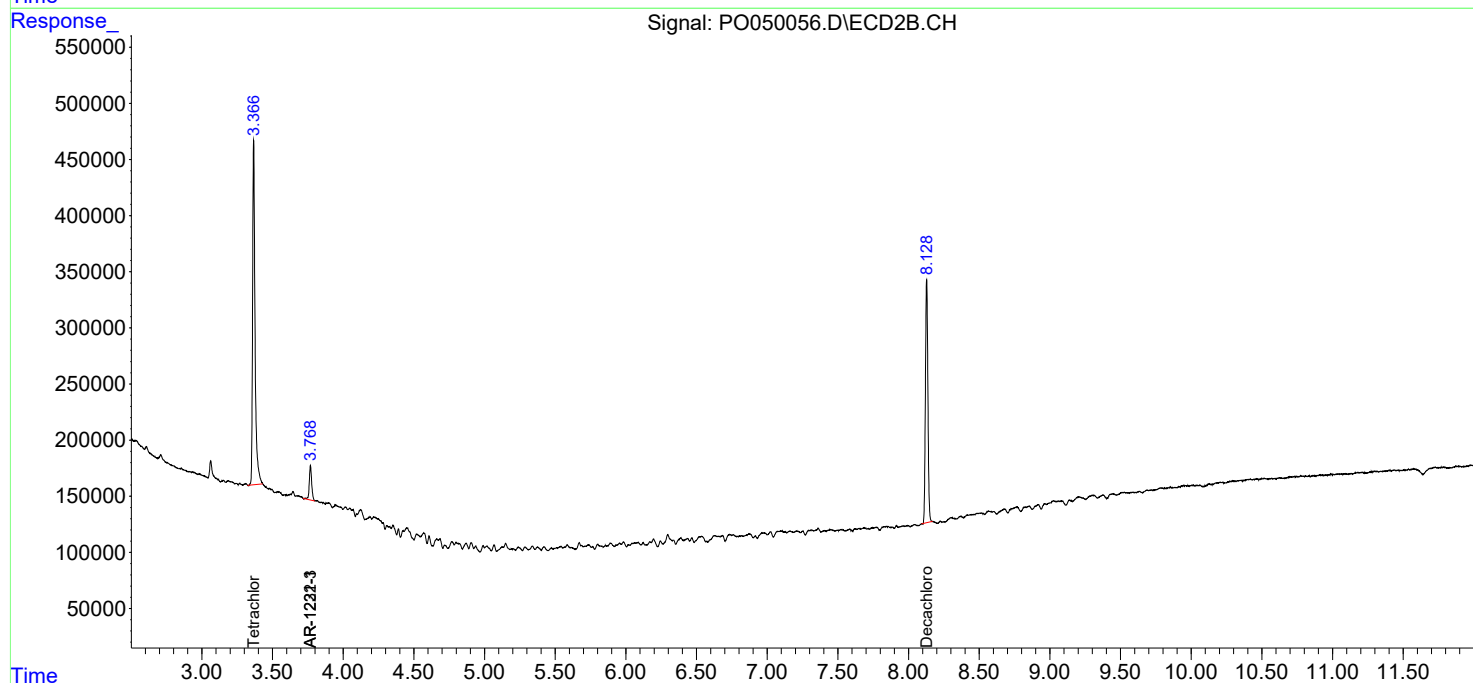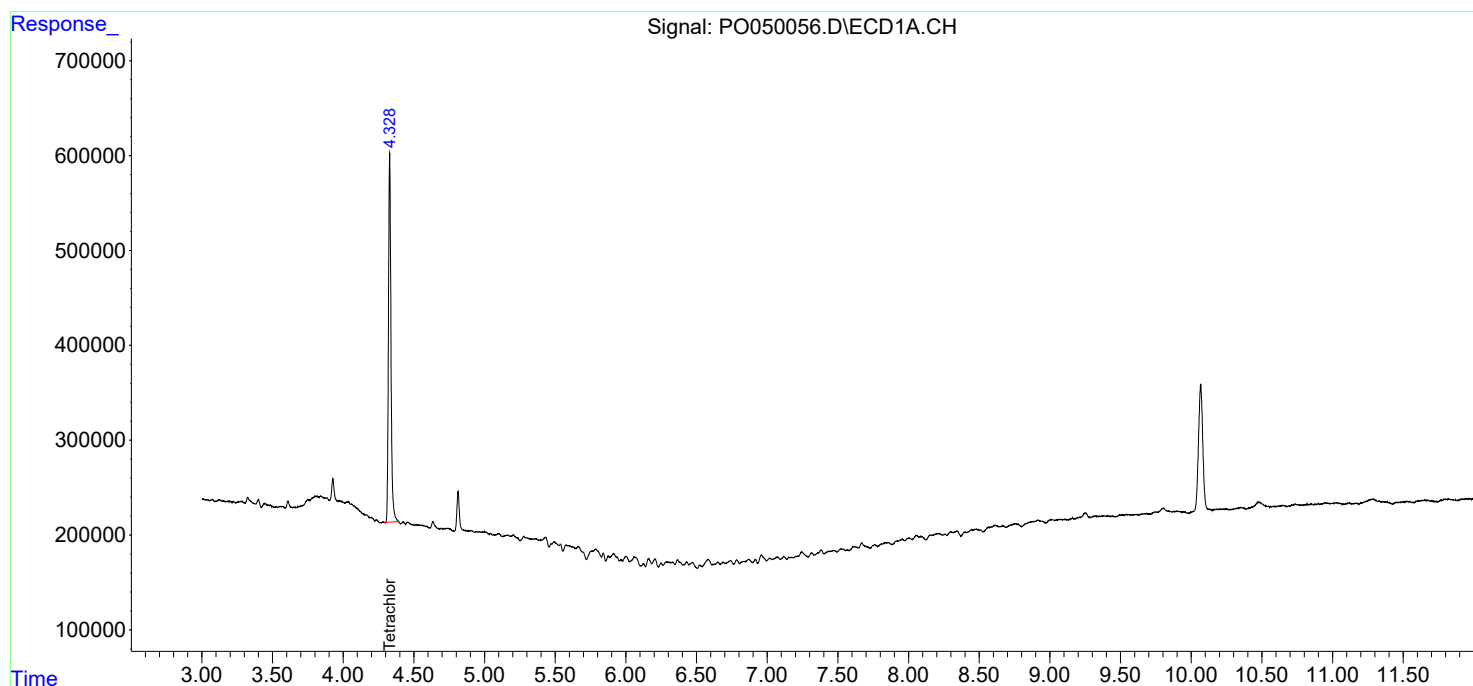


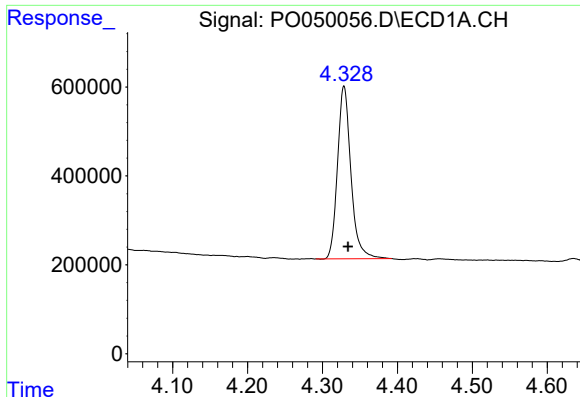

#1 Tetrachloro-m-xylene


R.T.: 4.329 min
Delta R.T.: -0.005 min
Response: 4837551
Conc: 19.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-FRAC-TANK

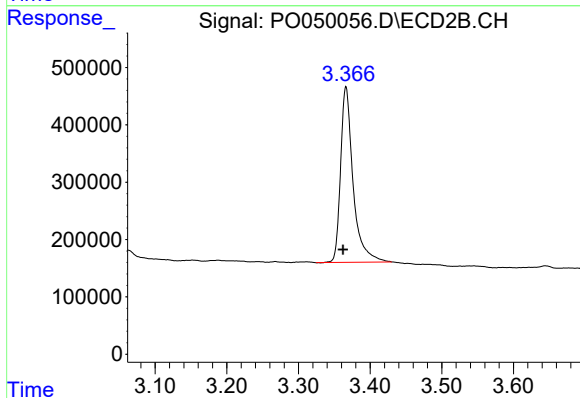


#1 Tetrachloro-m-xylene

R.T.: 3.366 min
Delta R.T.: 0.004 min
Response: 3713411
Conc: 18.95 ng/ml

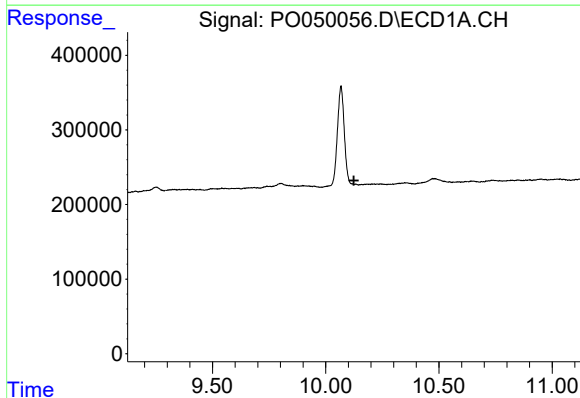


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.125 min
Response: 0
Conc: N.D.

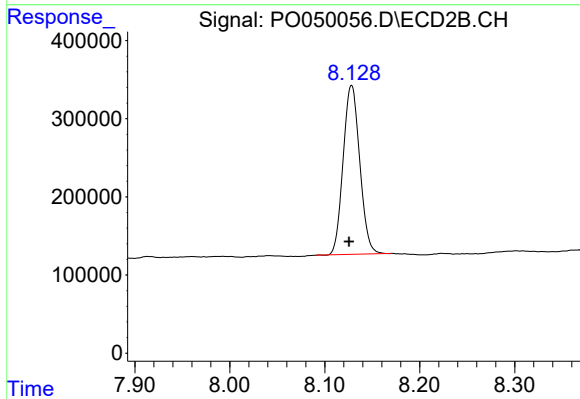

#2 Decachlorobiphenyl


R.T.: 8.128 min
Delta R.T.: 0.003 min
Response: 2625827
Conc: 15.27 ng/ml

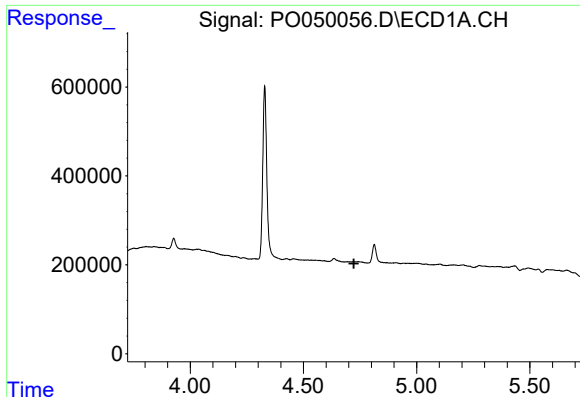

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MS-FRAC-TANK

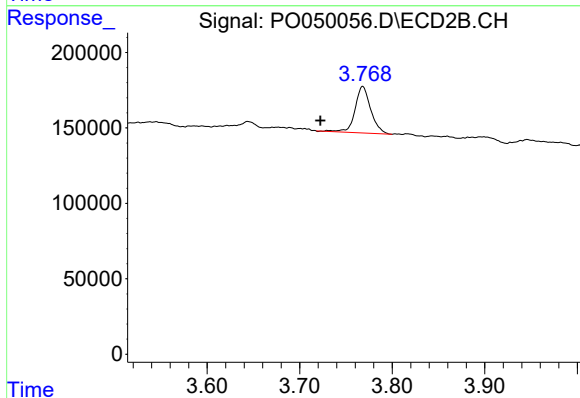


#10 AR-1221-3

R.T.: 3.768 min
Delta R.T.: 0.046 min
Response: 363967
Conc: 73.62 ng/ml

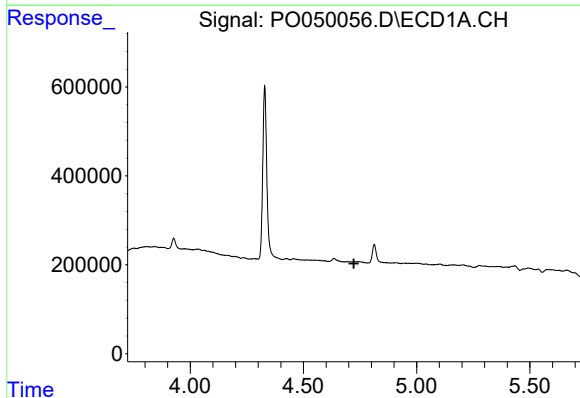

#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

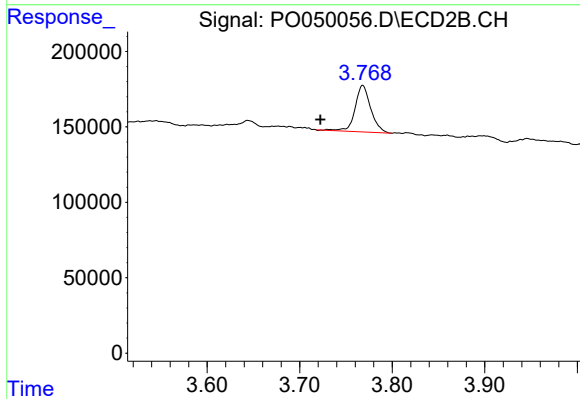

#11 AR-1232-1

R.T.: 3.768 min
Delta R.T.: 0.046 min
Response: 363967
Conc: 101.98 ng/ml