

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101518\
 Data File : P0050070.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2018 7:54
 Operator : SM/SJ
 Sample : J5509-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-CON

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 10:24:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.363	6095610	4848311	24.744	24.746
2) SA Decachlor...	10.068	8.124	11369	3641229	0.060	21.174 #
Target Compounds						
31) L7 AR-1260-1	0.000	5.795	0	285858	N.D.	19.895 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050070.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2018 7:54
Operator : SM/SJ
Sample : J5509-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 10:24:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

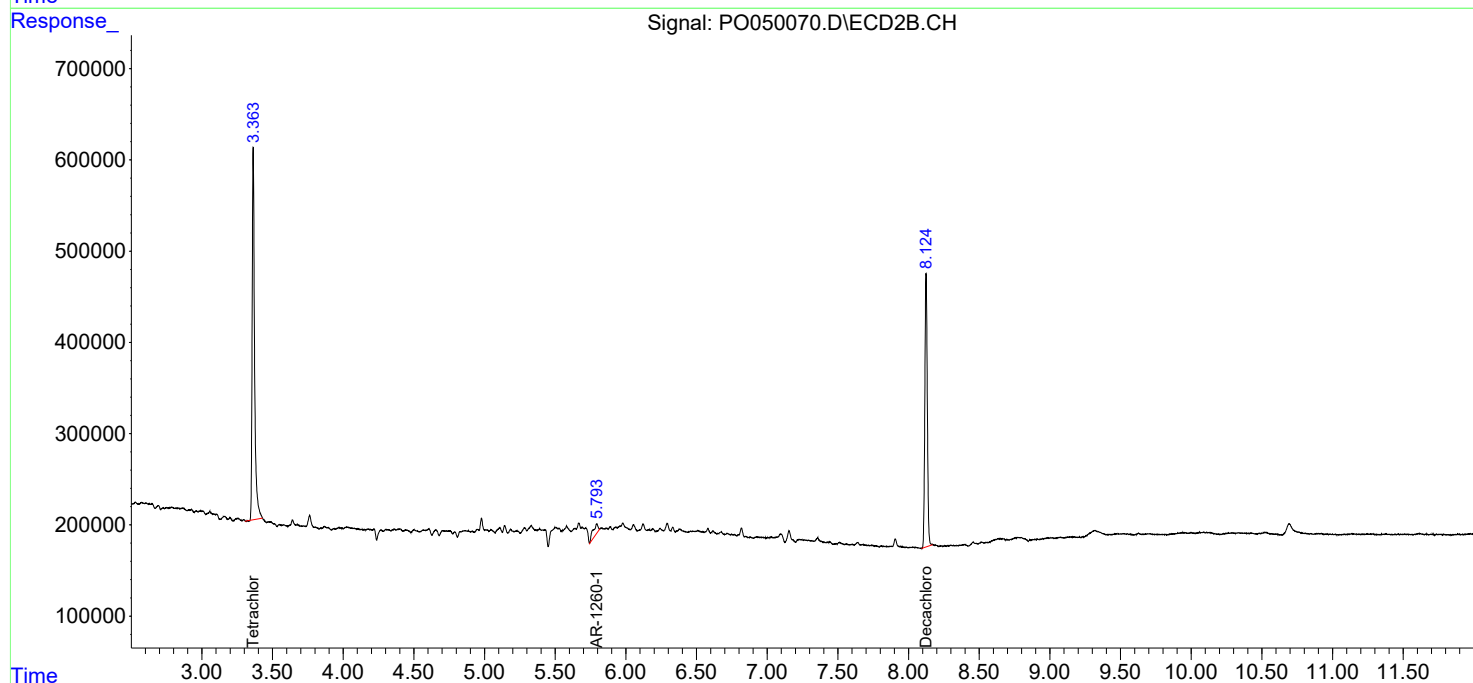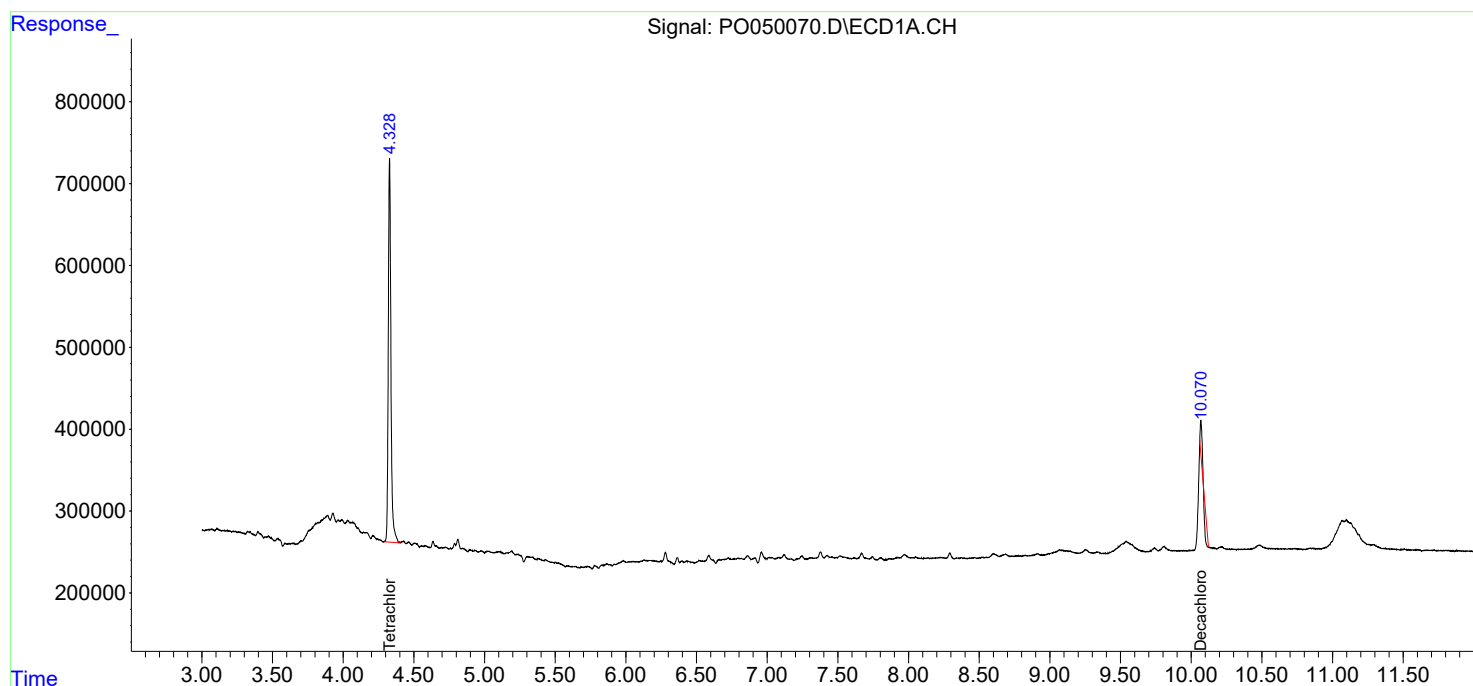


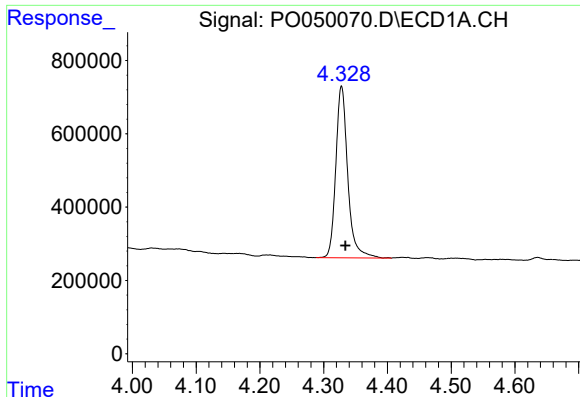

#1 Tetrachloro-m-xylene


R.T.: 4.328 min
Delta R.T.: -0.006 min
Response: 6095610
Conc: 24.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-CON

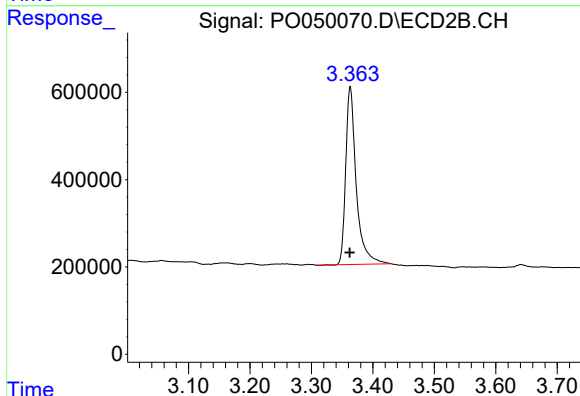


#1 Tetrachloro-m-xylene

R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 4848311
Conc: 24.75 ng/ml

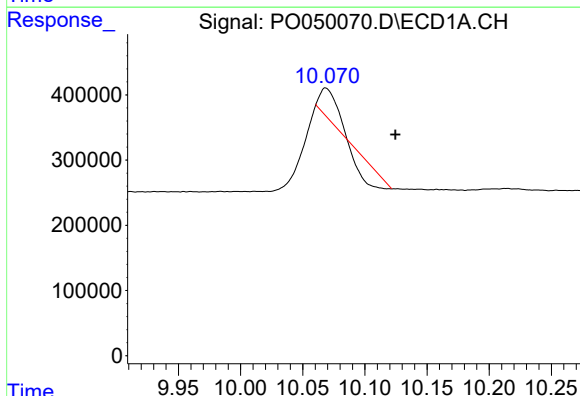


#2 Decachlorobiphenyl

R.T.: 10.068 min
Delta R.T.: -0.056 min
Response: 11369
Conc: 0.06 ng/ml

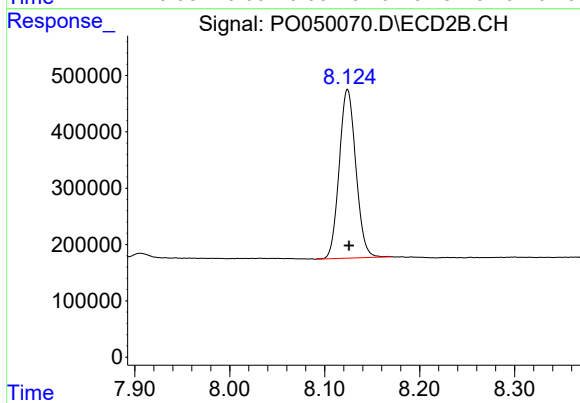

#2 Decachlorobiphenyl


R.T.: 8.124 min
Delta R.T.: -0.001 min
Response: 3641229
Conc: 21.17 ng/ml

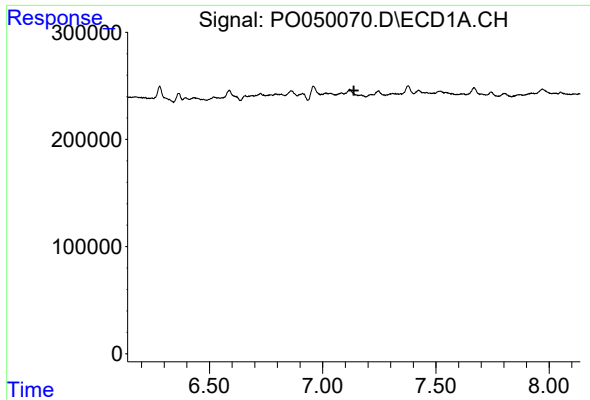

#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 7.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MS-CON

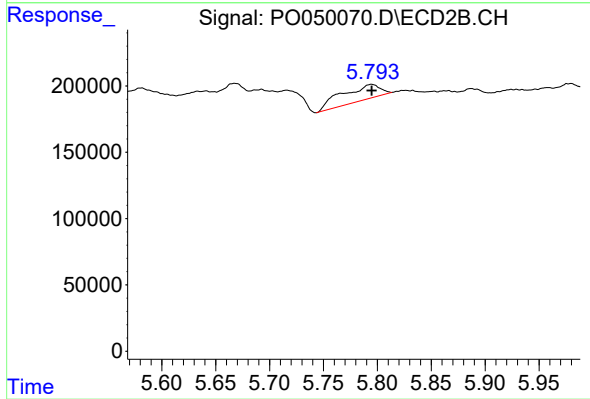

#31 AR-1260-1

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 285858
Conc: 19.90 ng/ml