

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101518\
 Data File : P0050027.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2018 16:37
 Operator : SM/SJ
 Sample : J5508-01 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A365210

Manual Integrations
 APPROVED

Sohil
 10/16/2018 2:45:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 18:00:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.323	3.364	994171	318064	4.036m	1.623m#
2) SA Decachlor...	10.070	8.128	415472	388123	2.207m	2.257m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050027.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2018 16:37
Operator : SM/SJ
Sample : J5508-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A365210


Manual Integrations
APPROVED

Sohil
10/16/2018 2:45:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 18:00:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

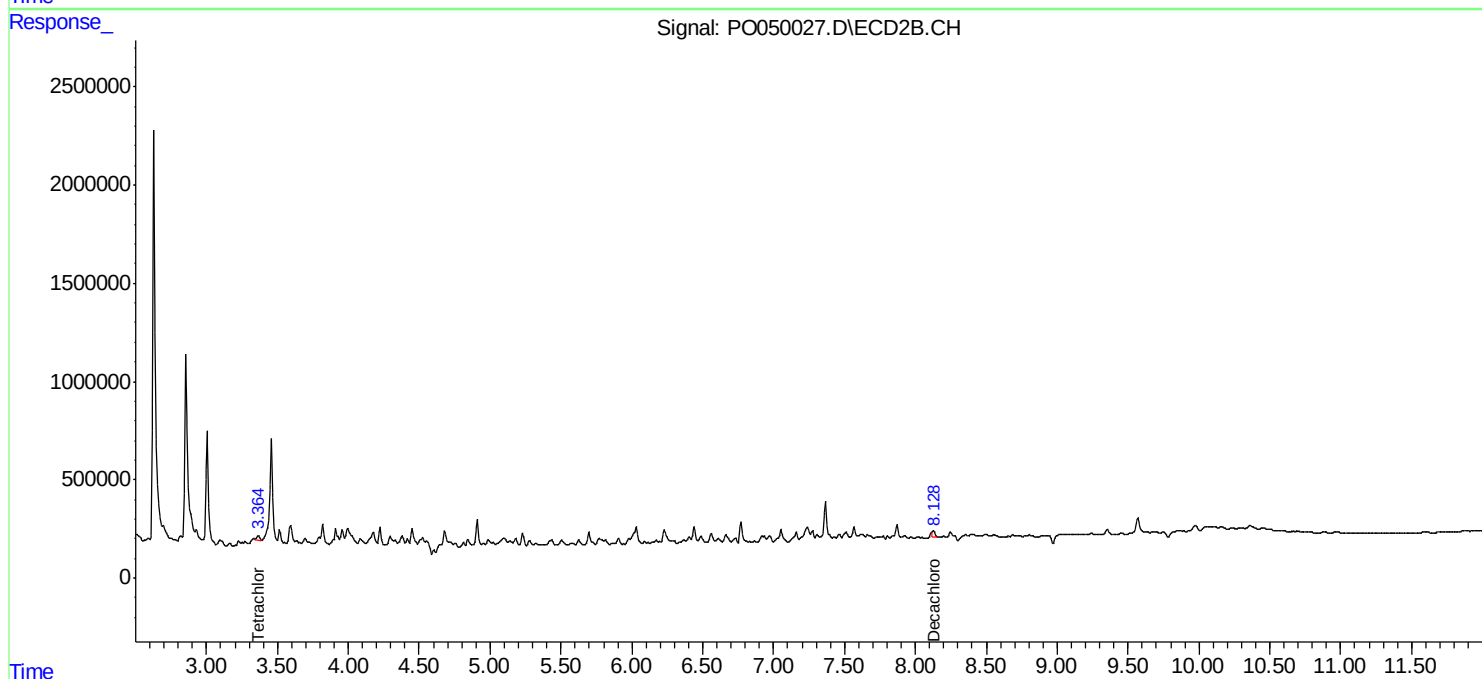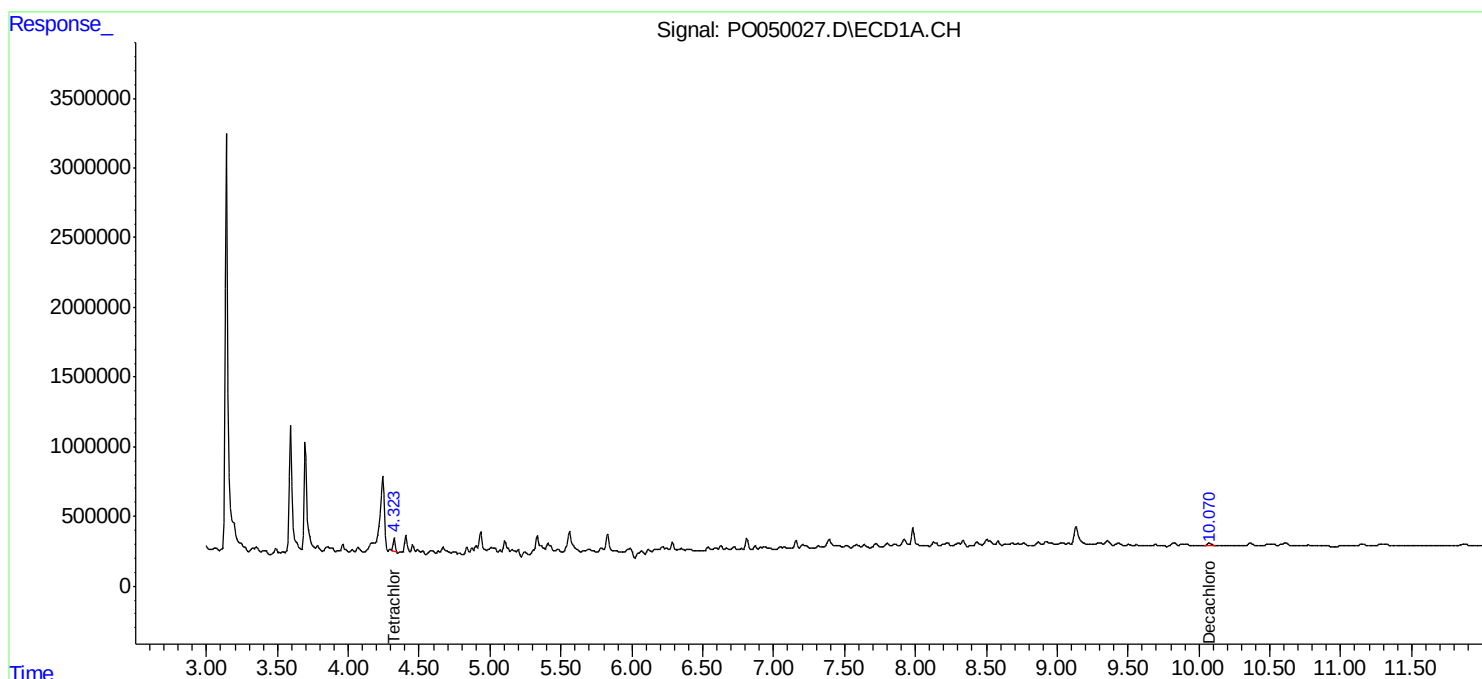

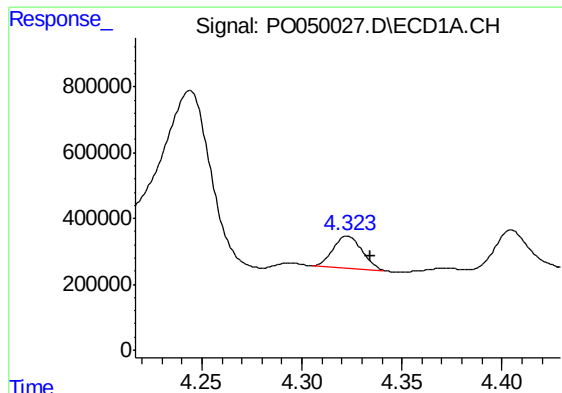


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.011 min
Response: 994171
Conc: 4.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
A365210


Manual Integrations
APPROVED

Sohil
10/16/2018 2:45:59 PM

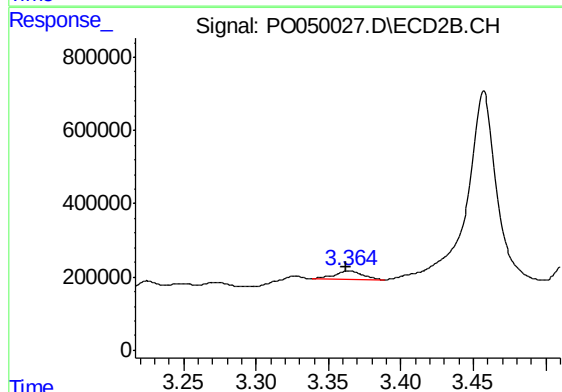


#1 Tetrachloro-m-xylene

R.T.: 3.364 min
Delta R.T.: 0.001 min
Response: 318064
Conc: 1.62 ng/ml m

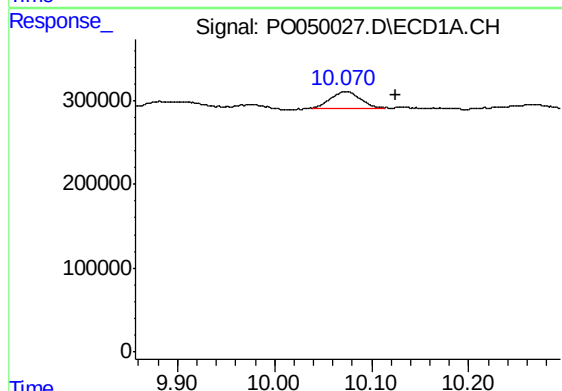

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: -0.054 min
Response: 415472
Conc: 2.21 ng/ml m

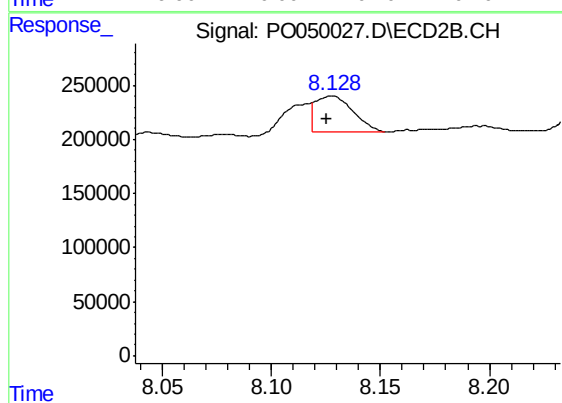

#2 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 388123
Conc: 2.26 ng/ml m