

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101518\
 Data File : P0050035.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2018 19:17
 Operator : SM/SJ
 Sample : J5455-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-OILY-WATER

Manual Integrations
 APPROVED

Sohil
 10/16/2018 2:46:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:16:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.328	3.367	3445727	2305437	13.987	11.767
2)	SA Decachlor...	10.078	8.126	2300616	2132679	12.221m	12.402

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050035.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2018 19:17
Operator : SM/SJ
Sample : J5455-05
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MS-OILY-WATER


Manual Integrations
APPROVED

Sohil
10/16/2018 2:46:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:16:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

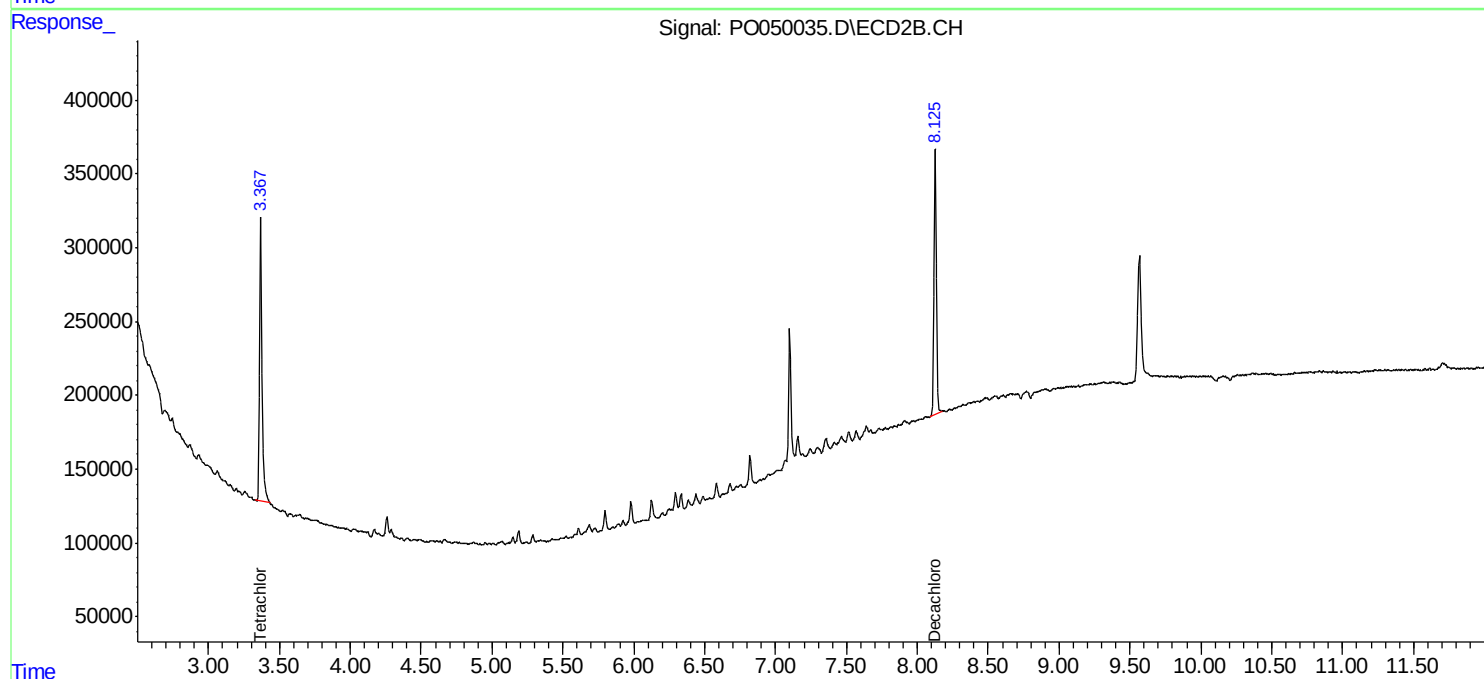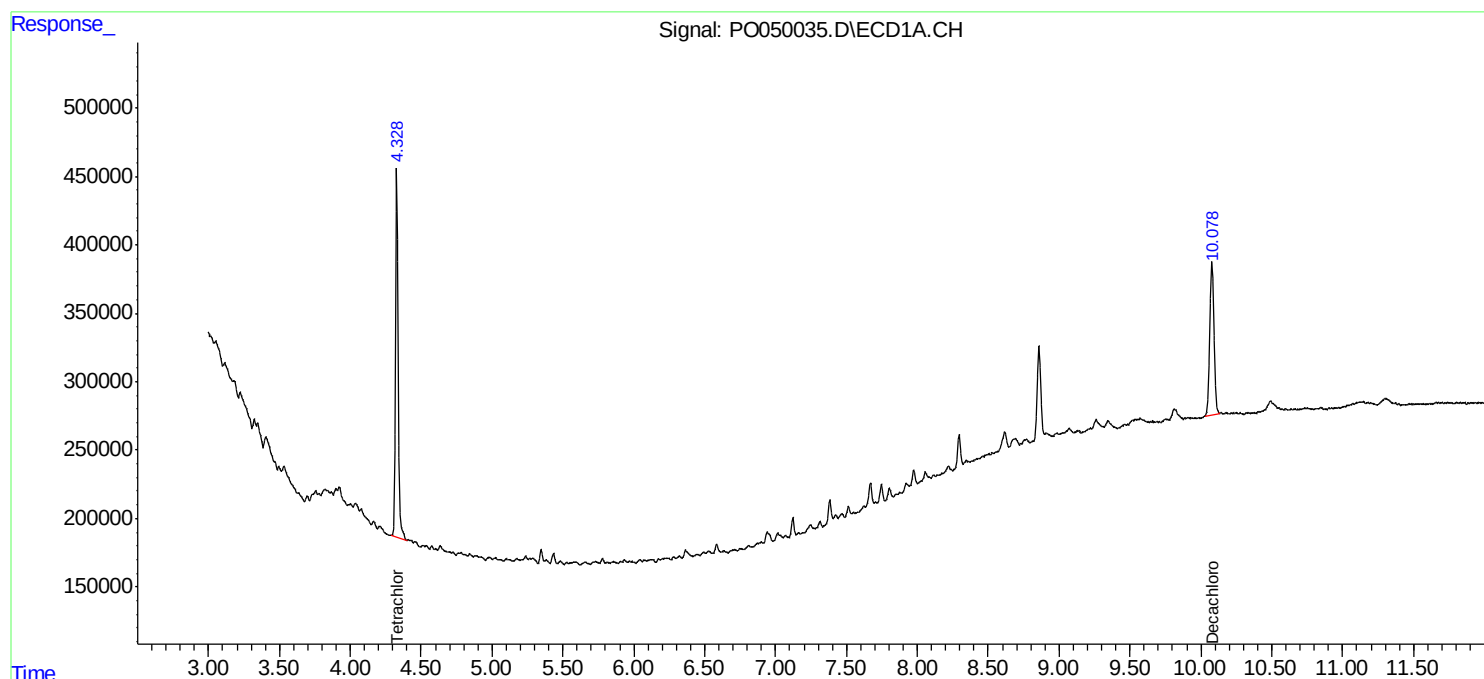

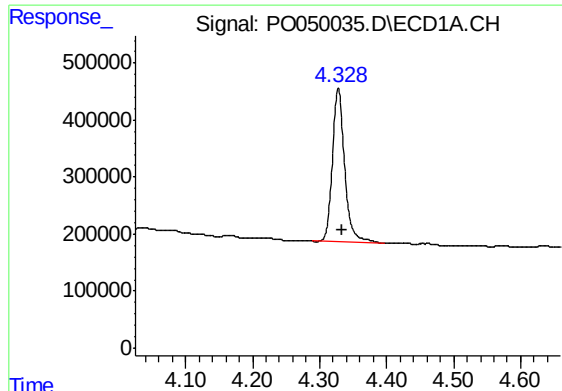


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.006 min
Response: 3445727
Conc: 13.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-OILY-WATER


Manual Integrations
APPROVED

Sohil
10/16/2018 2:46:06 PM

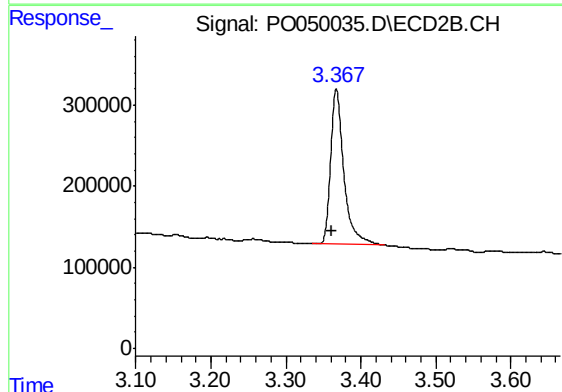


#1 Tetrachloro-m-xylene

R.T.: 3.367 min
Delta R.T.: 0.005 min
Response: 2305437
Conc: 11.77 ng/ml

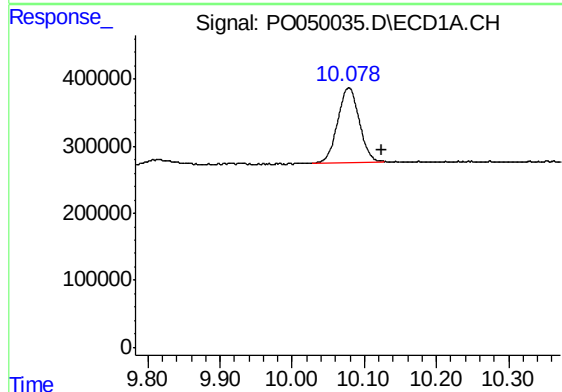

#2 Decachlorobiphenyl

R.T.: 10.078 min
Delta R.T.: -0.046 min
Response: 2300616
Conc: 12.22 ng/ml m

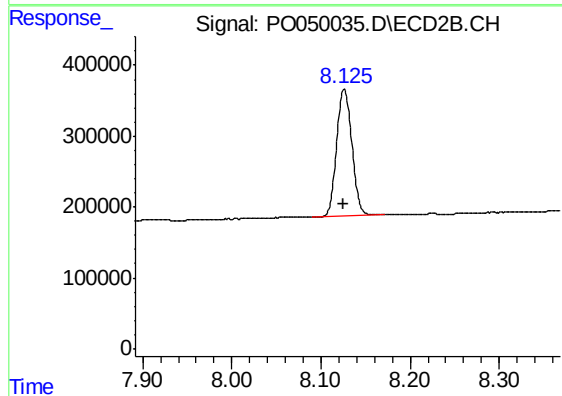

#2 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 2132679
Conc: 12.40 ng/ml