

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101518\
 Data File : P0050039.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2018 20:32
 Operator : SM/SJ
 Sample : J5456-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-FRAC-TANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:36:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.367	4720255	3594007	19.161	18.344
2) SA Decachlor...	10.085	8.130	2600876	2459356	13.816m	14.302

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050039.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2018 20:32
Operator : SM/SJ
Sample : J5456-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-FRAC-TANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:36:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

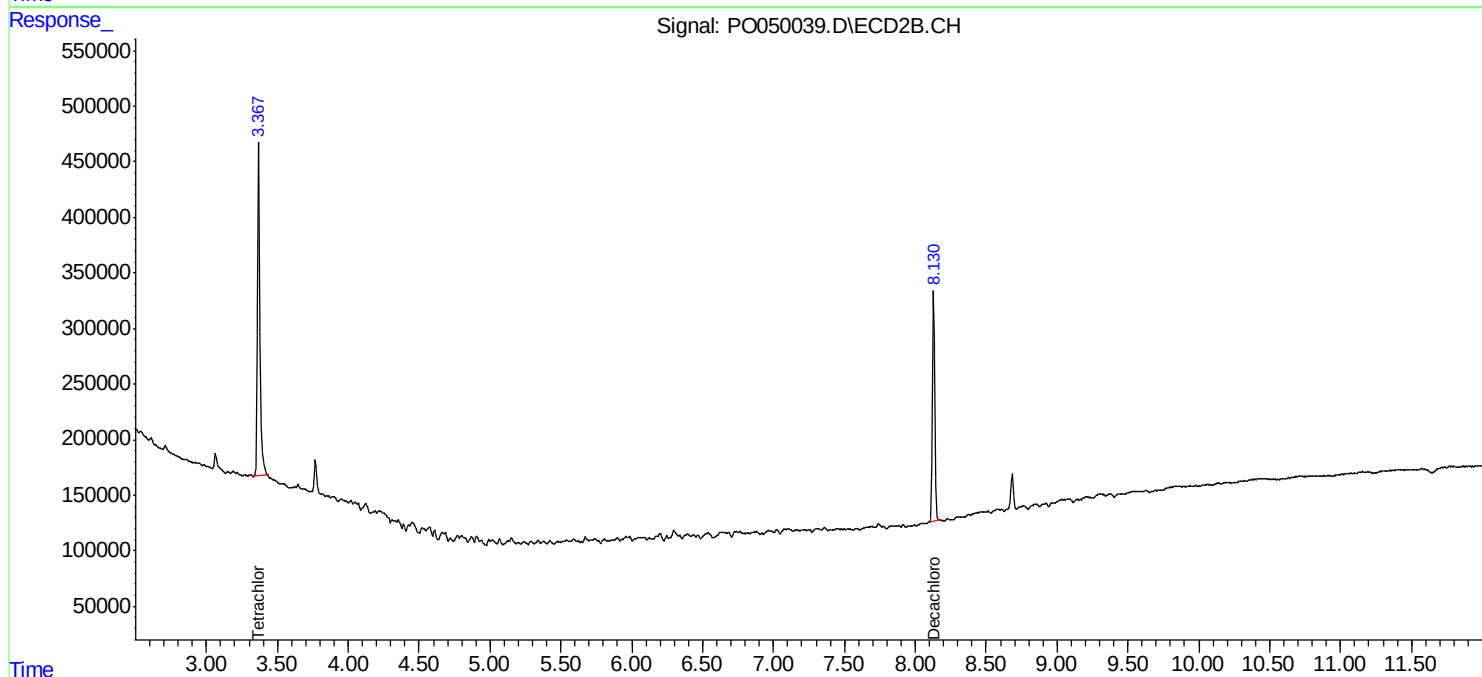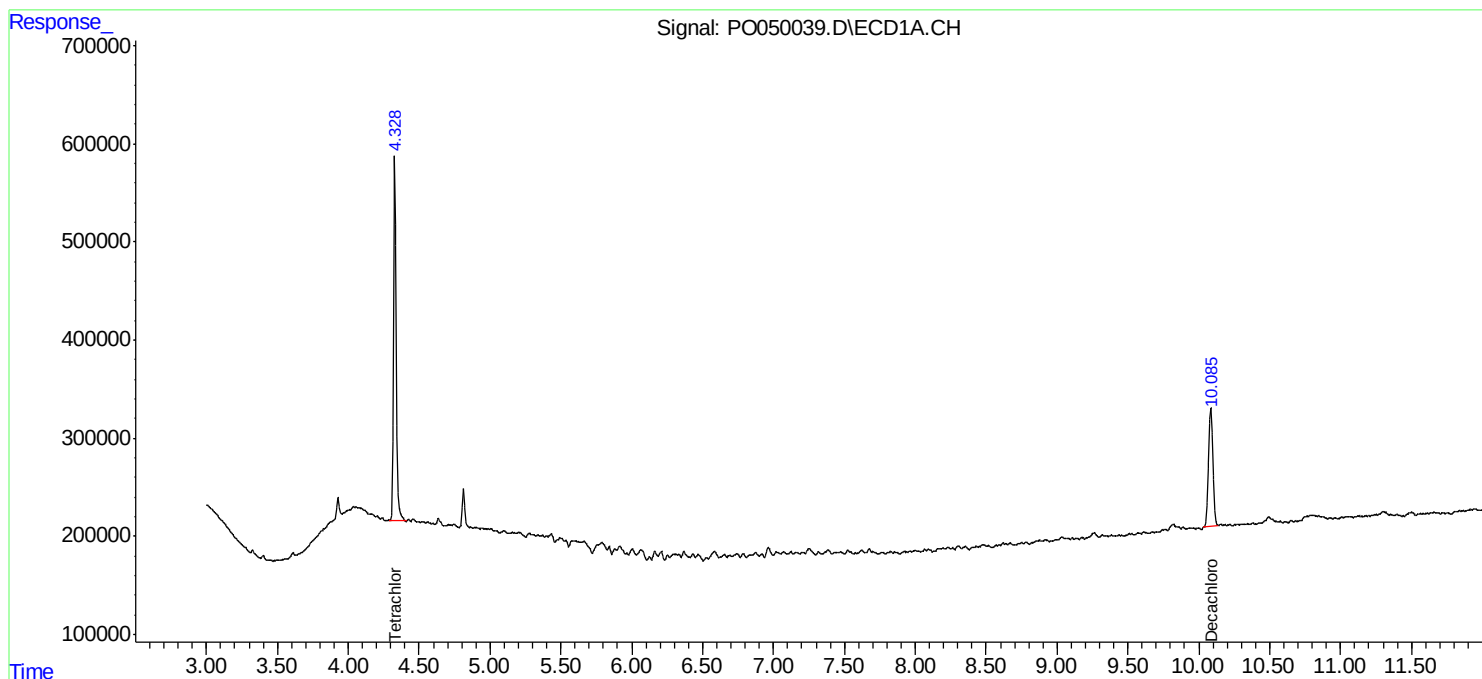


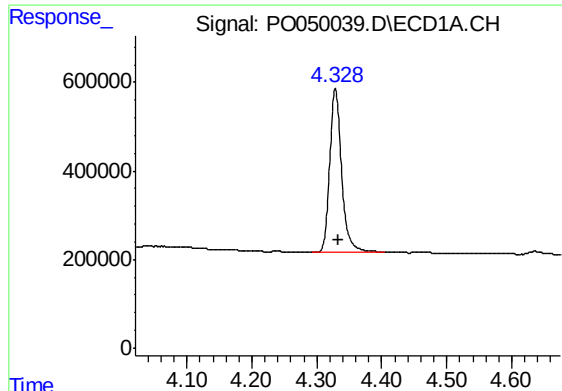

#1 Tetrachloro-m-xylene


R.T.: 4.329 min
Delta R.T.: -0.005 min
Response: 4720255
Conc: 19.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-FRAC-TANK

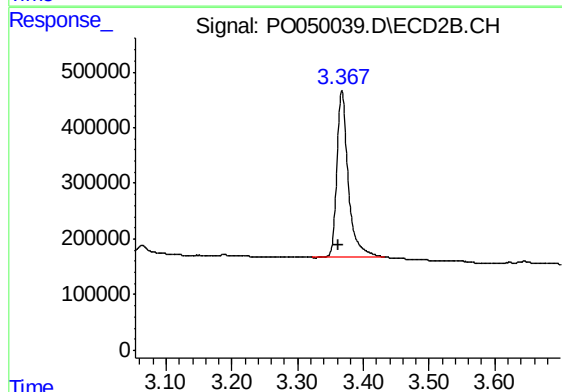


#1 Tetrachloro-m-xylene

R.T.: 3.367 min
Delta R.T.: 0.005 min
Response: 3594007
Conc: 18.34 ng/ml

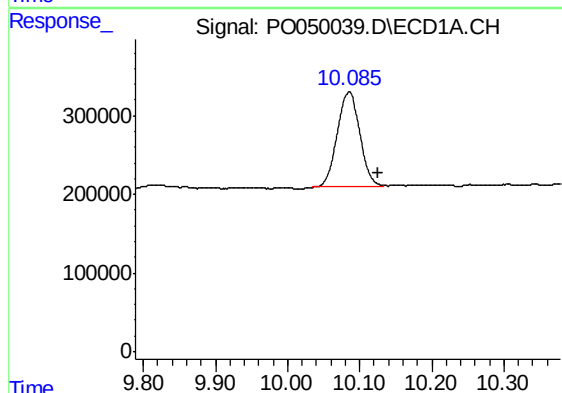

#2 Decachlorobiphenyl

R.T.: 10.085 min
Delta R.T.: -0.039 min
Response: 2600876
Conc: 13.82 ng/ml m

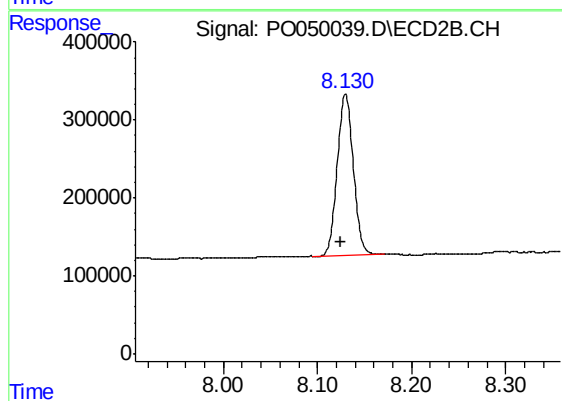

#2 Decachlorobiphenyl

R.T.: 8.130 min
Delta R.T.: 0.005 min
Response: 2459356
Conc: 14.30 ng/ml