

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101518\
 Data File : P0050042.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2018 21:29
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Sohil
 10/16/2018 2:46:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:36:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.328	3.365	6072569	5199601	24.650	26.539
2)	SA Decachlor...	10.071	8.127	3404259	3281674	18.084m	19.084

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050042.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2018 21:29
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
10/16/2018 2:46:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:36:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

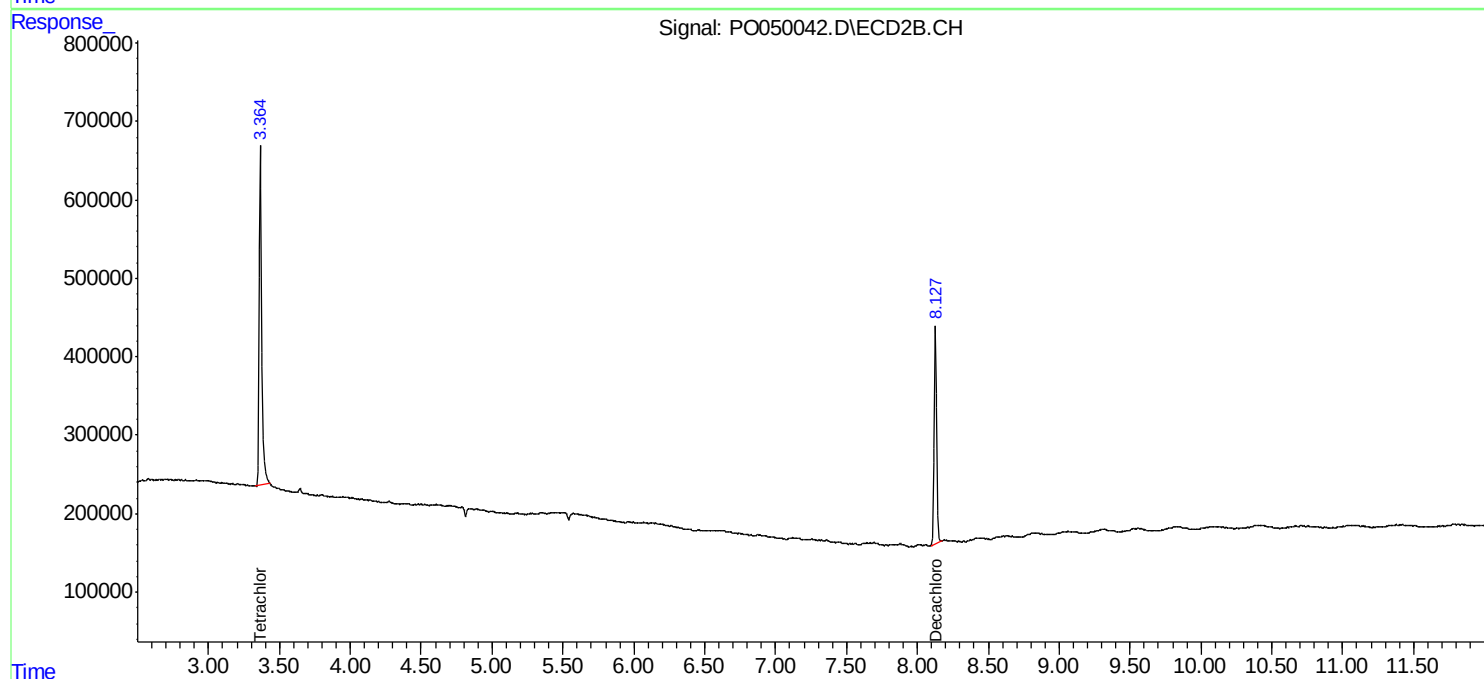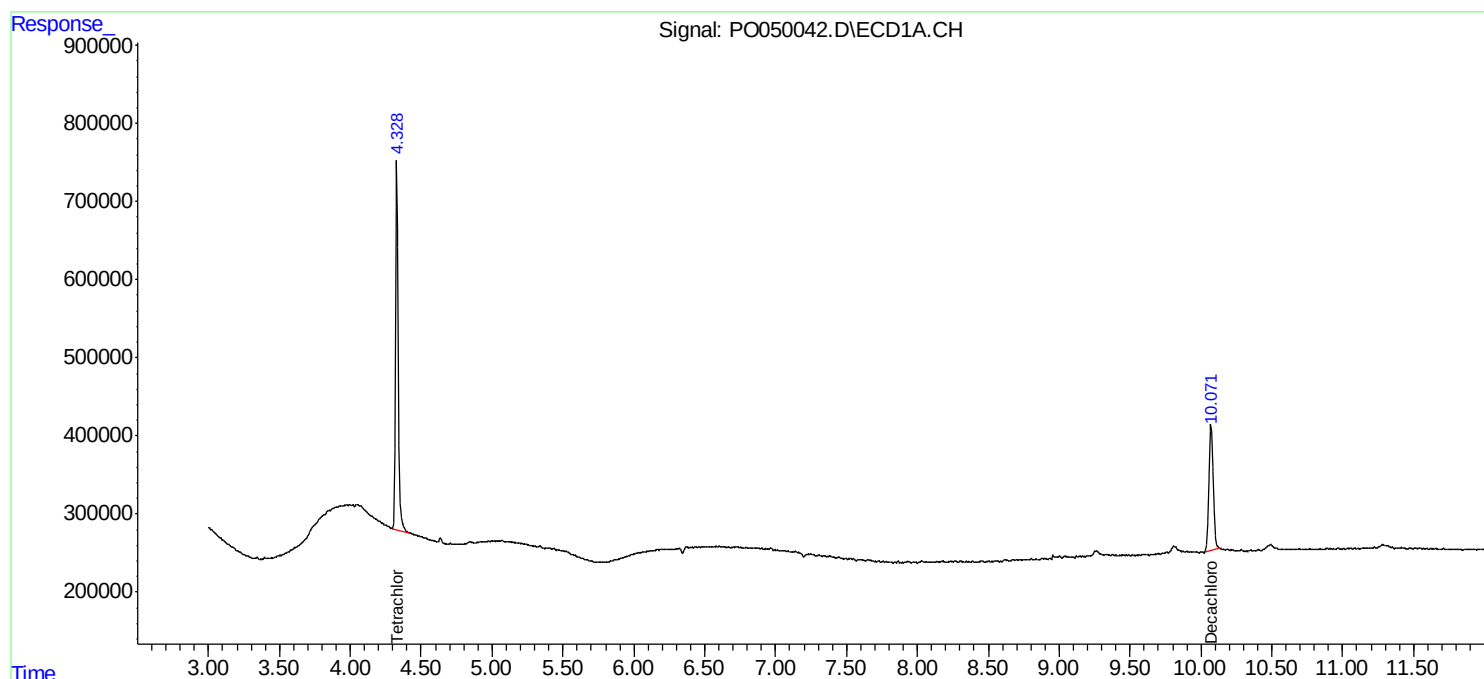

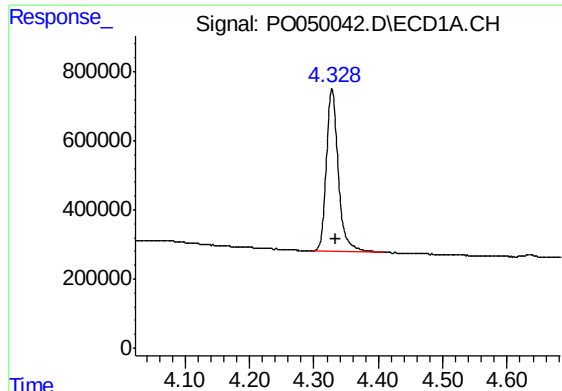


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.006 min
Response: 6072569
Conc: 24.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
10/16/2018 2:46:38 PM

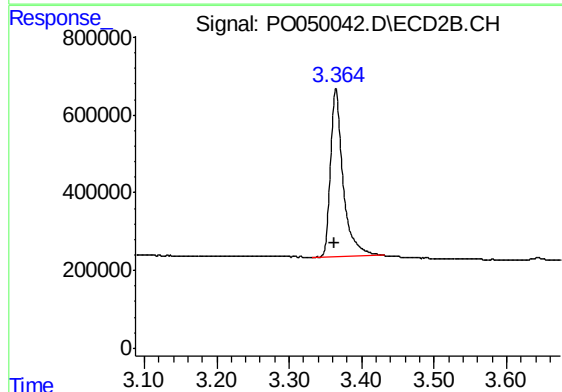


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: 0.002 min
Response: 5199601
Conc: 26.54 ng/ml

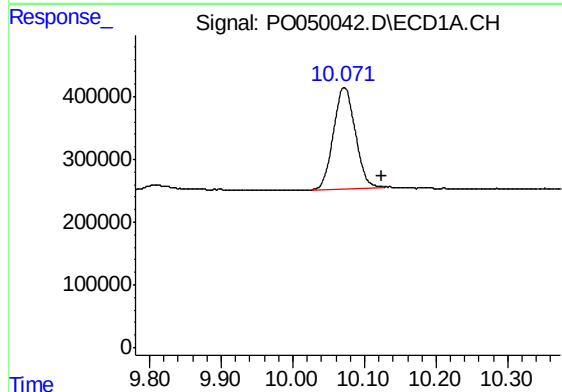

#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: -0.054 min
Response: 3404259
Conc: 18.08 ng/ml m

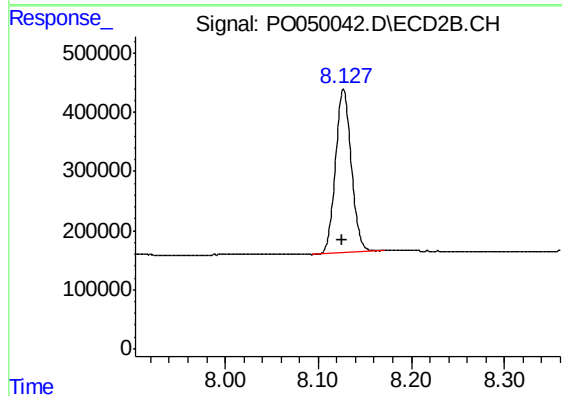

#2 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.002 min
Response: 3281674
Conc: 19.08 ng/ml