

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101518\
 Data File : P0050045.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2018 23:04
 Operator : SM/SJ
 Sample : J5455-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-OILY-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 09:30:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.368	3417097	2377197	13.871	12.133
2) SA Decachlor...	0.000	8.127	0	2091015	N.D.	12.160 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050045.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2018 23:04
Operator : SM/SJ
Sample : J5455-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-OILY-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 09:30:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

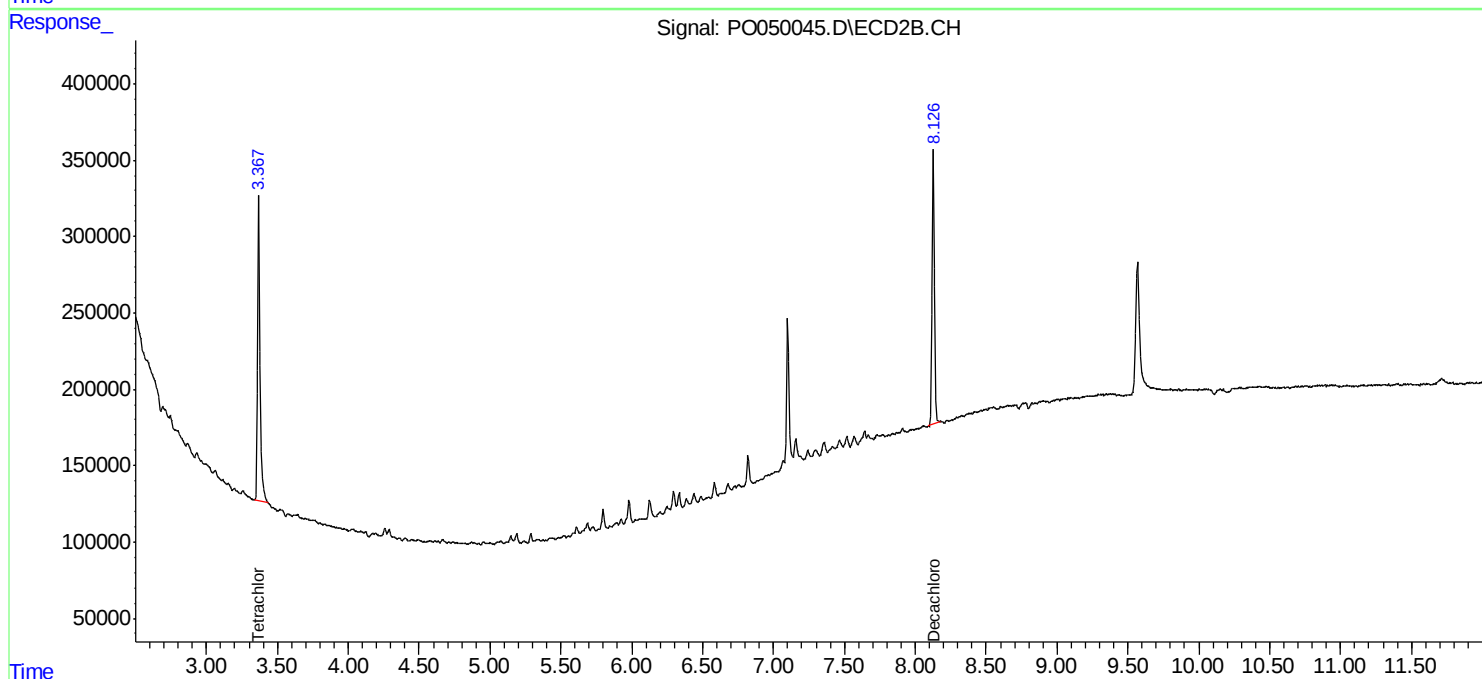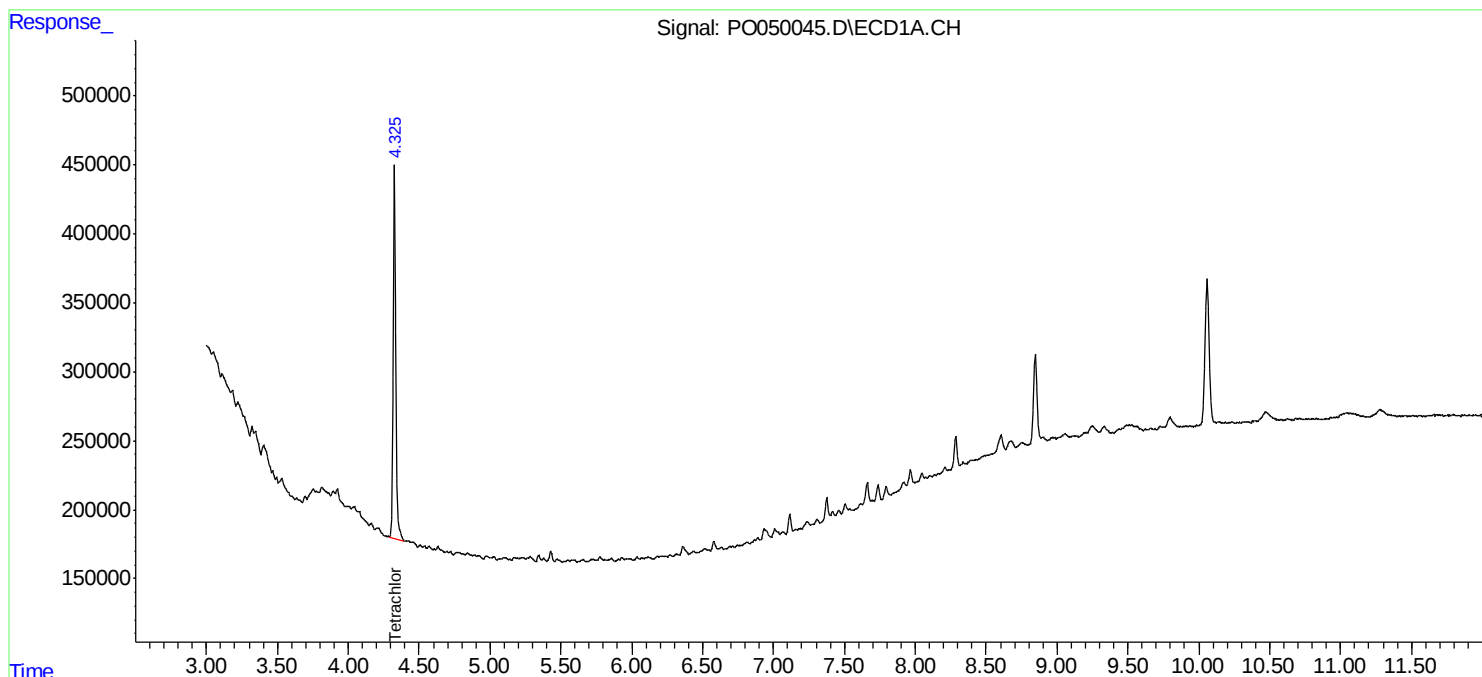


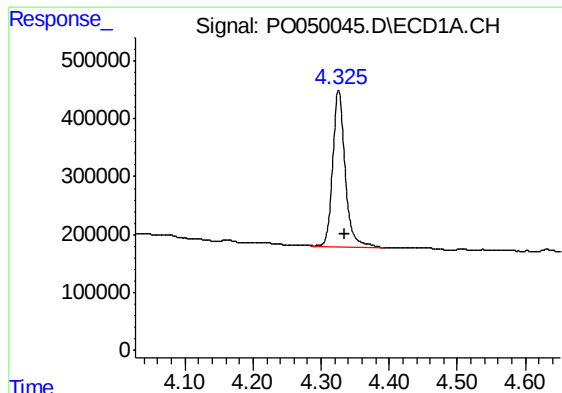

#1 Tetrachloro-m-xylene


R.T.: 4.326 min
Delta R.T.: -0.008 min
Response: 3417097
Conc: 13.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-OILY-WATER

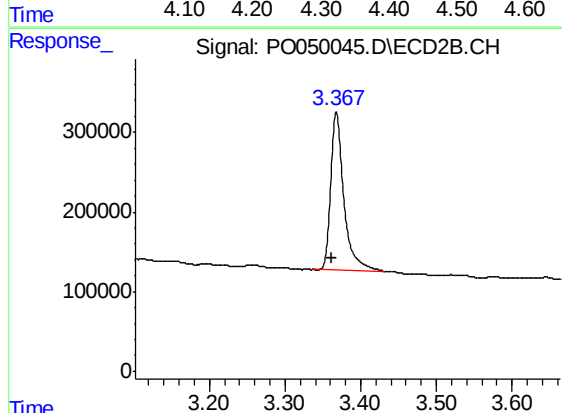


#1 Tetrachloro-m-xylene

R.T.: 3.368 min
Delta R.T.: 0.005 min
Response: 2377197
Conc: 12.13 ng/ml

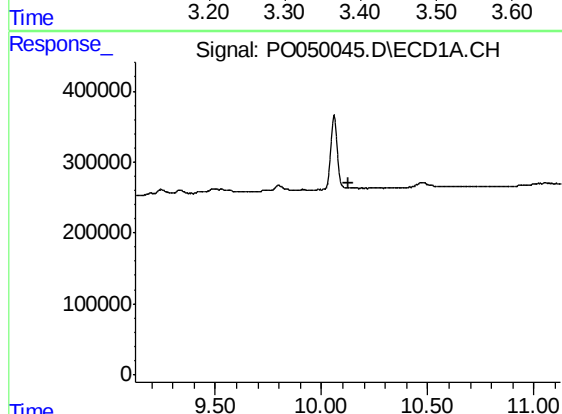

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.125 min
Response: 0
Conc: N.D.

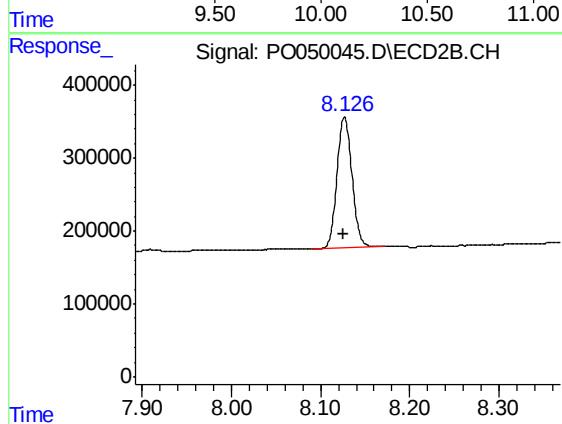

#2 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.001 min
Response: 2091015
Conc: 12.16 ng/ml