

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
 Data File : P0050049.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2018 00:20
 Operator : SM/SJ
 Sample : J5456-01RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-FRAC-TANKRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 09:35:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.329	3.367	4697305	3671246	19.068	18.738
2)	SA Decachlor...	10.082	8.128	2586419	2449064	13.739m	14.242

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101518\
Data File : PO050049.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2018 00:20
Operator : SM/SJ
Sample : J5456-01RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-FRAC-TANKRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 09:35:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

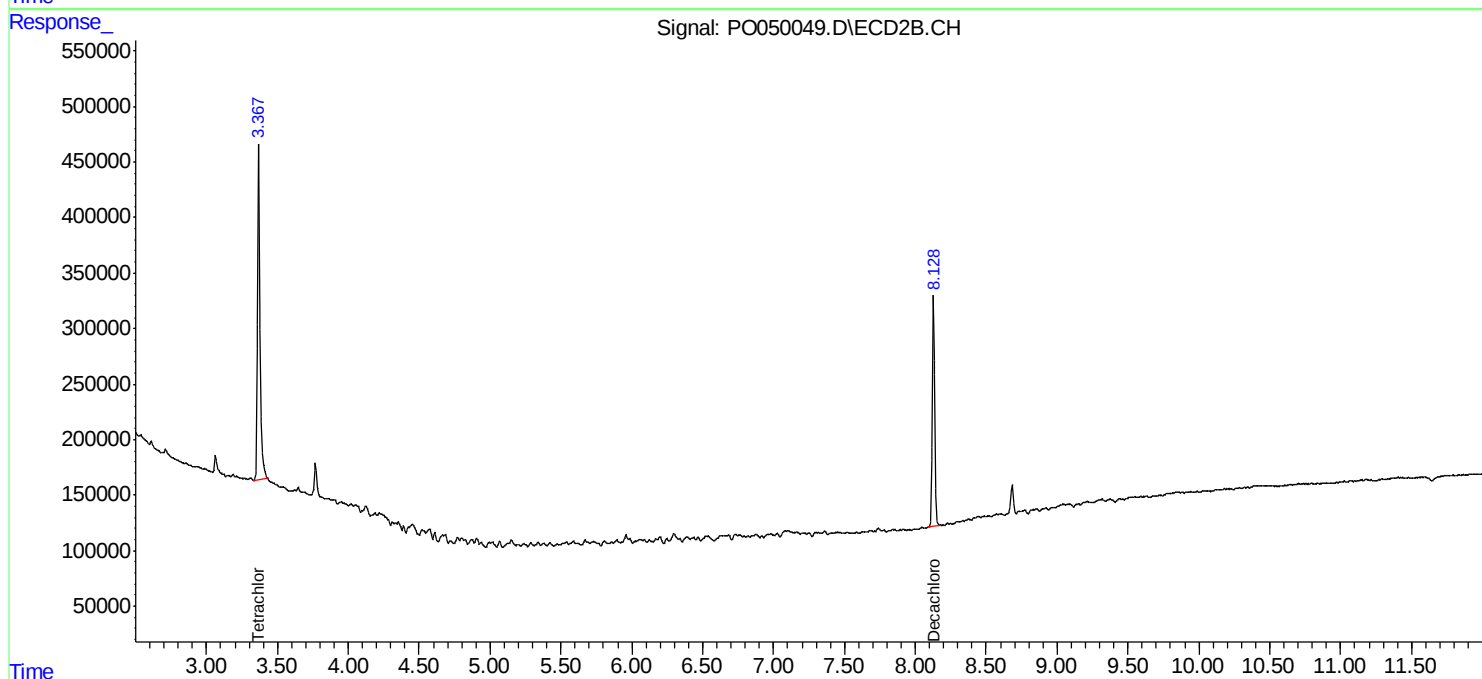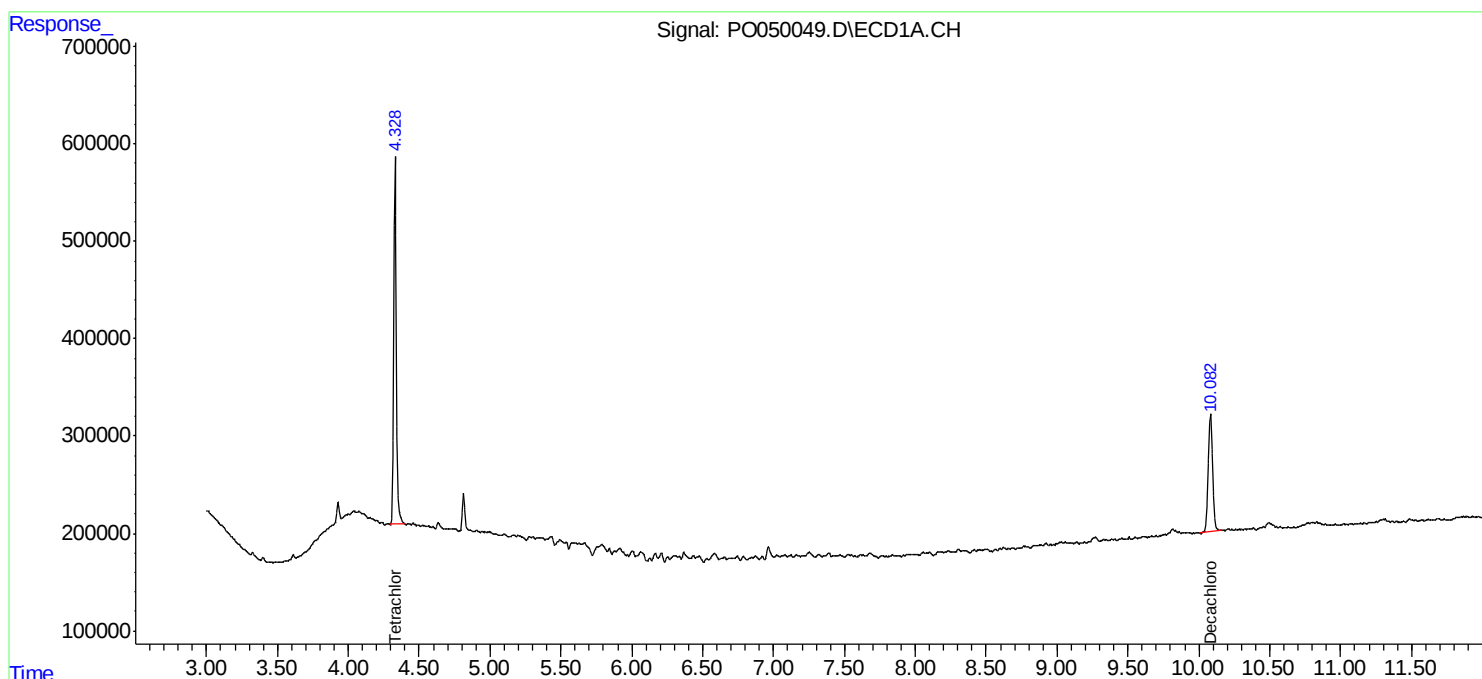


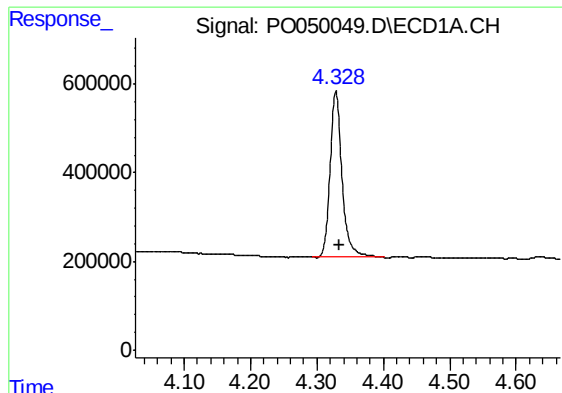

#1 Tetrachloro-m-xylene


R.T.: 4.329 min
Delta R.T.: -0.005 min
Response: 4697305
Conc: 19.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-FRAC-TANKRE

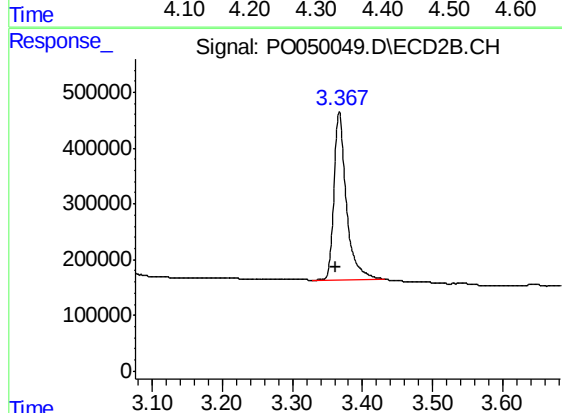


#1 Tetrachloro-m-xylene

R.T.: 3.367 min
Delta R.T.: 0.005 min
Response: 3671246
Conc: 18.74 ng/ml

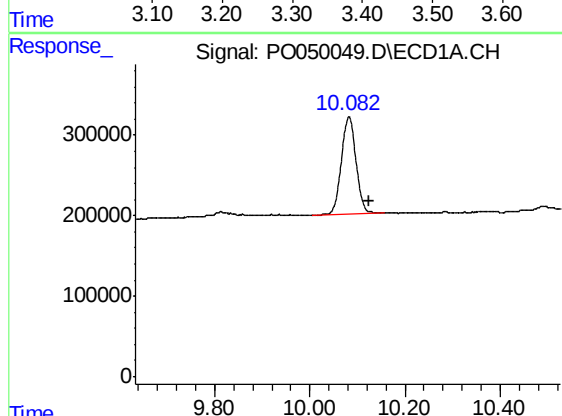

#2 Decachlorobiphenyl

R.T.: 10.082 min
Delta R.T.: -0.043 min
Response: 2586419
Conc: 13.74 ng/ml m

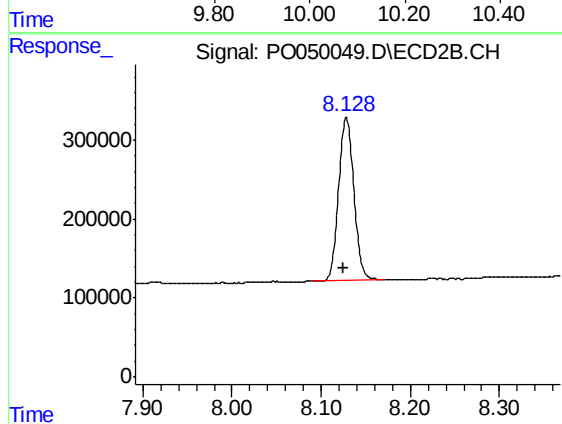

#2 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.003 min
Response: 2449064
Conc: 14.24 ng/ml