

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101519\
 Data File : P0061993.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2019 9:01
 Operator : HP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 13:35:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.483	1362594	1051412	22.032	24.519
2)	SA Decachlor...	9.950	8.336	1204534	669986	21.528	22.834
Target Compounds							
7)	L1 AR-1016-5	0.000	4.933	0	1415	N.D.	1.097 #
8)	L2 AR-1221-1	0.000	3.631	0	6396	N.D.	12.579 #
14)	L3 AR-1232-4	0.000	4.848	0	10084	N.D.	12.396 #
15)	L3 AR-1232-5	0.000	4.933	0	1415	N.D.	1.602 #
19)	L4 AR-1242-4	0.000	4.848	0	10084	N.D.	10.682 #
23)	L5 AR-1248-3	0.000	4.848	0	10084	N.D.	7.597 #
24)	L5 AR-1248-4	0.000	4.933	0	1415	N.D.	0.894 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101519\
Data File : PO061993.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 9:01
Operator : HP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 13:35:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

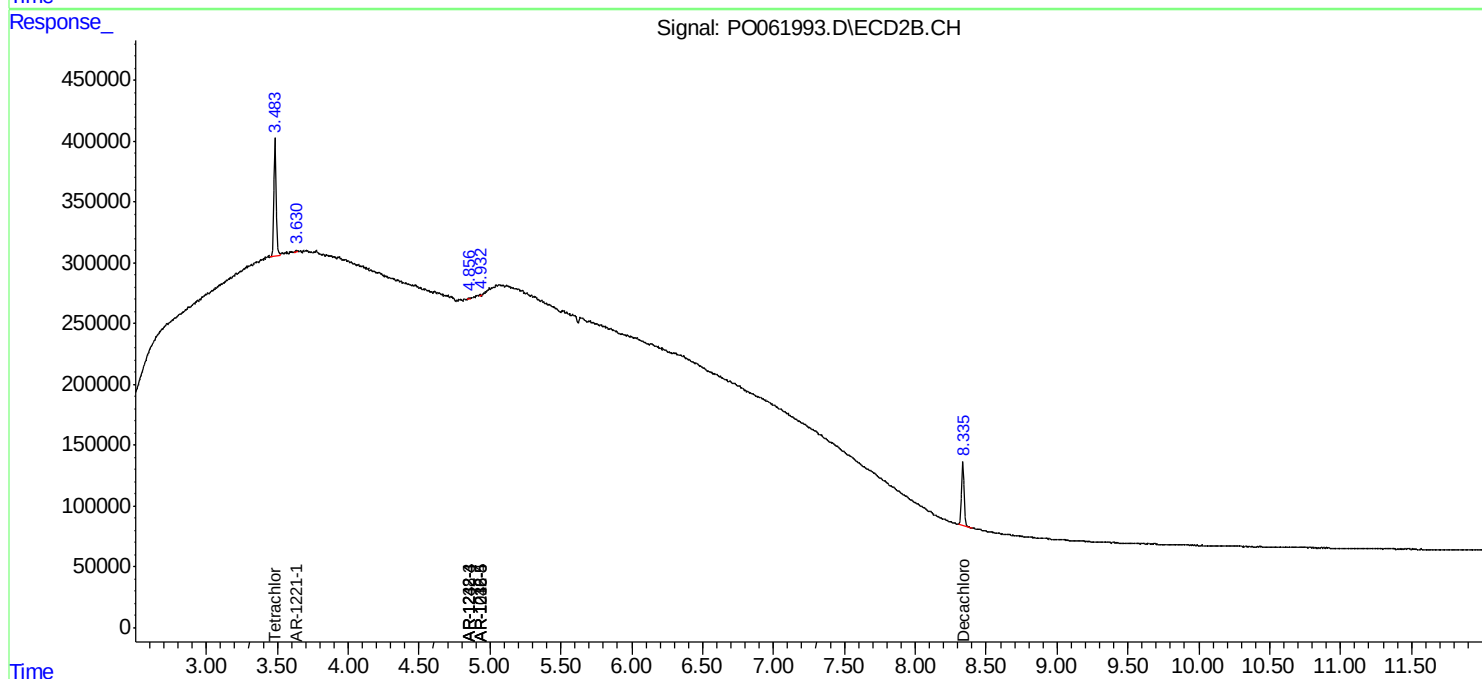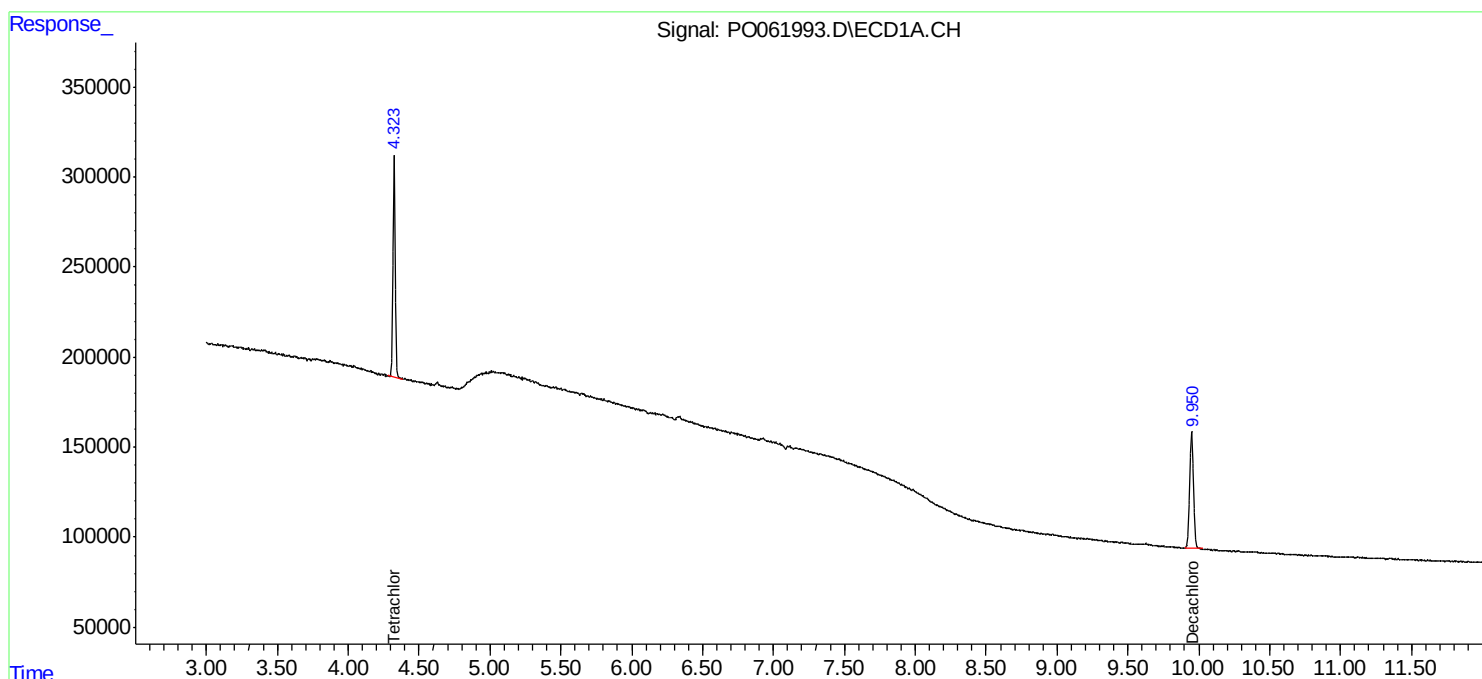


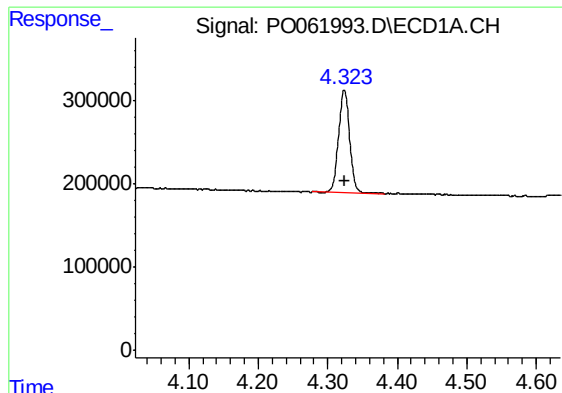

#1 Tetrachloro-m-xylene


R.T.: 4.324 min
Delta R.T.: -0.001 min
Response: 1362594
Conc: 22.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

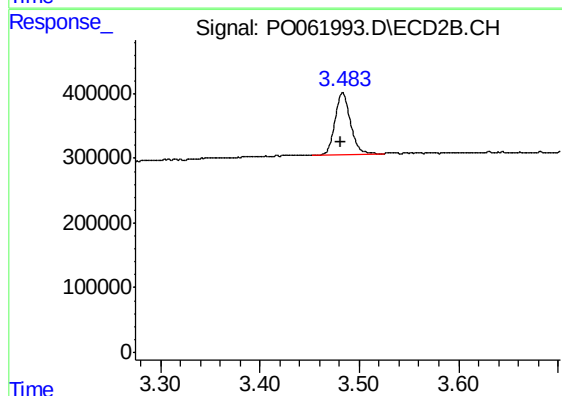


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.002 min
Response: 1051412
Conc: 24.52 ng/ml

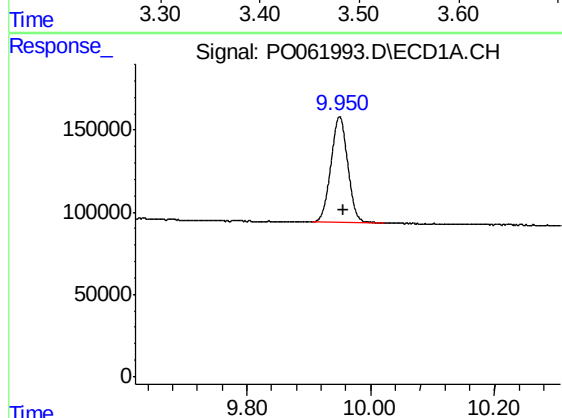


#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.007 min
Response: 1204534
Conc: 21.53 ng/ml

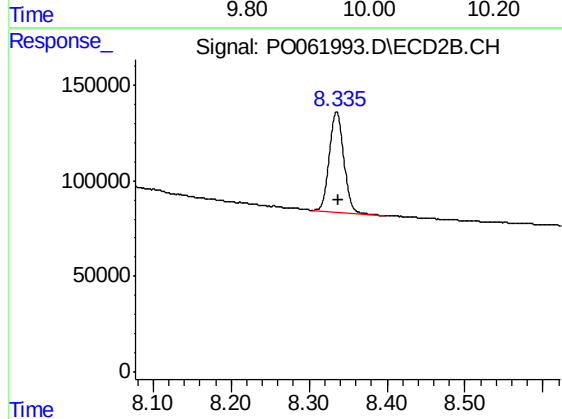

#2 Decachlorobiphenyl


R.T.: 8.336 min
Delta R.T.: -0.002 min
Response: 669986
Conc: 22.83 ng/ml

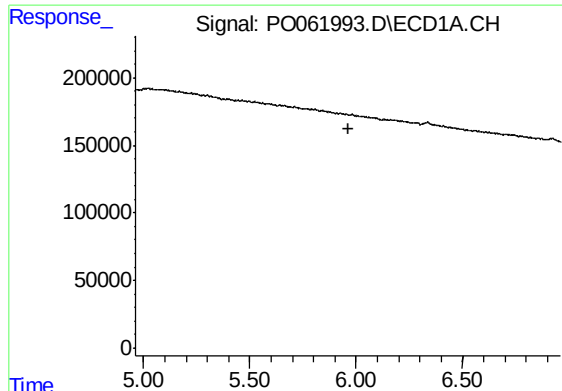

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.961 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

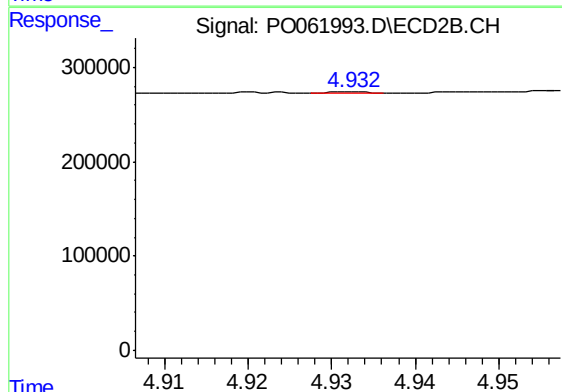


#7 AR-1016-5

R.T.: 4.933 min
Delta R.T.: -0.030 min
Response: 1415
Conc: 1.10 ng/ml

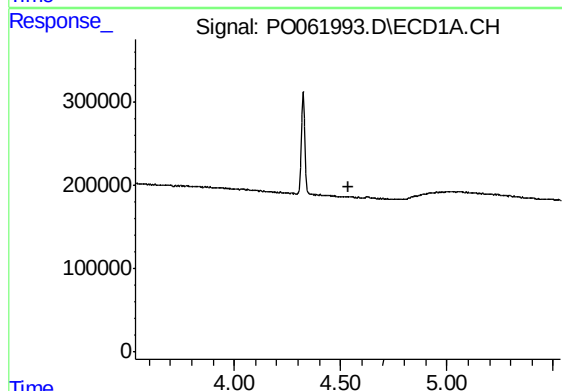


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.535 min
Response: 0
Conc: N.D.

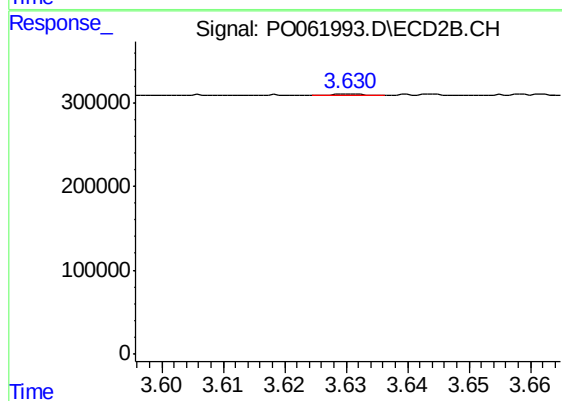

#8 AR-1221-1


R.T.: 3.631 min
Delta R.T.: -0.058 min
Response: 6396
Conc: 12.58 ng/ml

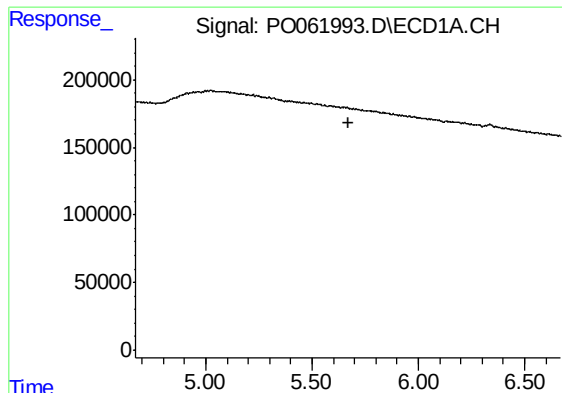

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

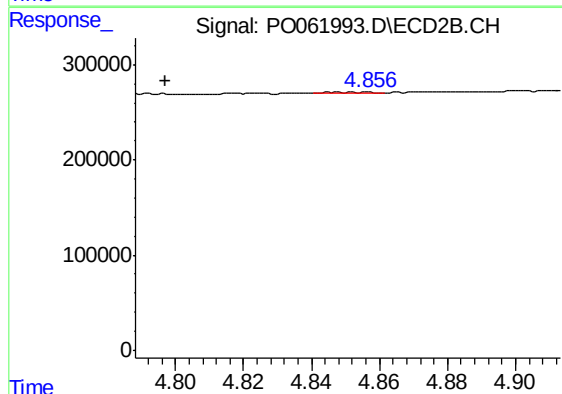


#14 AR-1232-4

R.T.: 4.848 min
Delta R.T.: 0.051 min
Response: 10084
Conc: 12.40 ng/ml

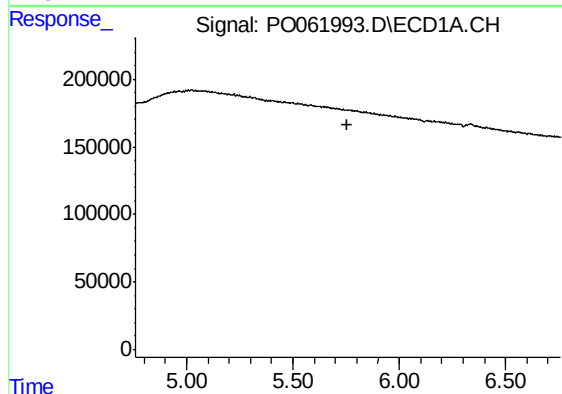


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.758 min
Response: 0
Conc: N.D.

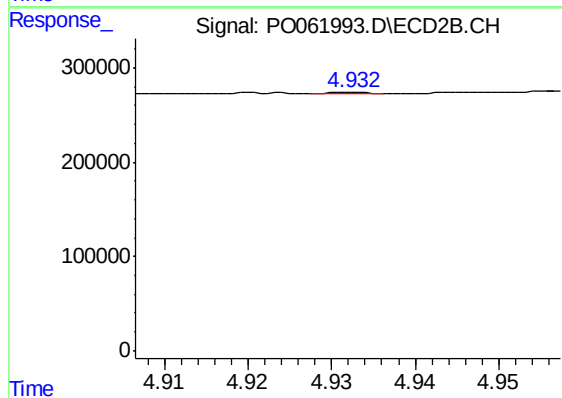

#15 AR-1232-5


R.T.: 4.933 min
Delta R.T.: -0.030 min
Response: 1415
Conc: 1.60 ng/ml

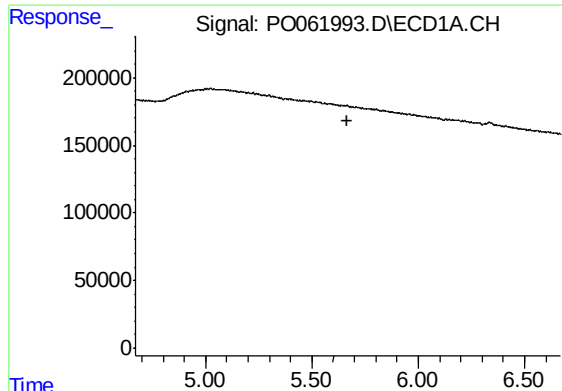

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

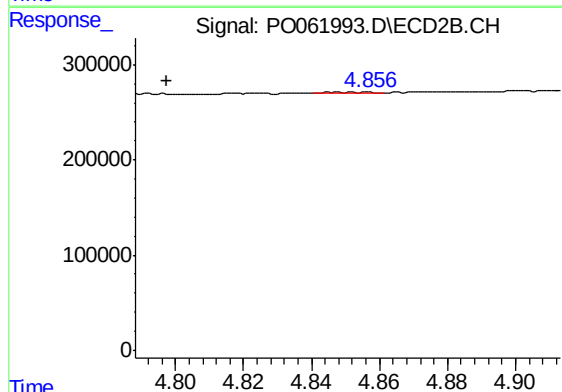


#19 AR-1242-4

R.T.: 4.848 min
Delta R.T.: 0.050 min
Response: 10084
Conc: 10.68 ng/ml

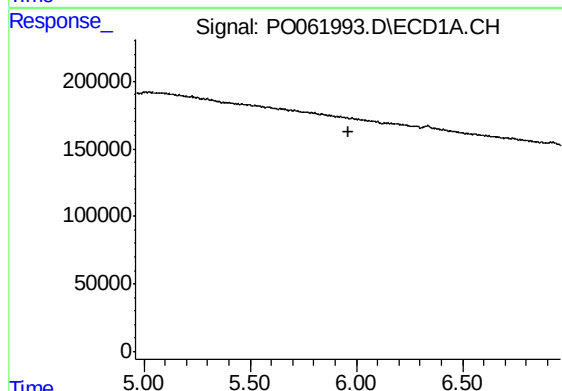


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

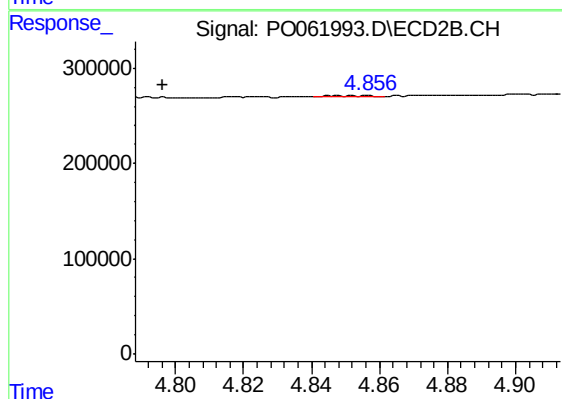

#23 AR-1248-3


R.T.: 4.848 min
Delta R.T.: 0.051 min
Response: 10084
Conc: 7.60 ng/ml

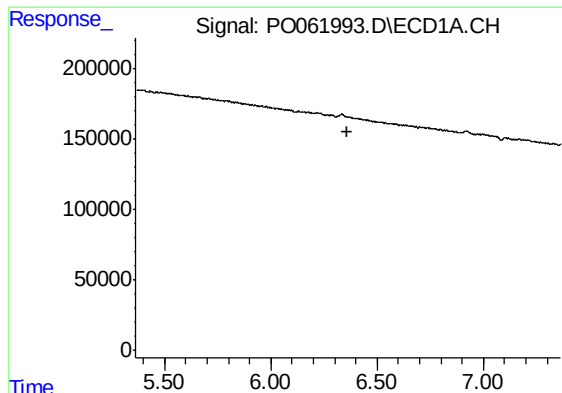

#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

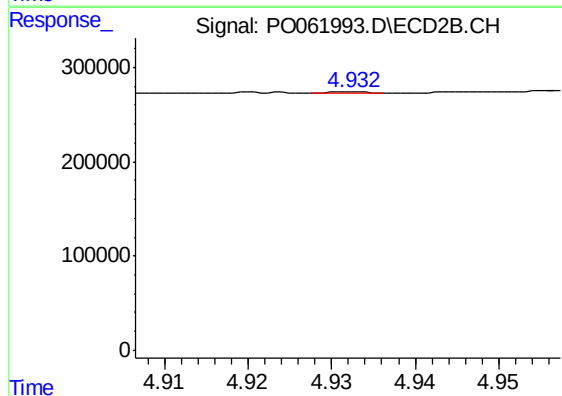

#24 AR-1248-4

R.T.: 4.933 min
Delta R.T.: -0.030 min
Response: 1415
Conc: 0.89 ng/ml