

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101519\
 Data File : PO062027.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2019 19:28
 Operator : HP/AJ
 Sample : K5352-11RE
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-20A-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:10:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.482	1137041	782146	18.385	18.240
2) SA Decachlor...	9.948	8.336	1022453	515558	18.274	17.571

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101519\
Data File : PO062027.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 19:28
Operator : HP/AJ
Sample : K5352-11RE
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-20A-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:10:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

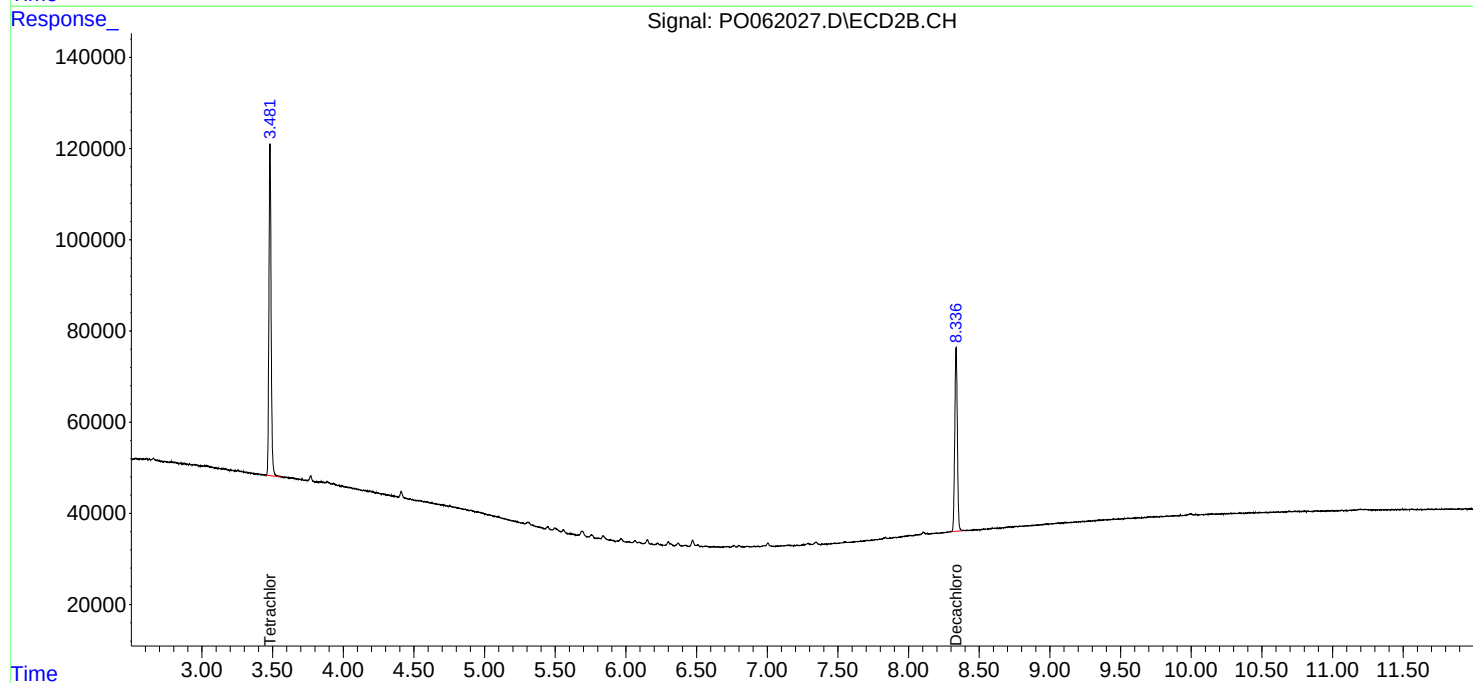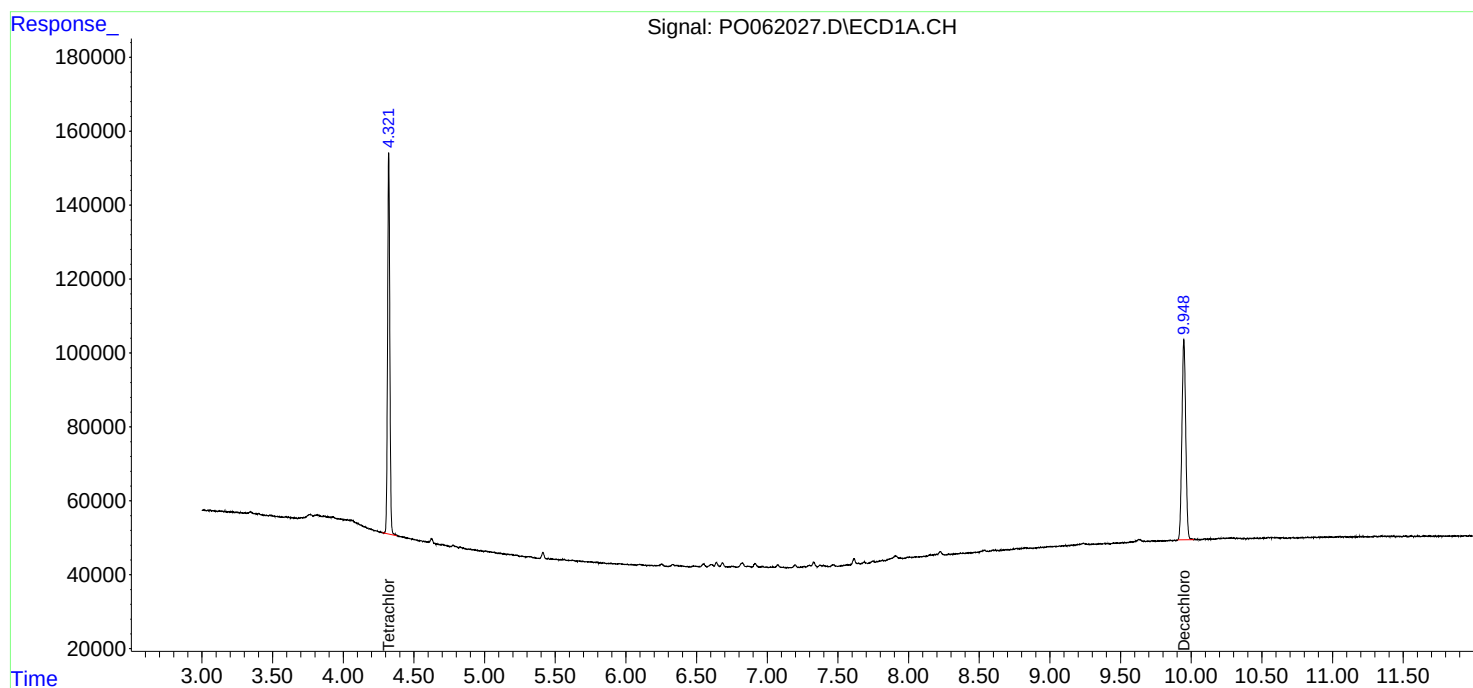


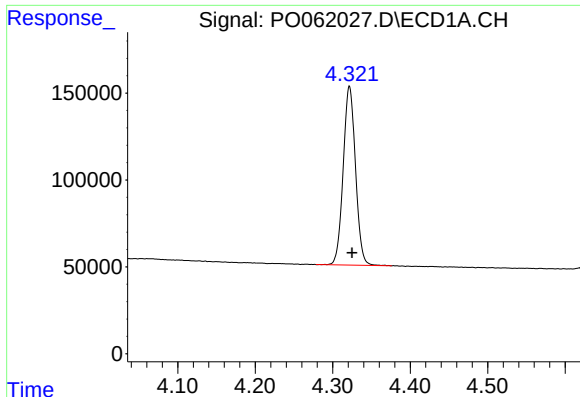

#1 Tetrachloro-m-xylene


R.T.: 4.322 min
Delta R.T.: -0.003 min
Response: 1137041
Conc: 18.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20A-D

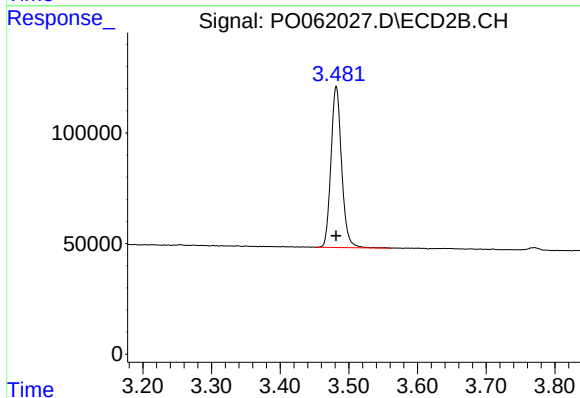


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 782146
Conc: 18.24 ng/ml

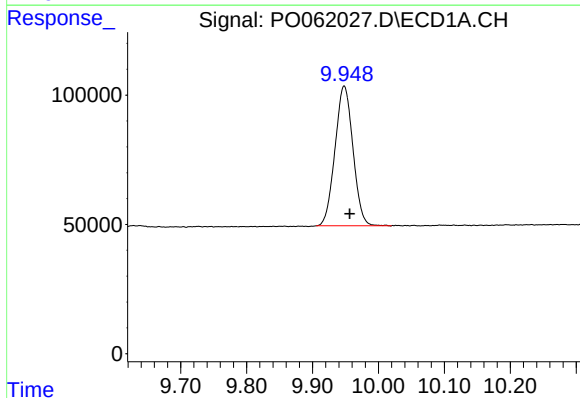

#2 Decachlorobiphenyl

R.T.: 9.948 min
Delta R.T.: -0.008 min
Response: 1022453
Conc: 18.27 ng/ml

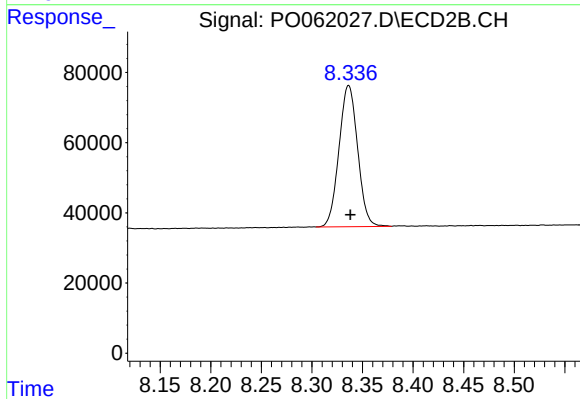

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.002 min
Response: 515558
Conc: 17.57 ng/ml