

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101519\
 Data File : P0062018.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2019 17:00
 Operator : HP/AJ
 Sample : K5355-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-31

Manual Integrations
 APPROVED

Ankita
 10/16/2019 12:01:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:06:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.323	3.484	1281015	885060	20.713	20.640
2)	SA Decachlor...	9.948	8.336	1223254	575701	21.862	19.621
Target Compounds							
31)	L7 AR-1260-1	7.075	5.966	598324	361790	210.150	170.276
32)	L7 AR-1260-2	7.327	6.153	955349	440331	278.482m	173.521 #
33)	L7 AR-1260-3	7.688	6.301	495933	313992	187.419	139.051 #
34)	L7 AR-1260-4	7.912	6.764	574190	255396	205.284m	145.454 #
35)	L7 AR-1260-5	8.223	7.004	840605	552271	160.556m	153.305

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101519\
Data File : PO062018.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 17:00
Operator : HP/AJ
Sample : K5355-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
COMP-31


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:06:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

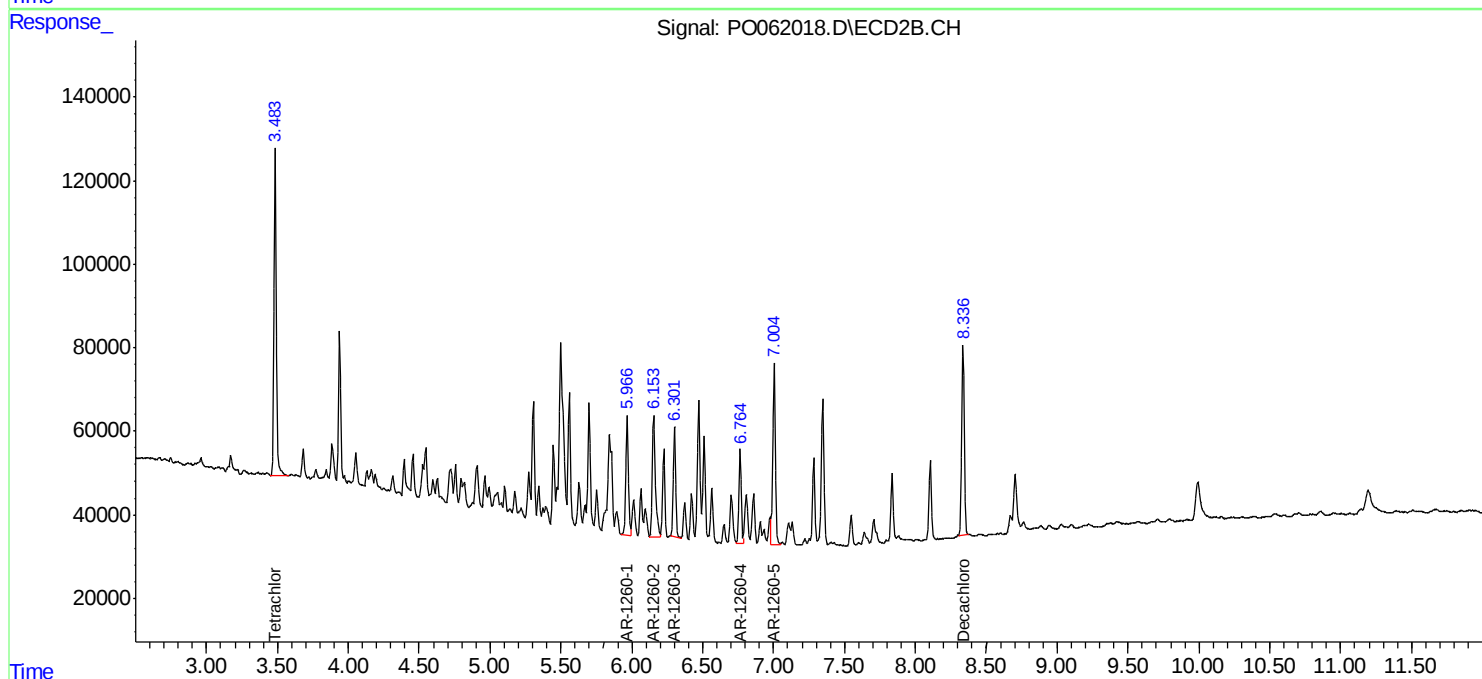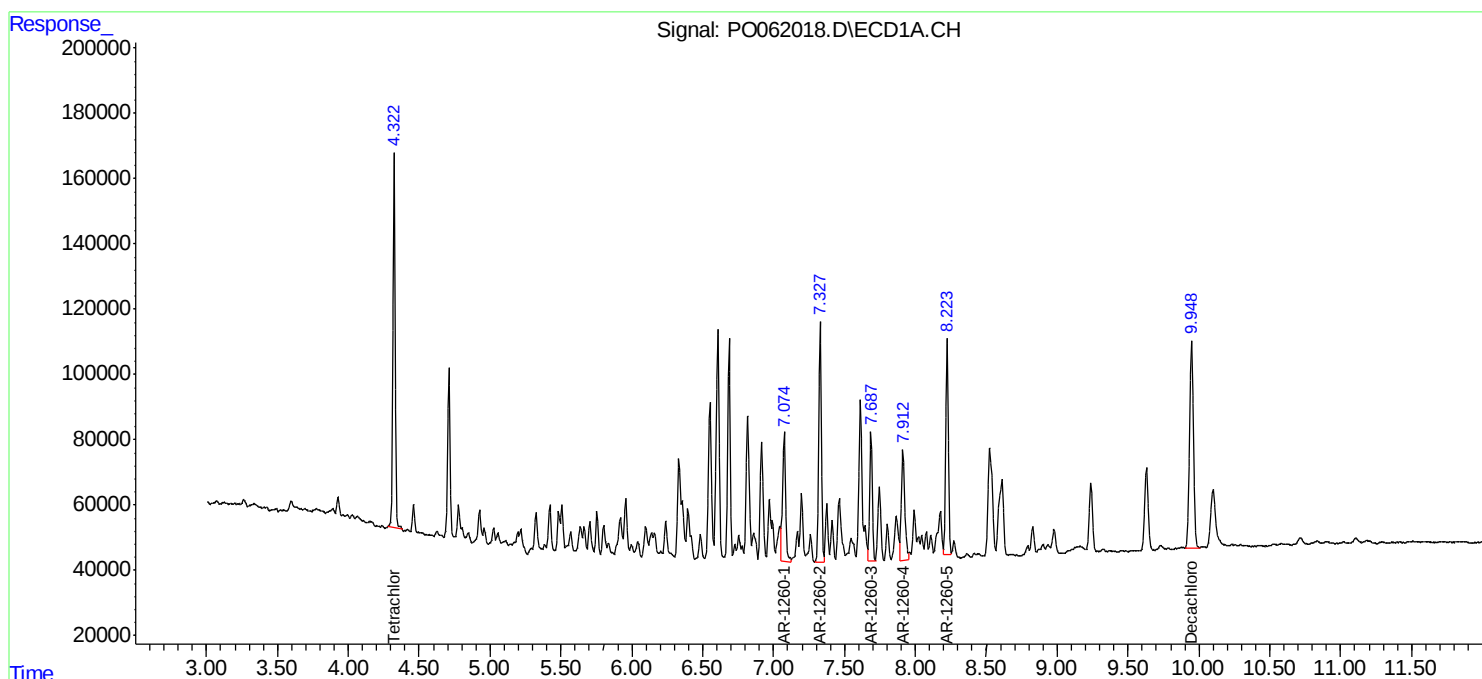

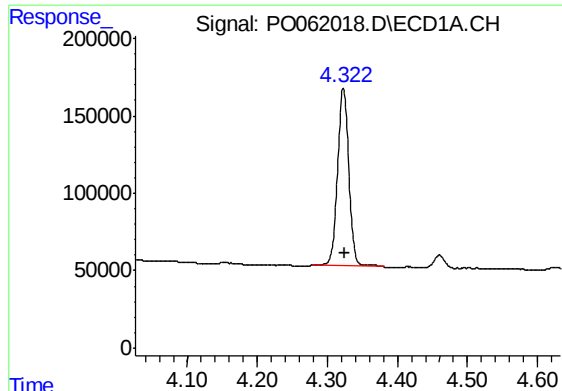


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.002 min
Response: 1281015
Conc: 20.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-31


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:47 PM

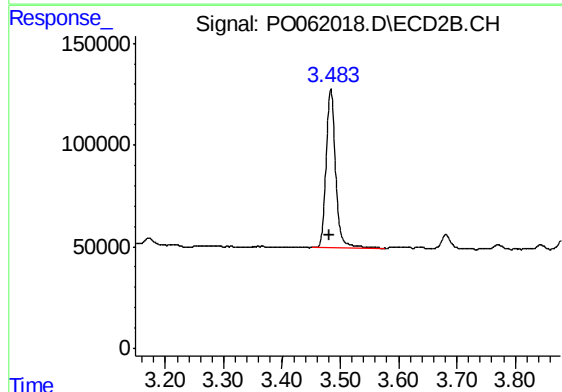


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.002 min
Response: 885060
Conc: 20.64 ng/ml

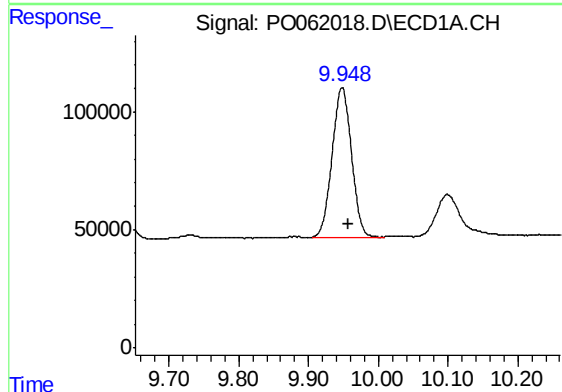


#2 Decachlorobiphenyl

R.T.: 9.948 min
Delta R.T.: -0.008 min
Response: 1223254
Conc: 21.86 ng/ml

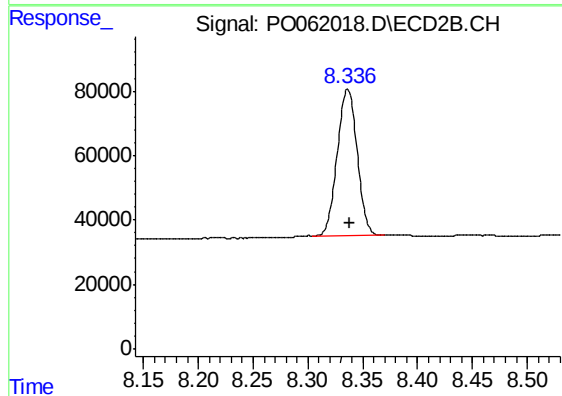

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.002 min
Response: 575701
Conc: 19.62 ng/ml

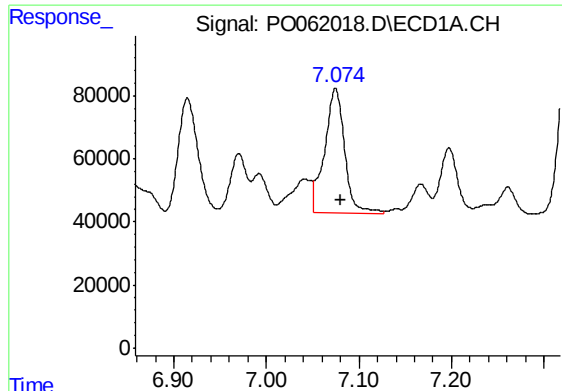


#31 AR-1260-1

R.T.: 7.075 min
Delta R.T.: -0.005 min
Response: 598324
Conc: 210.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-31


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:47 PM

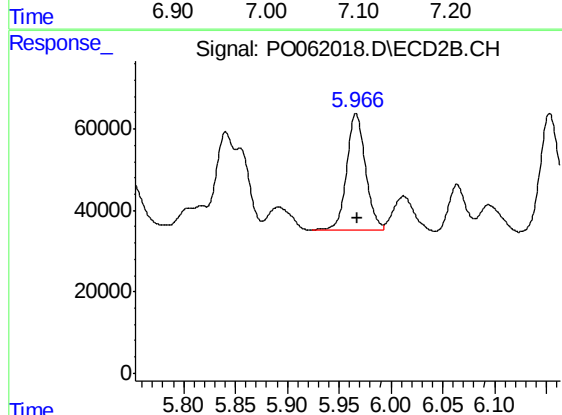


#31 AR-1260-1

R.T.: 5.966 min
Delta R.T.: -0.002 min
Response: 361790
Conc: 170.28 ng/ml

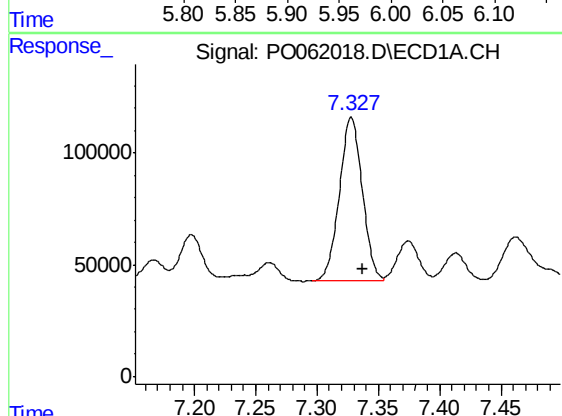


#32 AR-1260-2

R.T.: 7.327 min
Delta R.T.: -0.009 min
Response: 955349
Conc: 278.48 ng/ml m

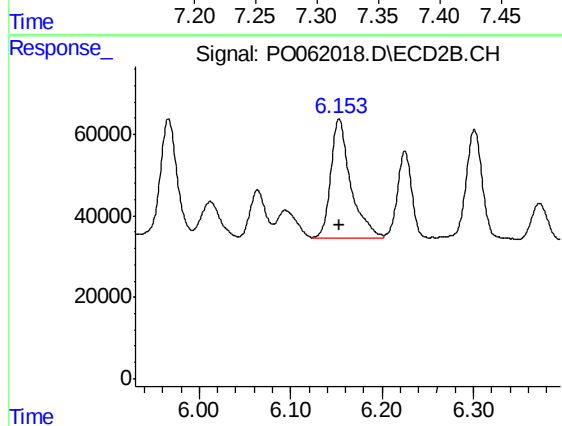

#32 AR-1260-2

R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 440331
Conc: 173.52 ng/ml

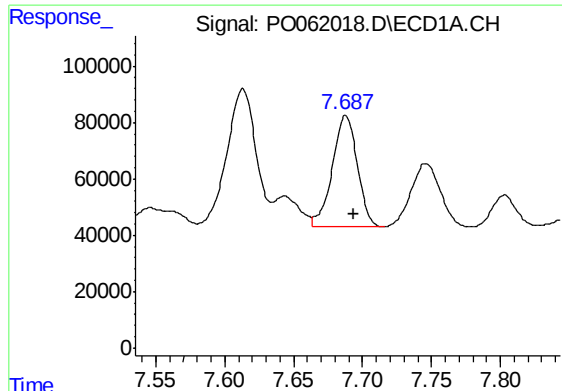


#33 AR-1260-3

R.T.: 7.688 min
Delta R.T.: -0.006 min
Response: 495933
Conc: 187.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-31


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:47 PM

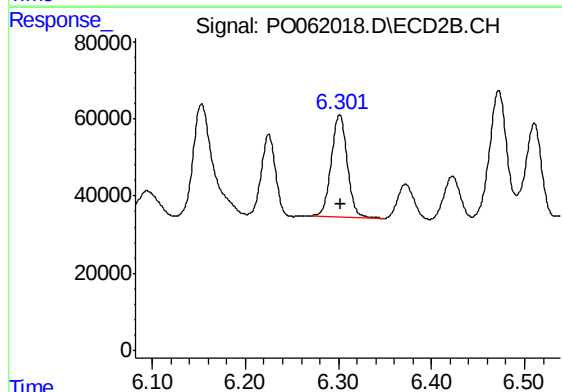


#33 AR-1260-3

R.T.: 6.301 min
Delta R.T.: -0.002 min
Response: 313992
Conc: 139.05 ng/ml

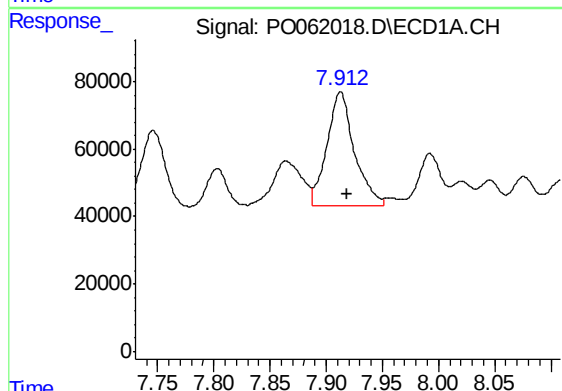


#34 AR-1260-4

R.T.: 7.912 min
Delta R.T.: -0.006 min
Response: 574190
Conc: 205.28 ng/ml m

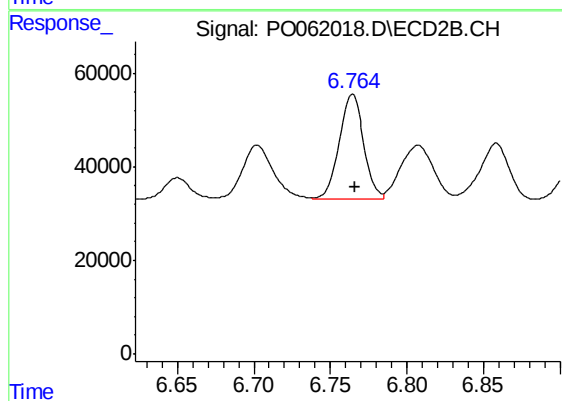

#34 AR-1260-4

R.T.: 6.764 min
Delta R.T.: -0.002 min
Response: 255396
Conc: 145.45 ng/ml

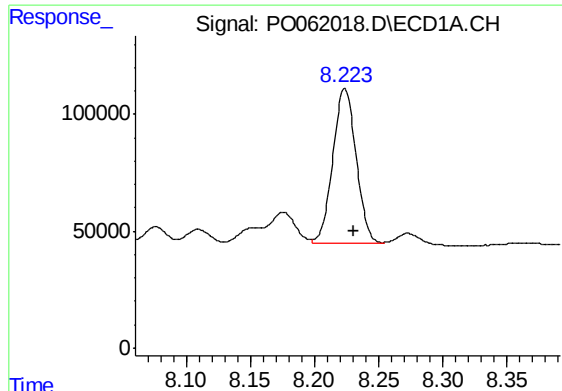


#35 AR-1260-5

R.T.: 8.223 min
Delta R.T.: -0.007 min
Response: 840605
Conc: 160.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-31

Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:47 PM

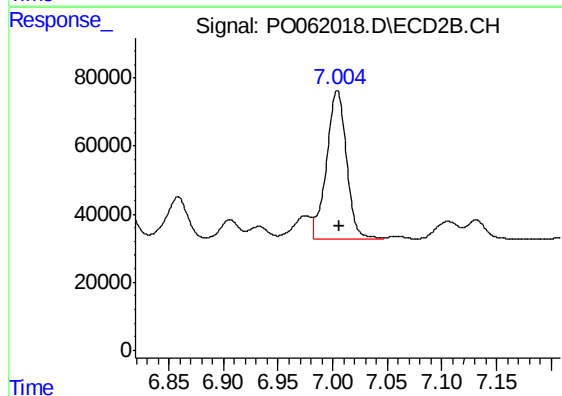

#35 AR-1260-5

R.T.: 7.004 min
Delta R.T.: -0.002 min
Response: 552271
Conc: 153.30 ng/ml