

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101519\
 Data File : P0062022.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2019 18:06
 Operator : HP/AJ
 Sample : K5355-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-33

Manual Integrations
 APPROVED

Ankita
 10/16/2019 12:01:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:08:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.322	3.482	1056455	777091	17.082	18.122
2)	SA Decachlor...	9.949	8.337	1030628	495345	18.420	16.882
Target Compounds							
31)	L7 AR-1260-1	7.074	5.966	245990	174779	86.399m	82.259
32)	L7 AR-1260-2	7.328	6.153	471822	220665	137.535m	86.957 #
33)	L7 AR-1260-3	7.688	6.301	201896	138891	76.299	61.508
34)	L7 AR-1260-4	7.912	6.764	278095	111677	99.424m	63.603 #
35)	L7 AR-1260-5	8.223	7.004	343332	265145	65.576m	73.601

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101519\
Data File : PO062022.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 18:06
Operator : HP/AJ
Sample : K5355-04
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
COMP-33


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:08:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

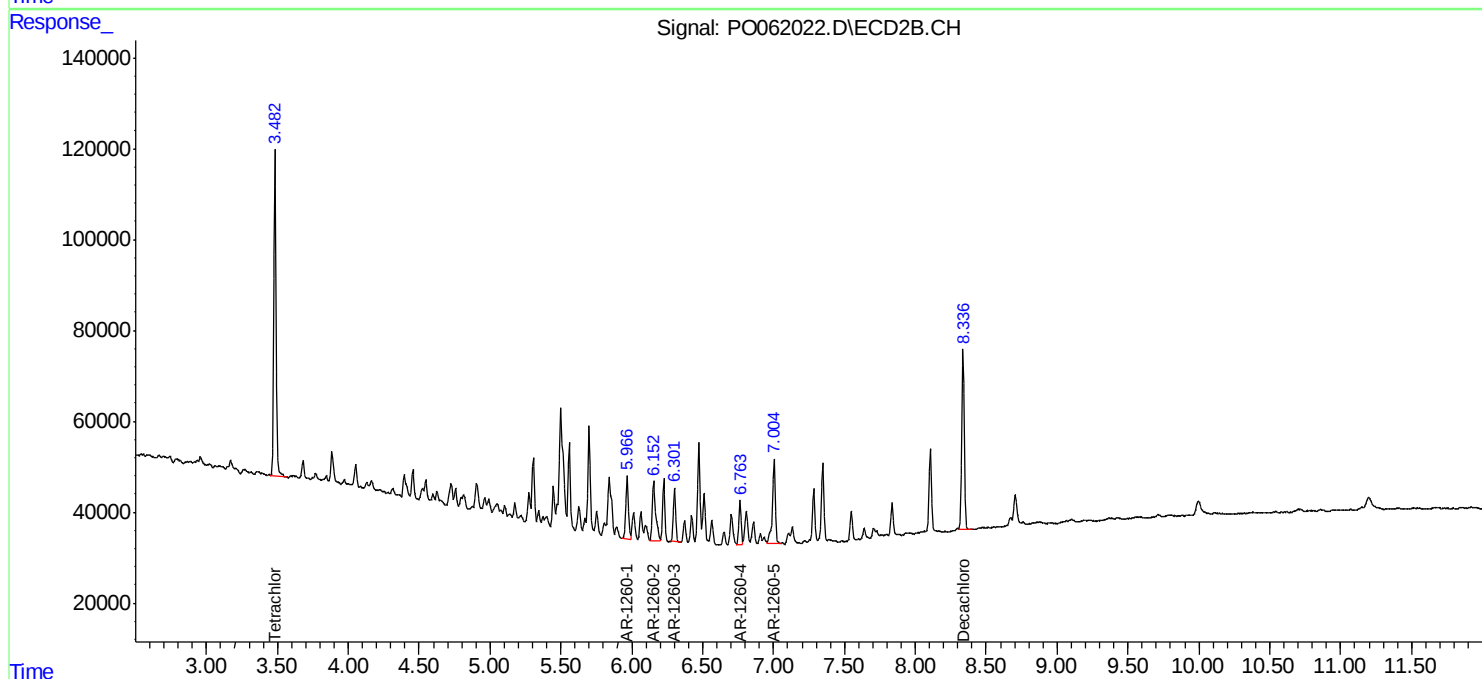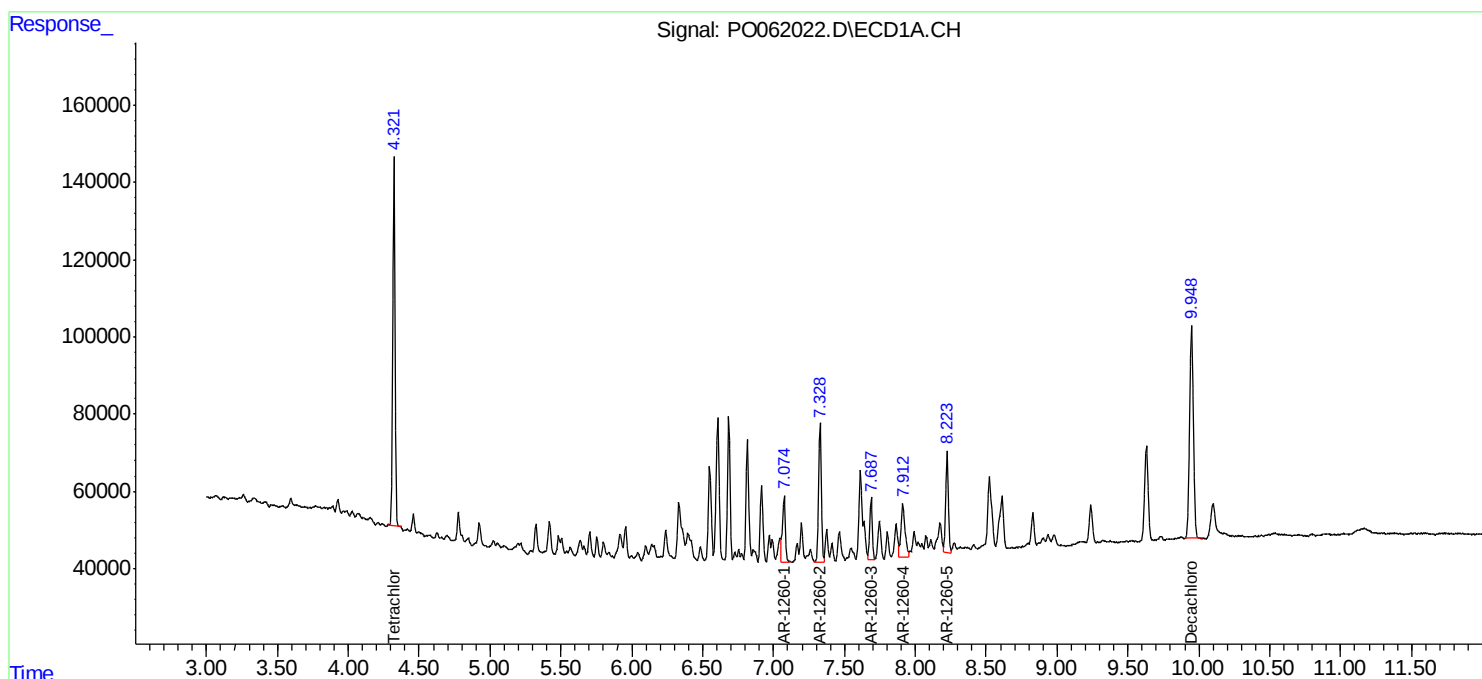

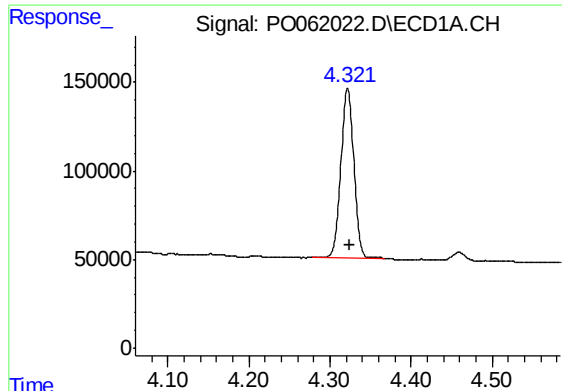


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.003 min
Response: 1056455
Conc: 17.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-33


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:54 PM

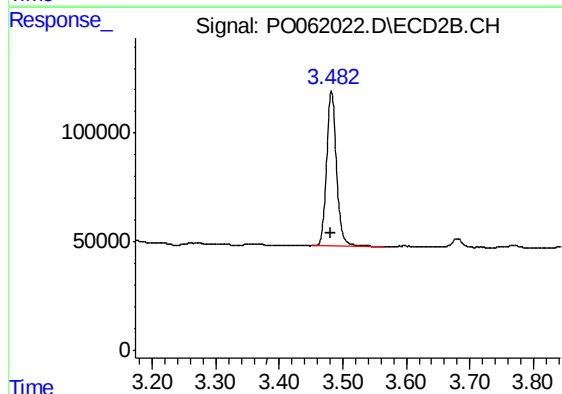


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 777091
Conc: 18.12 ng/ml

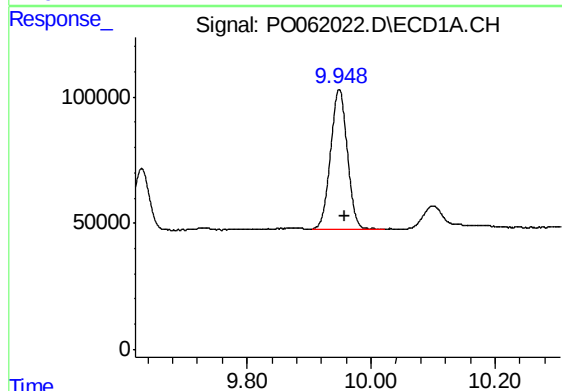


#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: -0.008 min
Response: 1030628
Conc: 18.42 ng/ml

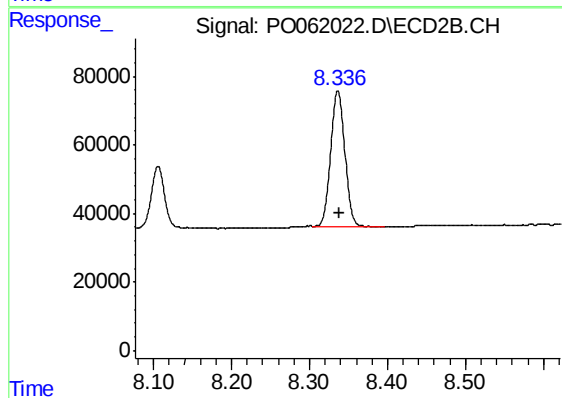

#2 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: -0.001 min
Response: 495345
Conc: 16.88 ng/ml

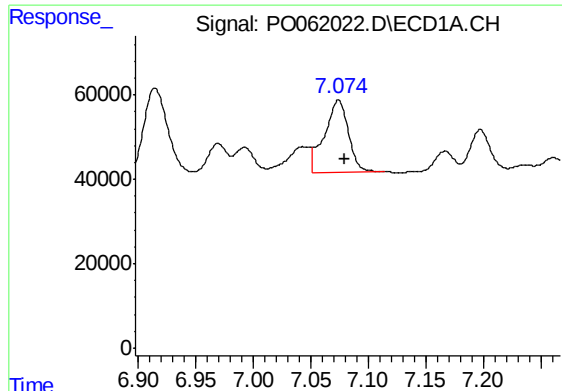


#31 AR-1260-1

R.T.: 7.074 min
Delta R.T.: -0.006 min
Response: 245990
Conc: 86.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-33


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:54 PM

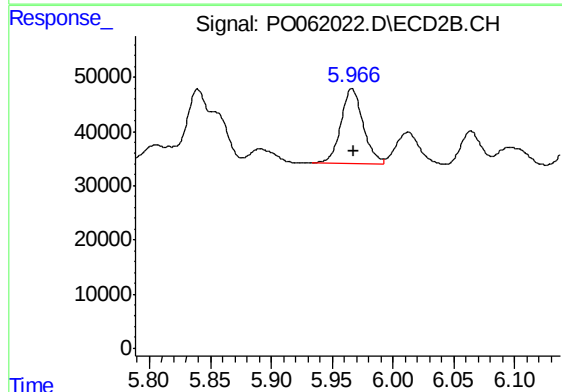


#31 AR-1260-1

R.T.: 5.966 min
Delta R.T.: -0.002 min
Response: 174779
Conc: 82.26 ng/ml

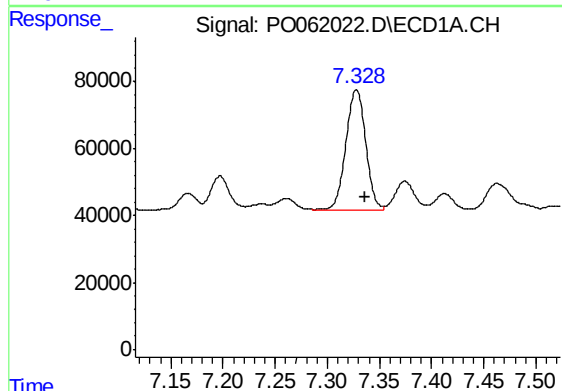


#32 AR-1260-2

R.T.: 7.328 min
Delta R.T.: -0.009 min
Response: 471822
Conc: 137.54 ng/ml m

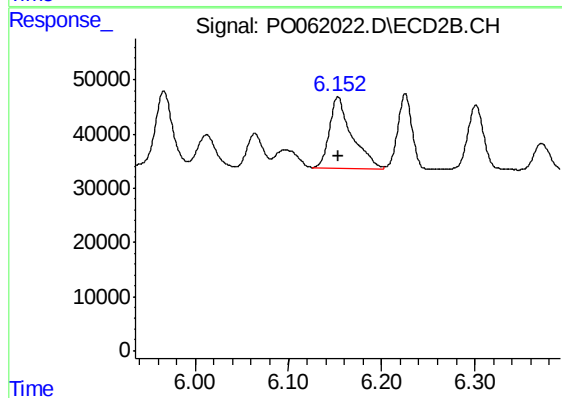

#32 AR-1260-2

R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 220665
Conc: 86.96 ng/ml

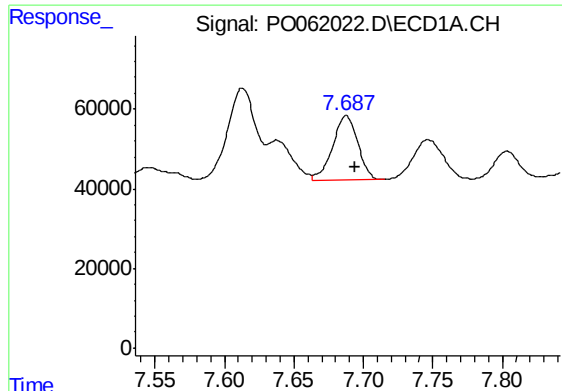


#33 AR-1260-3

R.T.: 7.688 min
Delta R.T.: -0.006 min
Response: 201896
Conc: 76.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-33


Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:54 PM

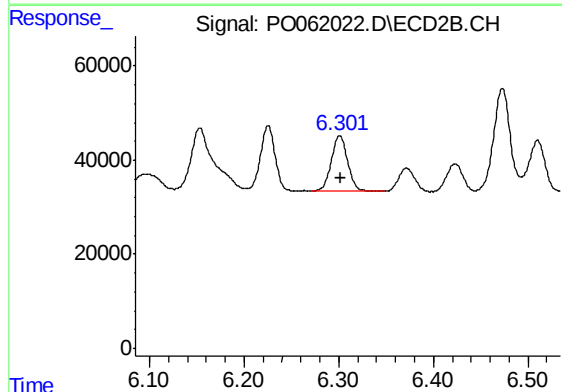


#33 AR-1260-3

R.T.: 6.301 min
Delta R.T.: -0.002 min
Response: 138891
Conc: 61.51 ng/ml

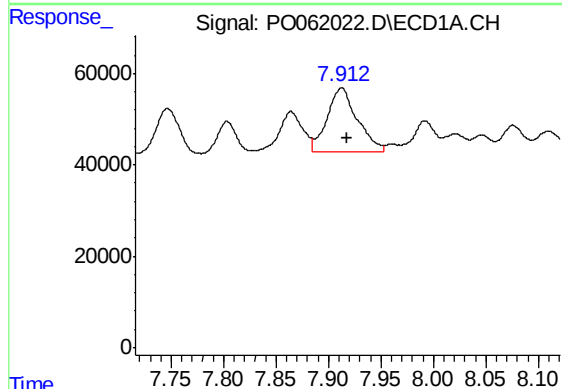


#34 AR-1260-4

R.T.: 7.912 min
Delta R.T.: -0.006 min
Response: 278095
Conc: 99.42 ng/ml m

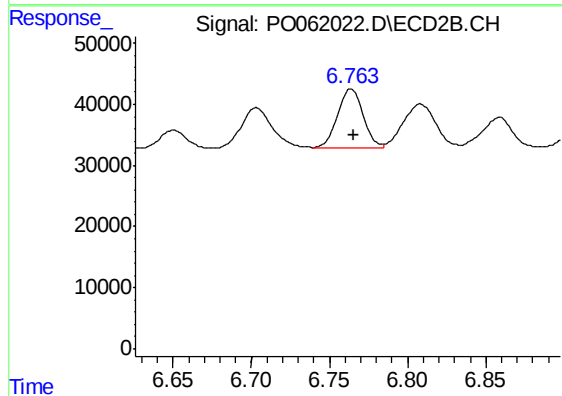

#34 AR-1260-4

R.T.: 6.764 min
Delta R.T.: -0.002 min
Response: 111677
Conc: 63.60 ng/ml

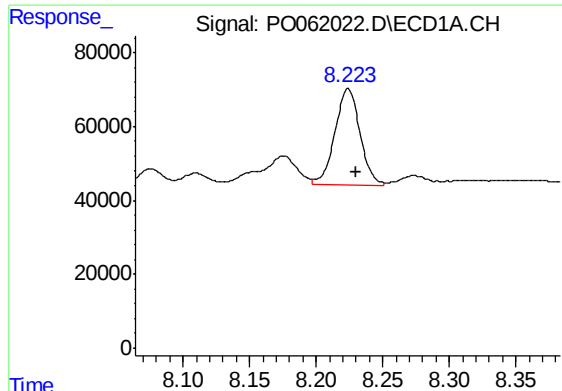


#35 AR-1260-5

R.T.: 8.223 min
Delta R.T.: -0.007 min
Response: 343332
Conc: 65.58 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-33

Manual Integrations
APPROVED

Ankita
10/16/2019 12:01:54 PM

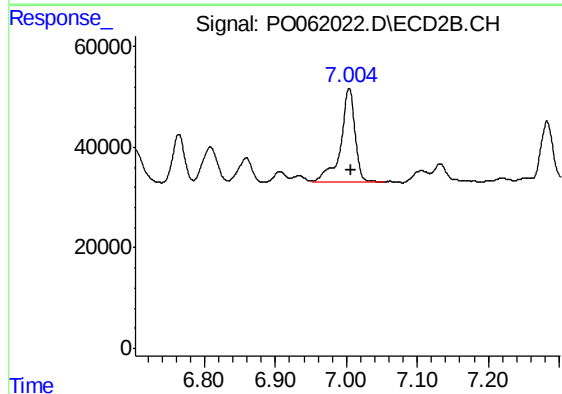

#35 AR-1260-5

R.T.: 7.004 min
Delta R.T.: -0.002 min
Response: 265145
Conc: 73.60 ng/ml