

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101519\
 Data File : P0062028.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2019 19:44
 Operator : HP/AJ
 Sample : K5334-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-2-PIT-COMPOSITE

Manual Integrations
 APPROVED

Ankita
 10/16/2019 2:44:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:10:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.478	1198673	1685519	19.381m	39.306m#
2) SA Decachlor...	9.963	8.354	712964	386903	12.742m	13.186m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101519\
Data File : PO062028.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2019 19:44
Operator : HP/AJ
Sample : K5334-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S-2-PIT-COMPOSITE


Manual Integrations
APPROVED

Ankita
10/16/2019 2:44:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:10:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

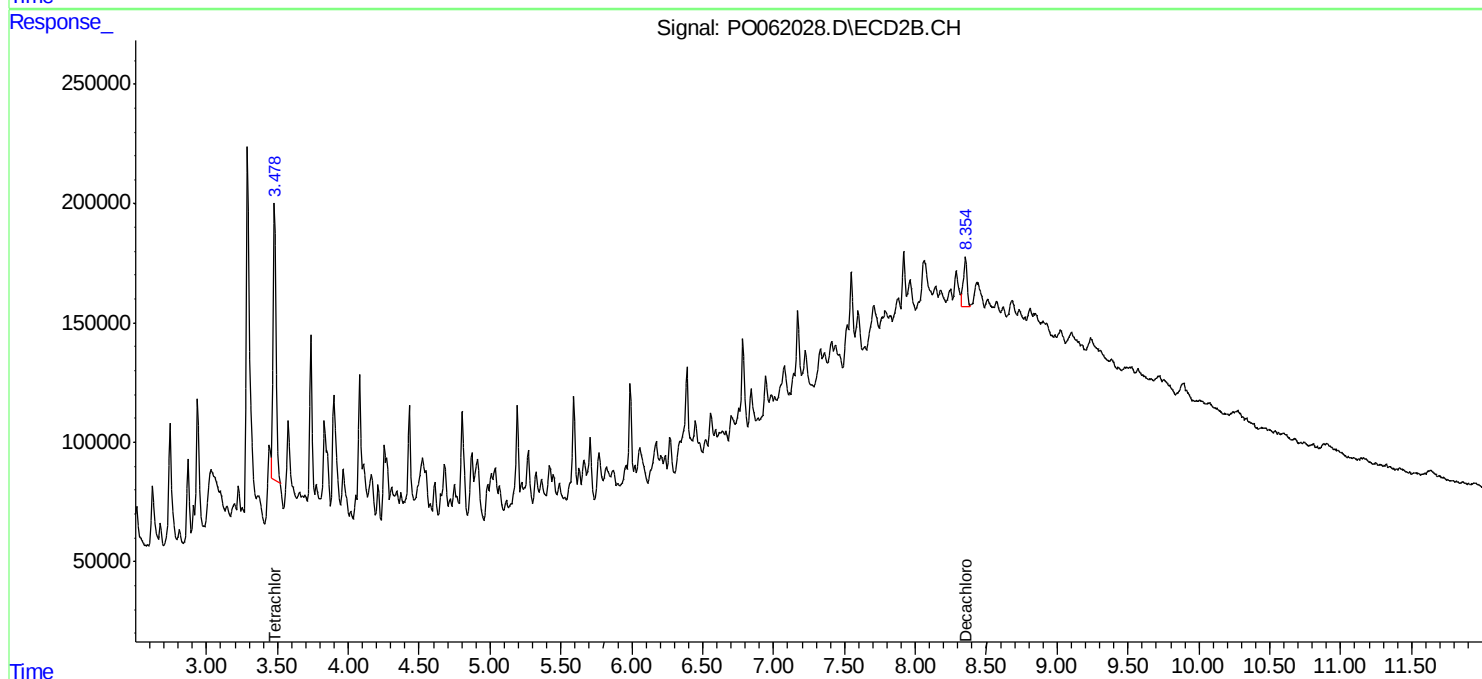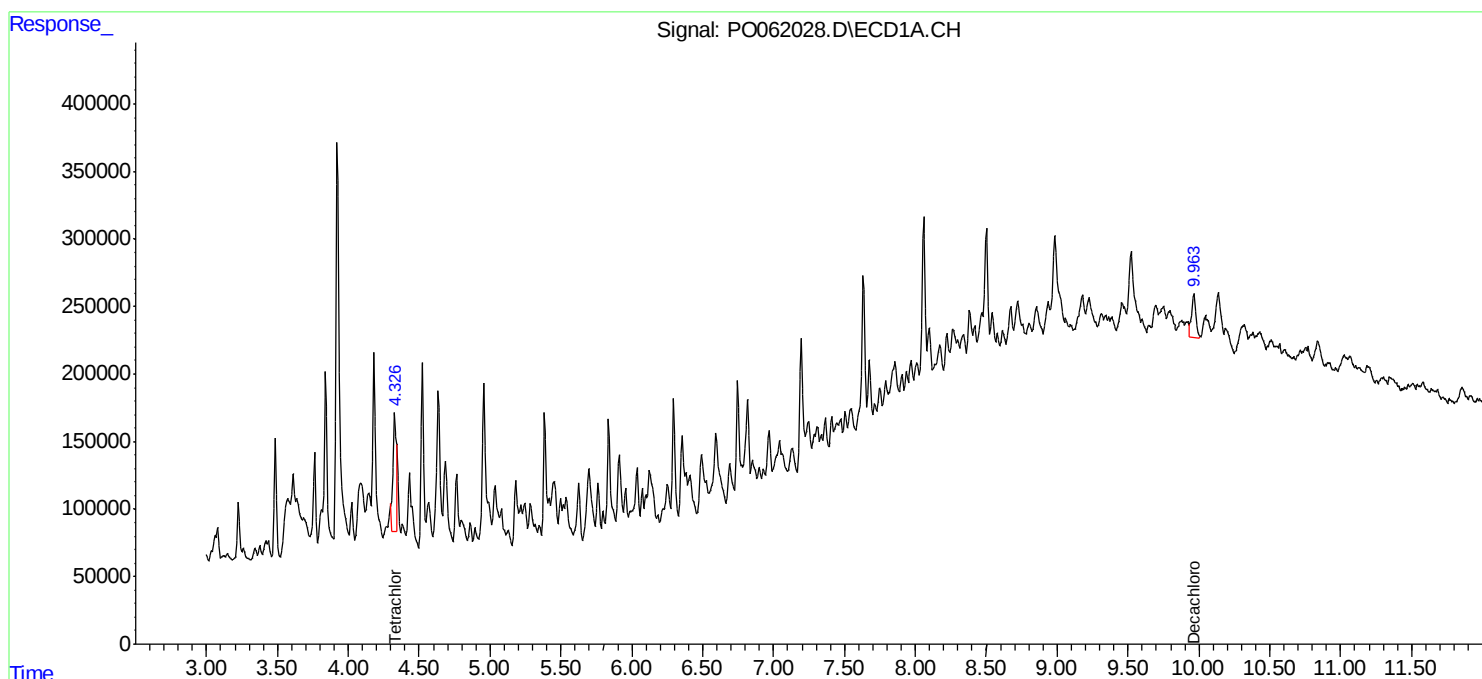

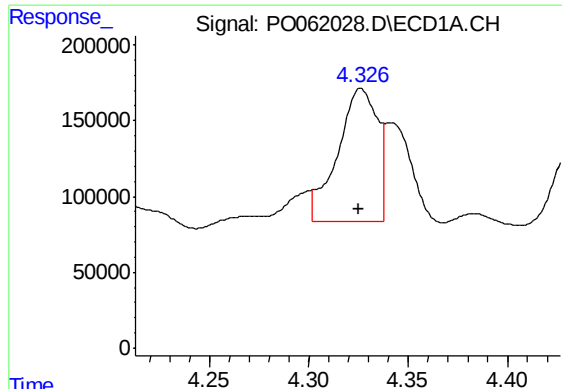


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 1198673
Conc: 19.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S-2-PIT-COMPOSITE


Manual Integrations
APPROVED

Ankita
10/16/2019 2:44:47 PM

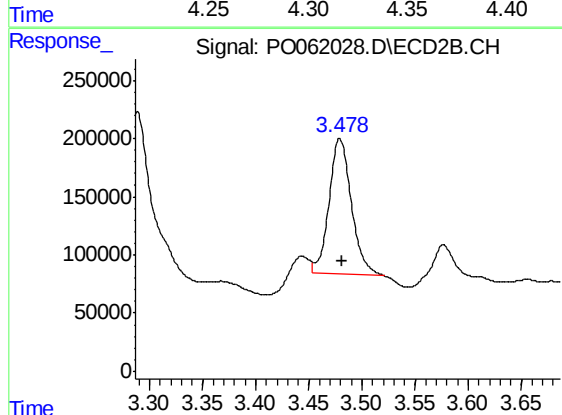


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: -0.003 min
Response: 1685519
Conc: 39.31 ng/ml m

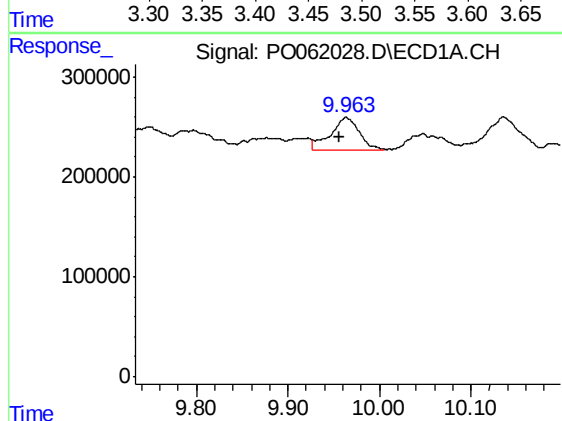

#2 Decachlorobiphenyl

R.T.: 9.963 min
Delta R.T.: 0.006 min
Response: 712964
Conc: 12.74 ng/ml m

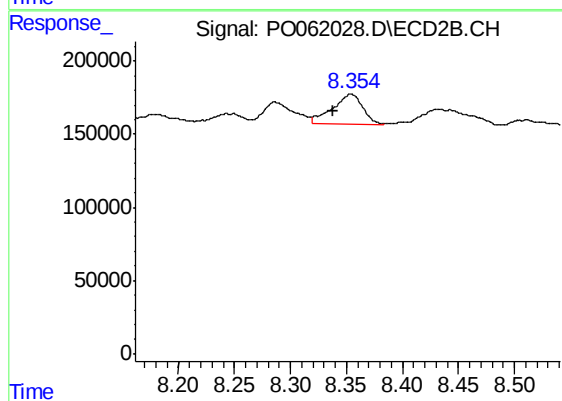

#2 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: 0.016 min
Response: 386903
Conc: 13.19 ng/ml m