

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0101719\  
Data File : P0063000.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 17 Oct 2019 16:58  
Operator : HP/AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 18 04:55:19 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0101119.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Oct 12 06:25:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|---------|--------|--------|--------|
| -----                       |                 |       |       |         |        |        |        |
| System Monitoring Compounds |                 |       |       |         |        |        |        |
| 1)                          | SA Tetrachlo... | 4.324 | 3.483 | 1251984 | 848911 | 20.243 | 19.797 |
| 2)                          | SA Decachlor... | 9.959 | 8.339 | 1289075 | 691164 | 23.039 | 23.556 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO101719\  
Data File : PO063000.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 17 Oct 2019 16:58  
Operator : HP/AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 18 04:55:19 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101119.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Oct 12 06:25:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

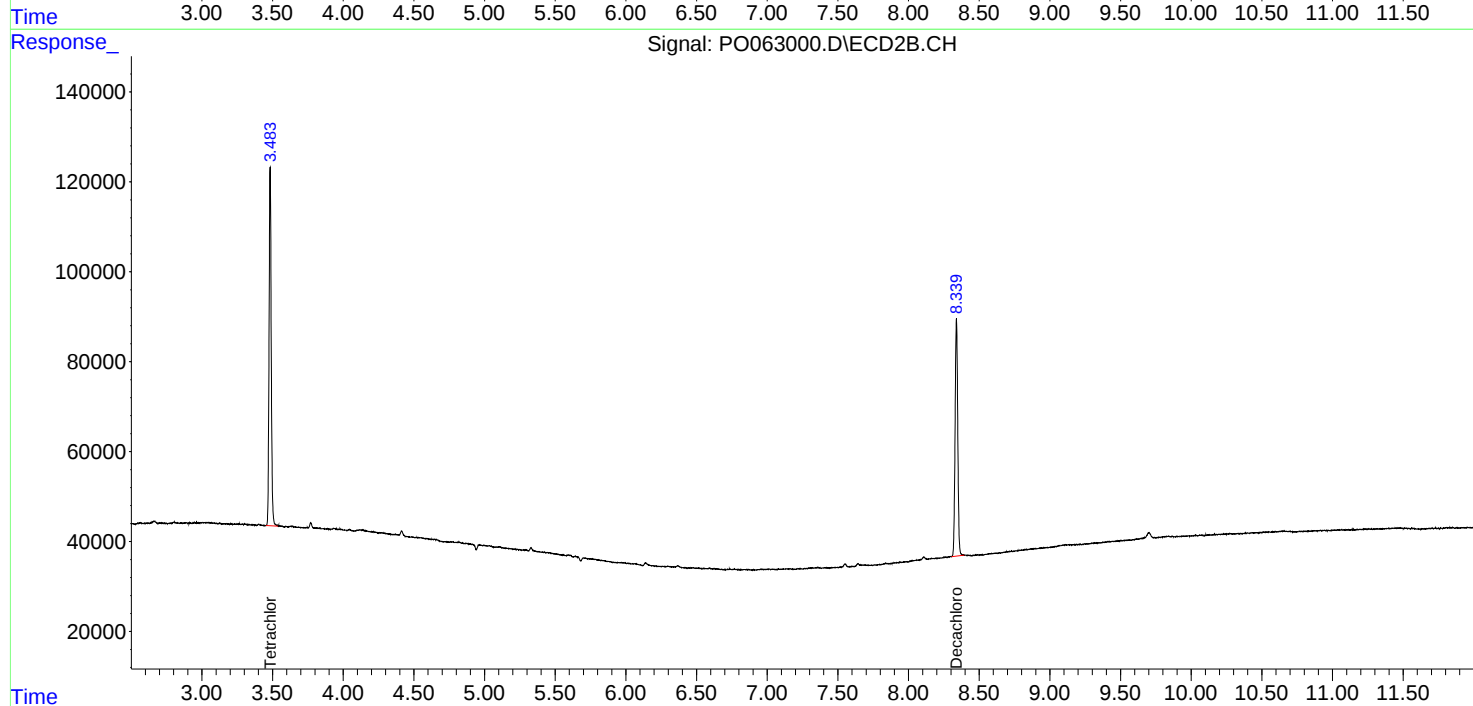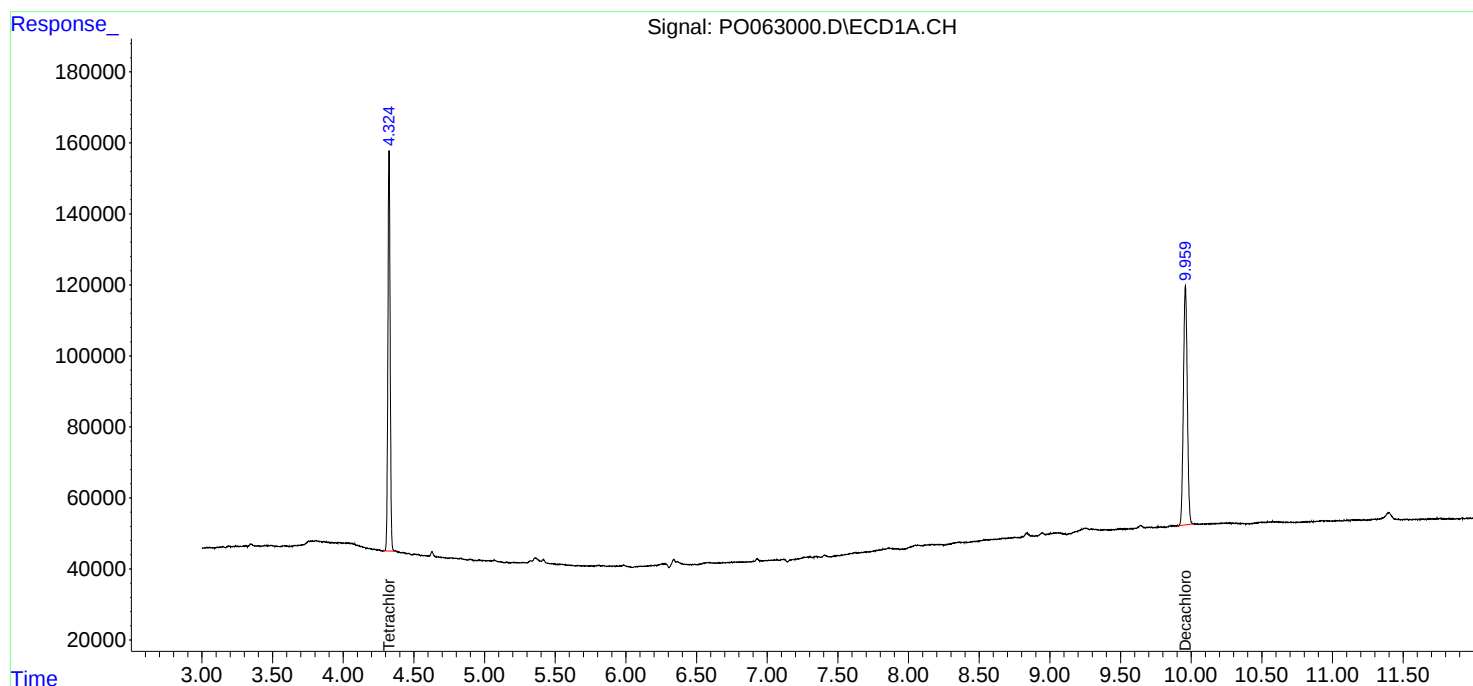


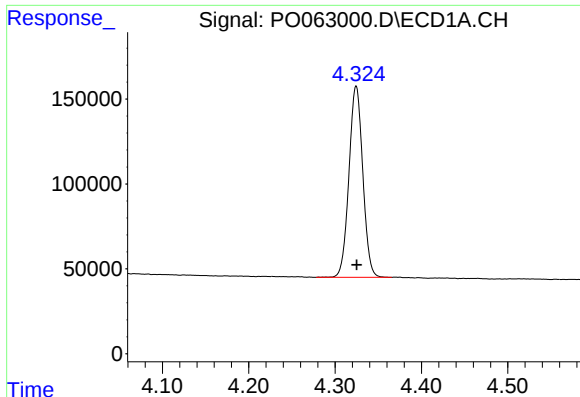

#1 Tetrachloro-m-xylene


R.T.: 4.324 min  
Delta R.T.: 0.000 min  
Response: 1251984  
Conc: 20.24 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :

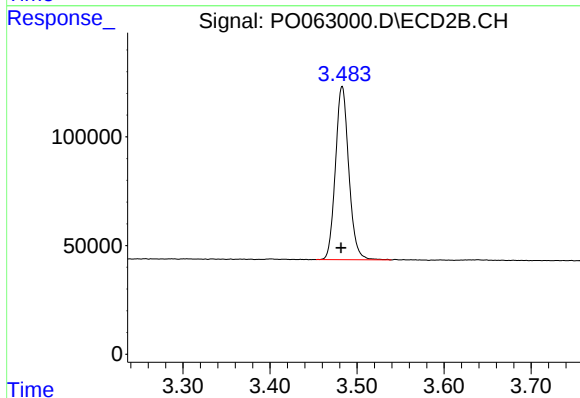


#1 Tetrachloro-m-xylene

R.T.: 3.483 min  
Delta R.T.: 0.002 min  
Response: 848911  
Conc: 19.80 ng/ml

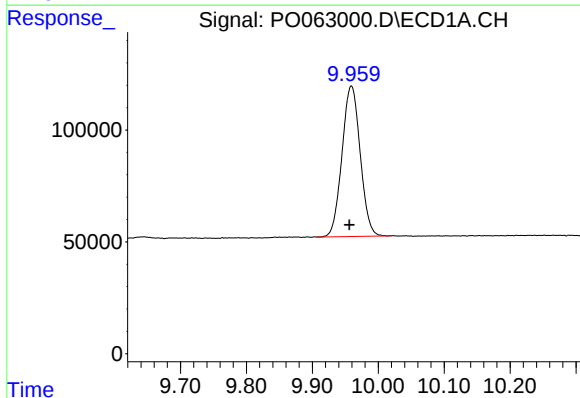

#2 Decachlorobiphenyl

R.T.: 9.959 min  
Delta R.T.: 0.003 min  
Response: 1289075  
Conc: 23.04 ng/ml

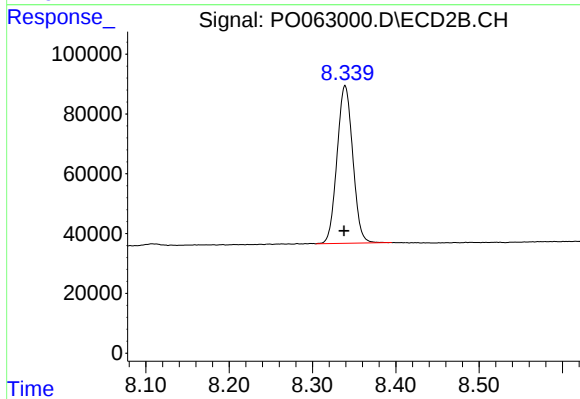

#2 Decachlorobiphenyl

R.T.: 8.339 min  
Delta R.T.: 0.001 min  
Response: 691164  
Conc: 23.56 ng/ml