

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101719\
 Data File : P0062095.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Oct 2019 15:36
 Operator : HP/AJ
 Sample : K5111-09
 Misc : AR1242 MDL-25 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/18/2019 5:49:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 04:53:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.325	3.483	1014285	713541	16.400	16.640
2)	SA Decachlor...	9.960	8.340	1121269	608617	20.040	20.743
Target Compounds							
16)	L4 AR-1242-1	5.488	4.529	50032	31741	27.000	26.392
17)	L4 AR-1242-2	5.510	4.546	70068	47291	26.414	26.550
18)	L4 AR-1242-3	5.570	4.714	46762	27346	28.633	28.723m
19)	L4 AR-1242-4	5.668	4.798	37316	21211	27.642m	22.468m
20)	L4 AR-1242-5	6.401	5.306	49278	26357	32.241	22.088 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101719\
Data File : PO062095.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2019 15:36
Operator : HP/AJ
Sample : K5111-09
Misc : AR1242 MDL-25 PPB
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 04:53:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

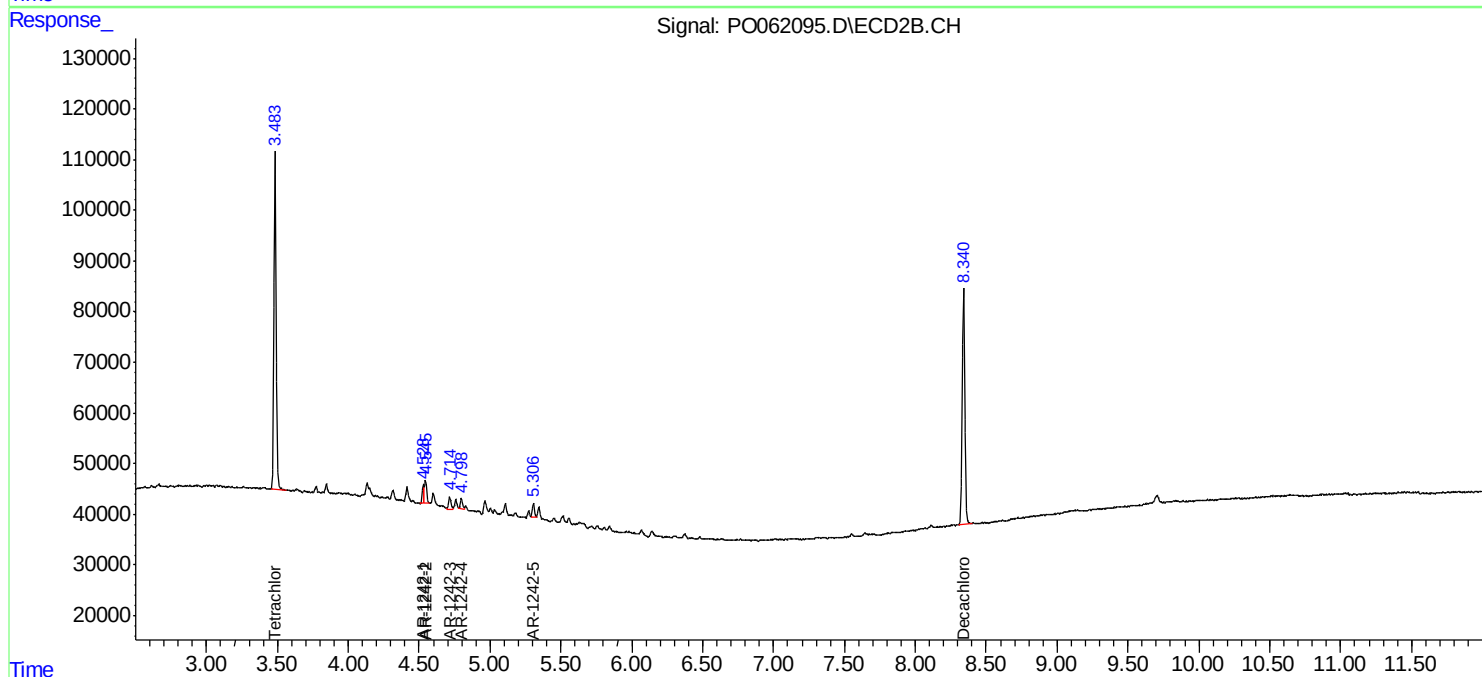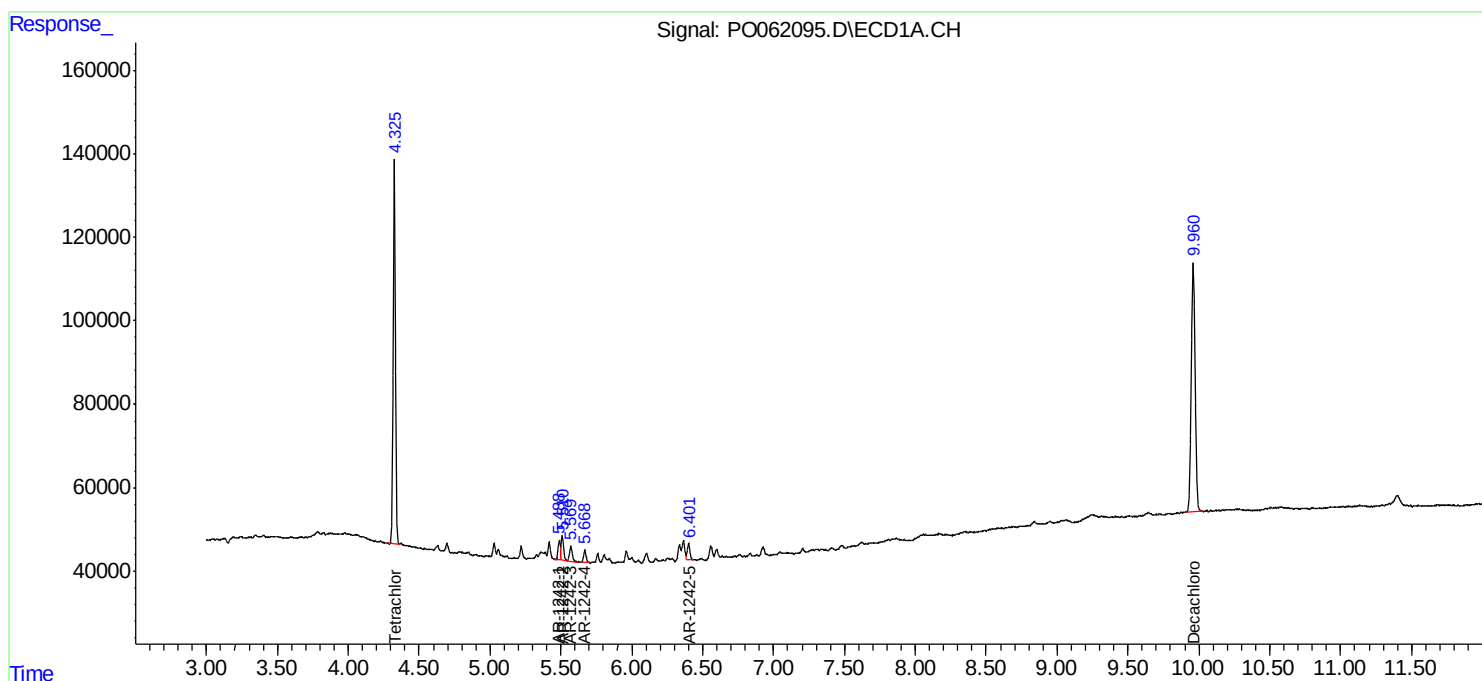

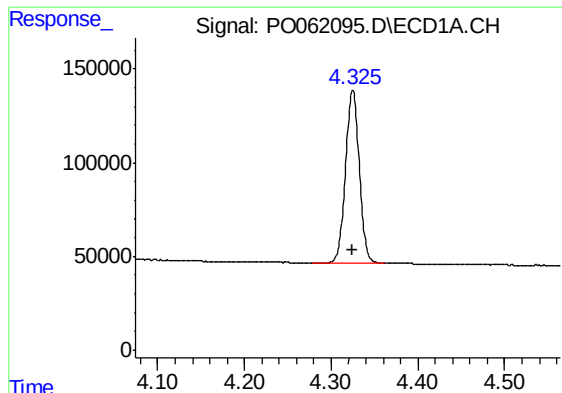


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 1014285
Conc: 16.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:04 PM

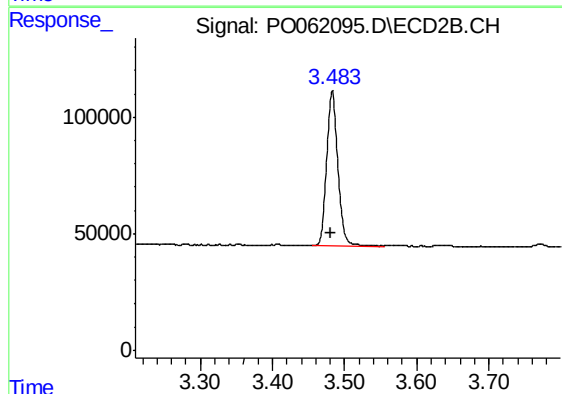


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.002 min
Response: 713541
Conc: 16.64 ng/ml

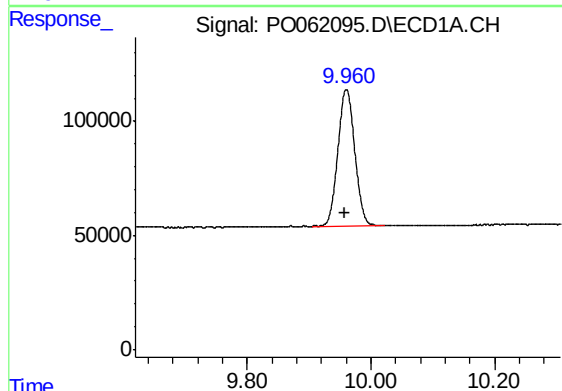


#2 Decachlorobiphenyl

R.T.: 9.960 min
Delta R.T.: 0.004 min
Response: 1121269
Conc: 20.04 ng/ml

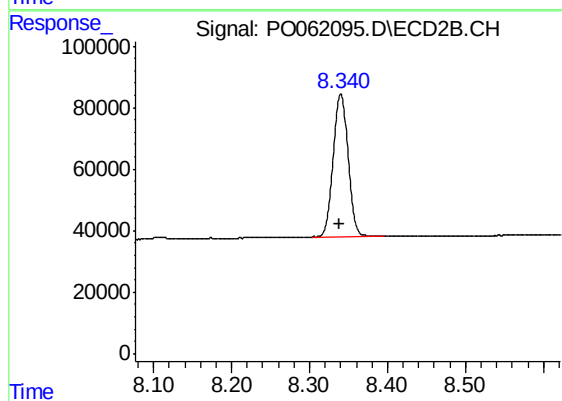

#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.002 min
Response: 608617
Conc: 20.74 ng/ml

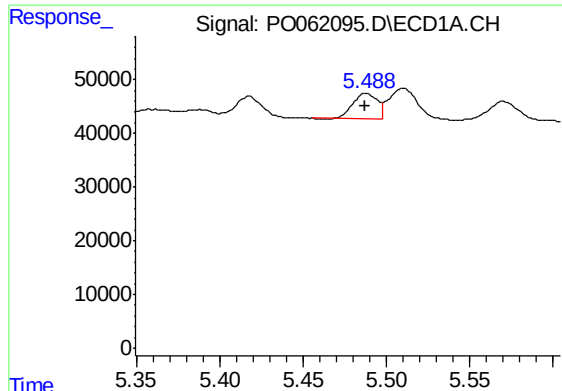


#16 AR-1242-1

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 50032
Conc: 27.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:04 PM

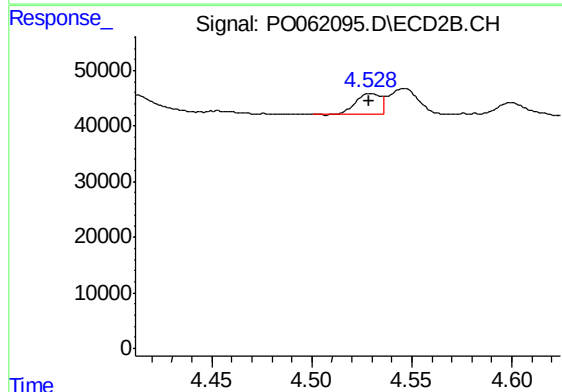


#16 AR-1242-1

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 31741
Conc: 26.39 ng/ml

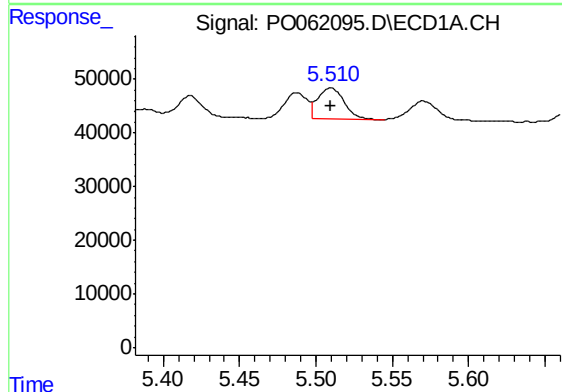


#17 AR-1242-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 70068
Conc: 26.41 ng/ml

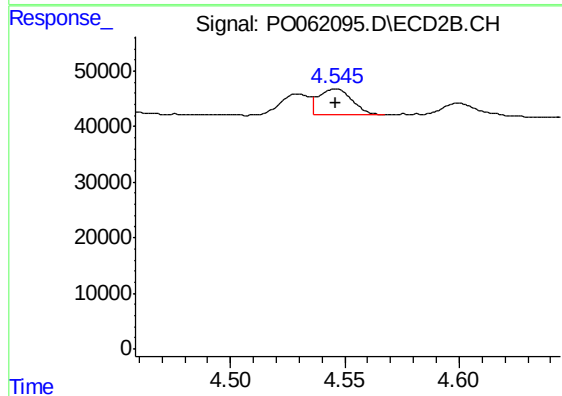

#17 AR-1242-2

R.T.: 4.546 min
Delta R.T.: 0.000 min
Response: 47291
Conc: 26.55 ng/ml

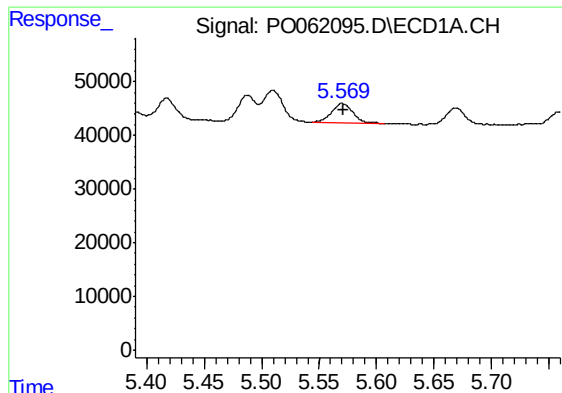


#18 AR-1242-3

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 46762
Conc: 28.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:04 PM

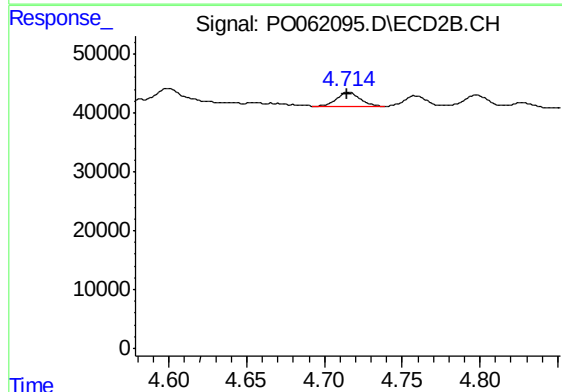


#18 AR-1242-3

R.T.: 4.714 min
Delta R.T.: -0.001 min
Response: 27346
Conc: 28.72 ng/ml m

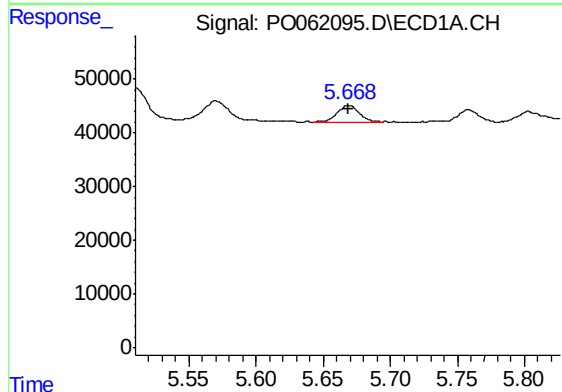


#19 AR-1242-4

R.T.: 5.668 min
Delta R.T.: -0.001 min
Response: 37316
Conc: 27.64 ng/ml m

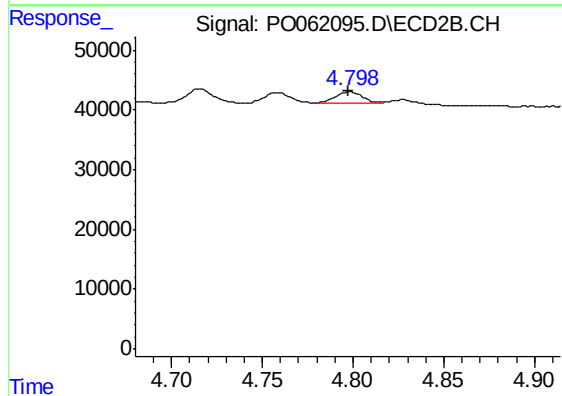

#19 AR-1242-4

R.T.: 4.798 min
Delta R.T.: 0.000 min
Response: 21211
Conc: 22.47 ng/ml m

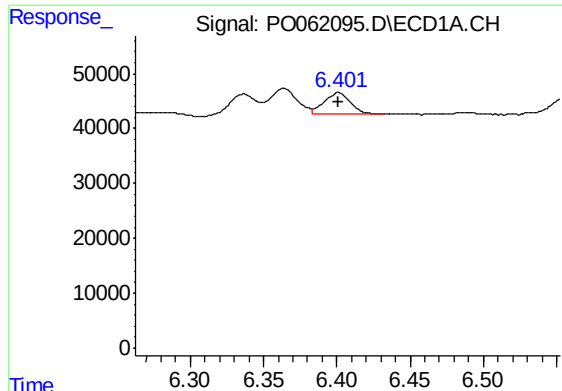


#20 AR-1242-5

R.T.: 6.401 min
Delta R.T.: 0.000 min
Response: 49278
Conc: 32.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019

Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:04 PM

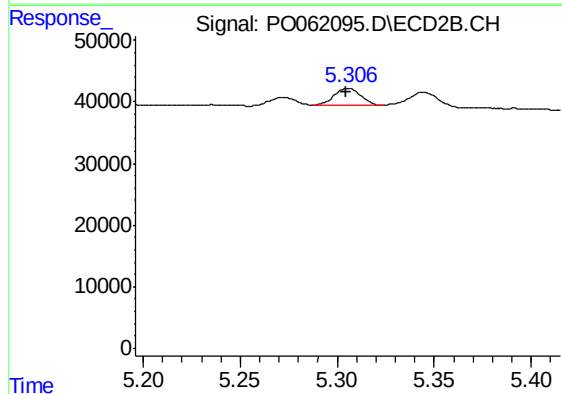

#20 AR-1242-5

R.T.: 5.306 min
Delta R.T.: 0.001 min
Response: 26357
Conc: 22.09 ng/ml