

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101719\
 Data File : P0062096.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Oct 2019 15:52
 Operator : HP/AJ
 Sample : K5111-09
 Misc : AR1248 MDL-25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/18/2019 5:49:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 04:53:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.483	1071044	757278	17.318	17.660
2)	SA Decachlor...	9.960	8.339	1188309	641537	21.238	21.865
Target Compounds							
21)	L5 AR-1248-1	5.486	4.529	37253	26976	25.992m	27.478
22)	L5 AR-1248-2	5.758	4.758	48875	32705	24.411	25.815
23)	L5 AR-1248-3	5.960	4.797	57870	28180	26.202m	21.228
24)	L5 AR-1248-4	6.363	4.963	95784	51636	37.494	32.632
25)	L5 AR-1248-5	6.401	5.344	77230	41951	31.585	27.258

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101719\
Data File : PO062096.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2019 15:52
Operator : HP/AJ
Sample : K5111-09
Misc : AR1248 MDL-25 PPB
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 04:53:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

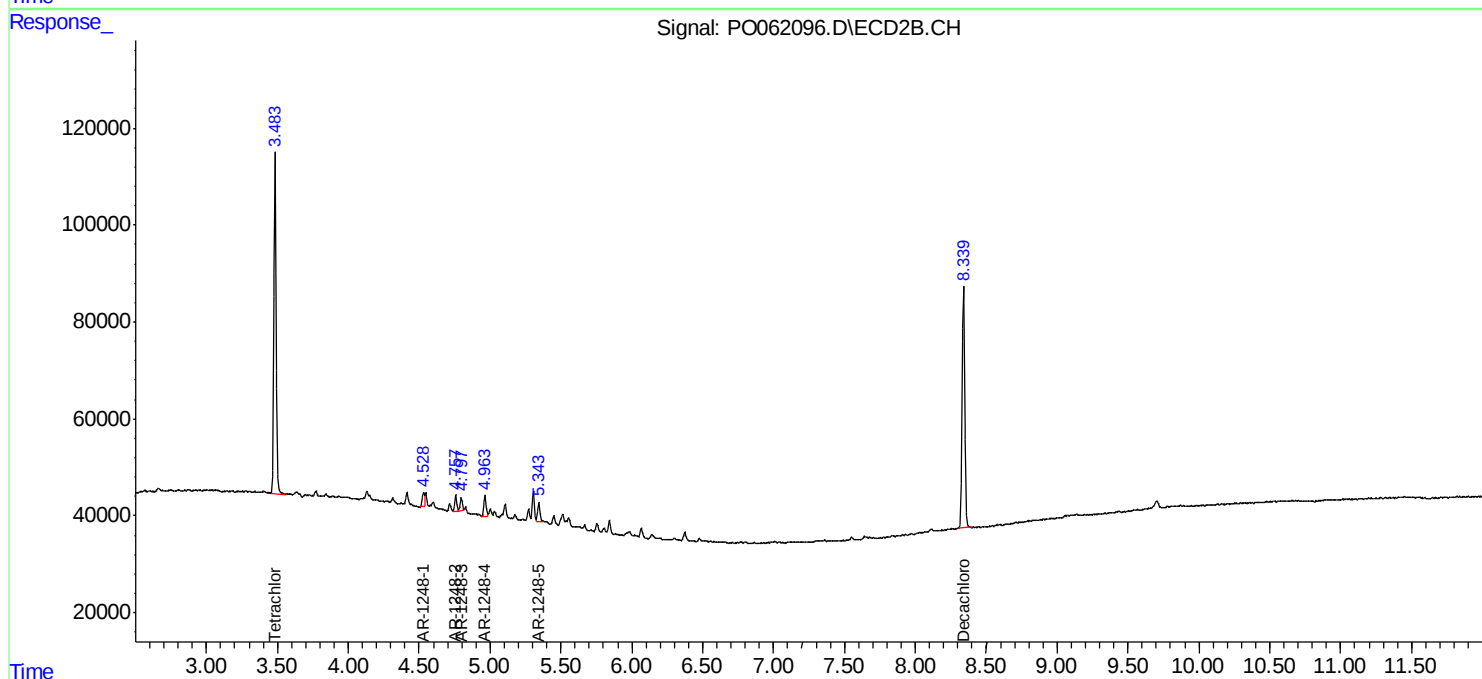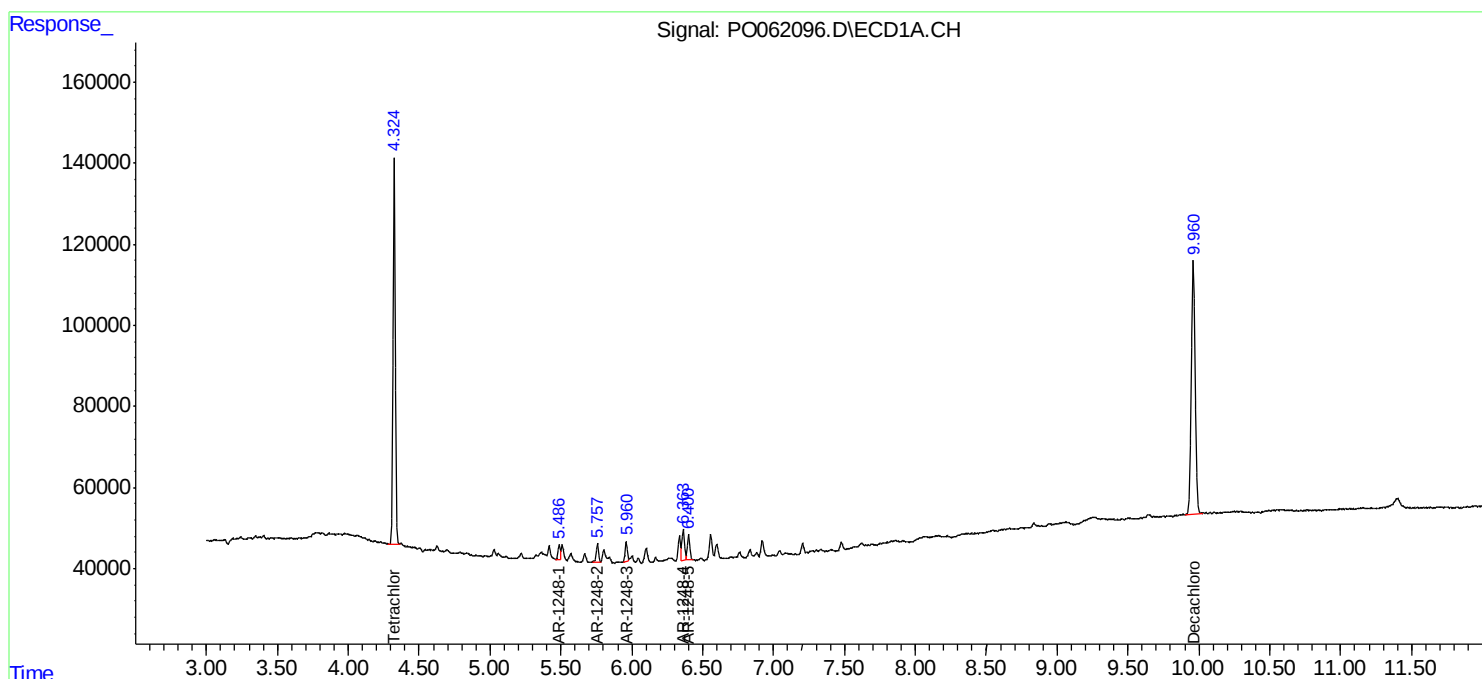

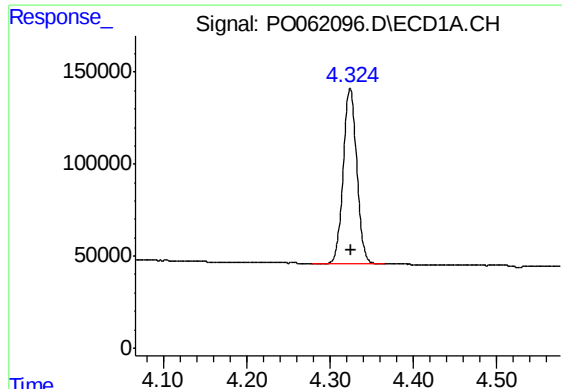


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: 0.000 min
Response: 1071044
Conc: 17.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:16 PM

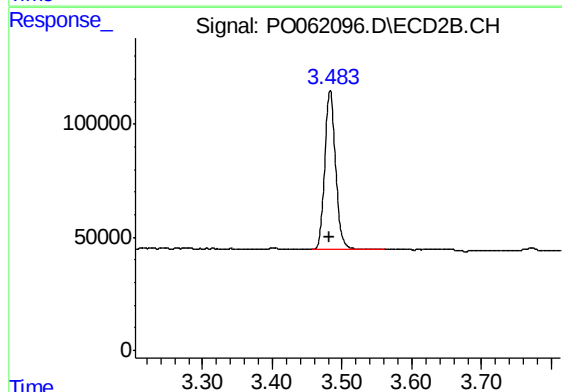


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.002 min
Response: 757278
Conc: 17.66 ng/ml

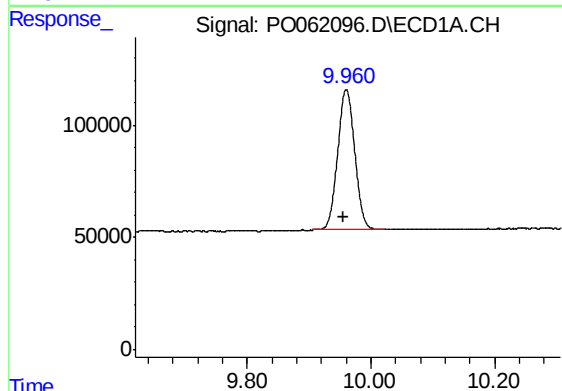


#2 Decachlorobiphenyl

R.T.: 9.960 min
Delta R.T.: 0.004 min
Response: 1188309
Conc: 21.24 ng/ml

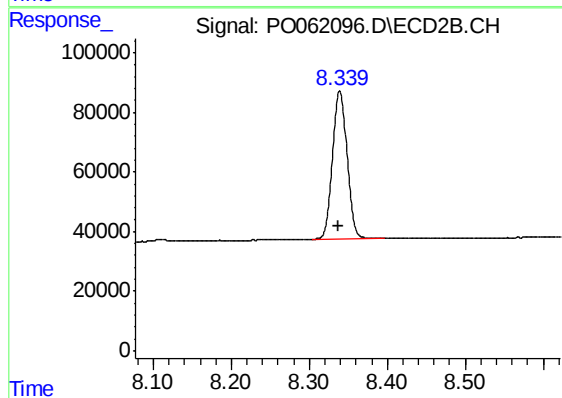

#2 Decachlorobiphenyl

R.T.: 8.339 min
Delta R.T.: 0.001 min
Response: 641537
Conc: 21.86 ng/ml

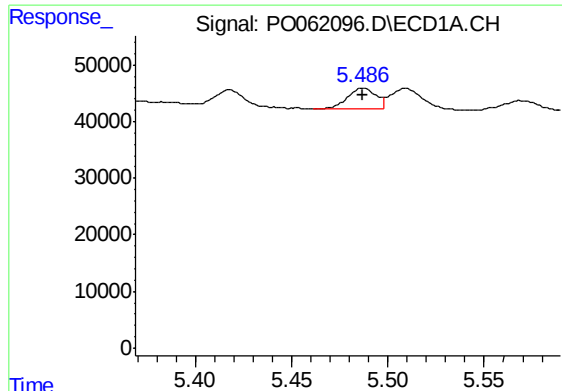


#21 AR-1248-1

R.T.: 5.486 min
Delta R.T.: -0.001 min
Response: 37253
Conc: 25.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:16 PM

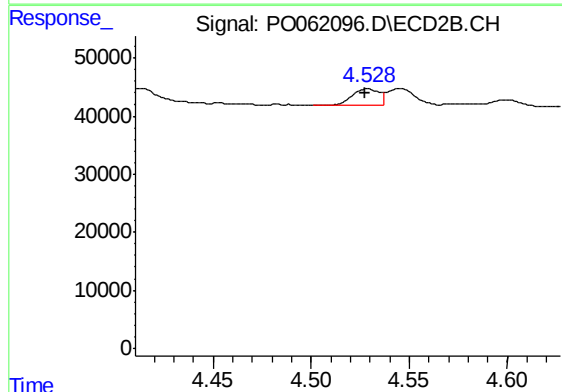


#21 AR-1248-1

R.T.: 4.529 min
Delta R.T.: 0.001 min
Response: 26976
Conc: 27.48 ng/ml

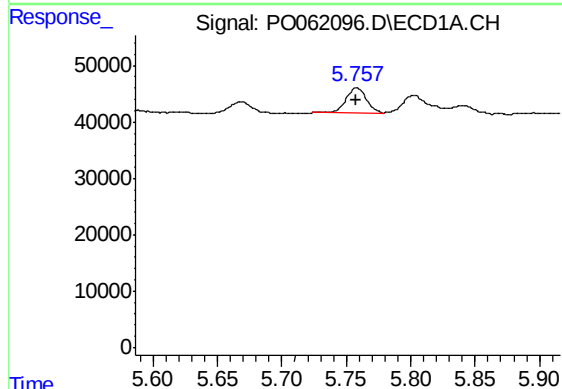


#22 AR-1248-2

R.T.: 5.758 min
Delta R.T.: 0.000 min
Response: 48875
Conc: 24.41 ng/ml

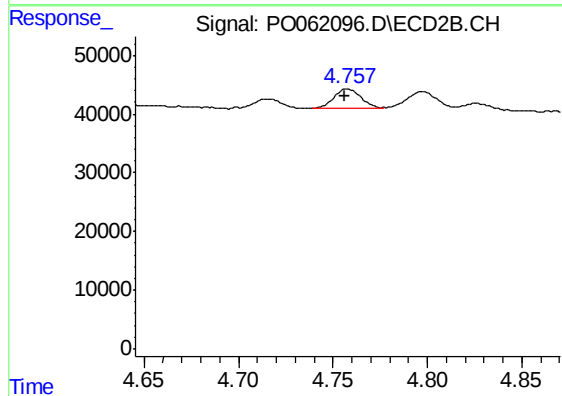

#22 AR-1248-2

R.T.: 4.758 min
Delta R.T.: 0.001 min
Response: 32705
Conc: 25.81 ng/ml

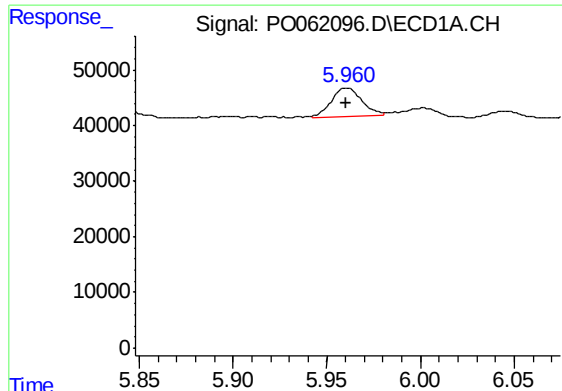


#23 AR-1248-3

R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 57870
Conc: 26.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:16 PM

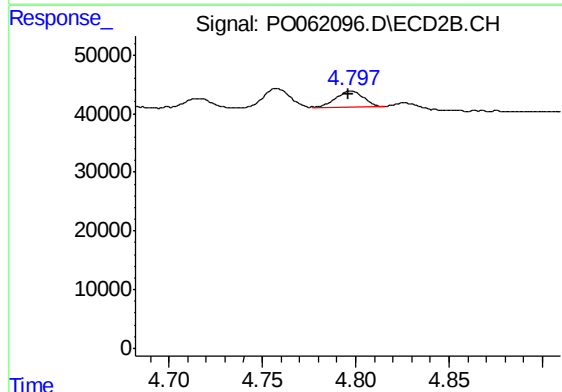


#23 AR-1248-3

R.T.: 4.797 min
Delta R.T.: 0.001 min
Response: 28180
Conc: 21.23 ng/ml

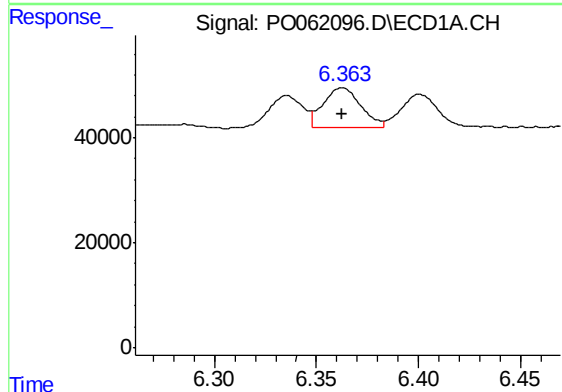


#24 AR-1248-4

R.T.: 6.363 min
Delta R.T.: 0.000 min
Response: 95784
Conc: 37.49 ng/ml

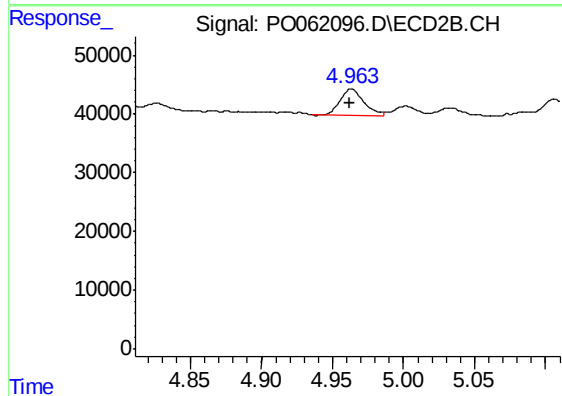

#24 AR-1248-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 51636
Conc: 32.63 ng/ml

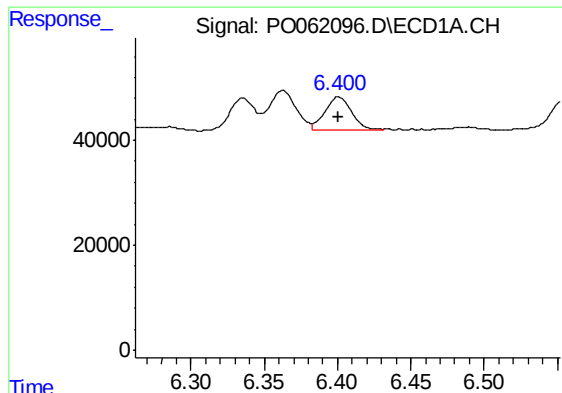


#25 AR-1248-5

R.T.: 6.401 min
Delta R.T.: 0.000 min
Response: 77230
Conc: 31.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019

Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:16 PM

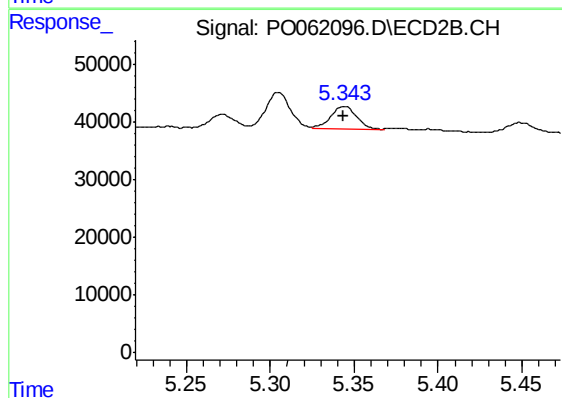

#25 AR-1248-5

R.T.: 5.344 min
Delta R.T.: 0.000 min
Response: 41951
Conc: 27.26 ng/ml