

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101719\
 Data File : P0062097.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Oct 2019 16:08
 Operator : HP/AJ
 Sample : K5111-09
 Misc : AR1254 MDL-25 PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/18/2019 5:49:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 04:54:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.483	964004	673804	15.587	15.713
2)	SA Decachlor...	9.959	8.339	1054464	575290	18.846	19.607
Target Compounds							
26)	L6 AR-1254-1	6.336	5.305	147667	67541	55.397m	27.615 #
27)	L6 AR-1254-2	6.552	5.449	127761	61899	31.249	29.227
28)	L6 AR-1254-3	6.919	5.842	157270	93228	37.588	28.614
29)	L6 AR-1254-4	7.203	6.066	101468	73969	33.673m	38.298
30)	L6 AR-1254-5	7.618	6.475	106323	82470	33.927m	31.225

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101719\
Data File : PO062097.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2019 16:08
Operator : HP/AJ
Sample : K5111-09
Misc : AR1254 MDL-25 PPB
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 04:54:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

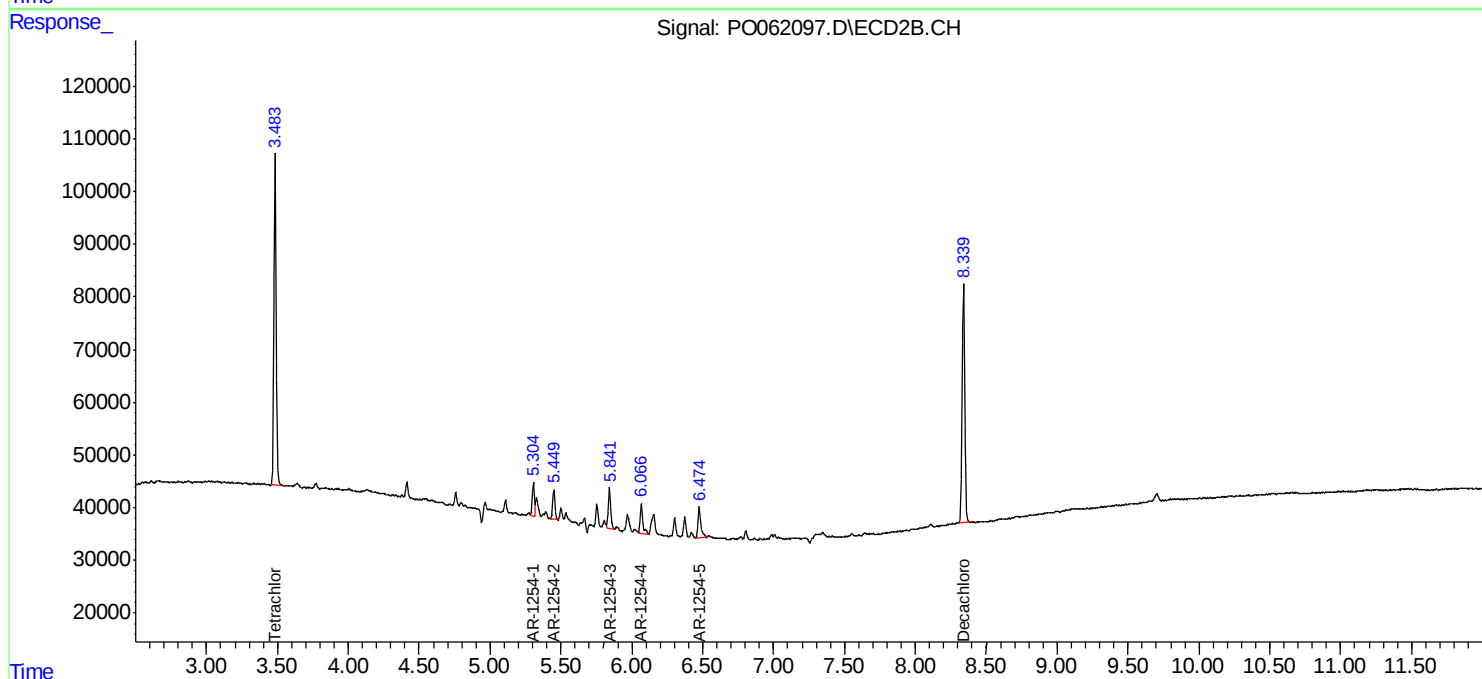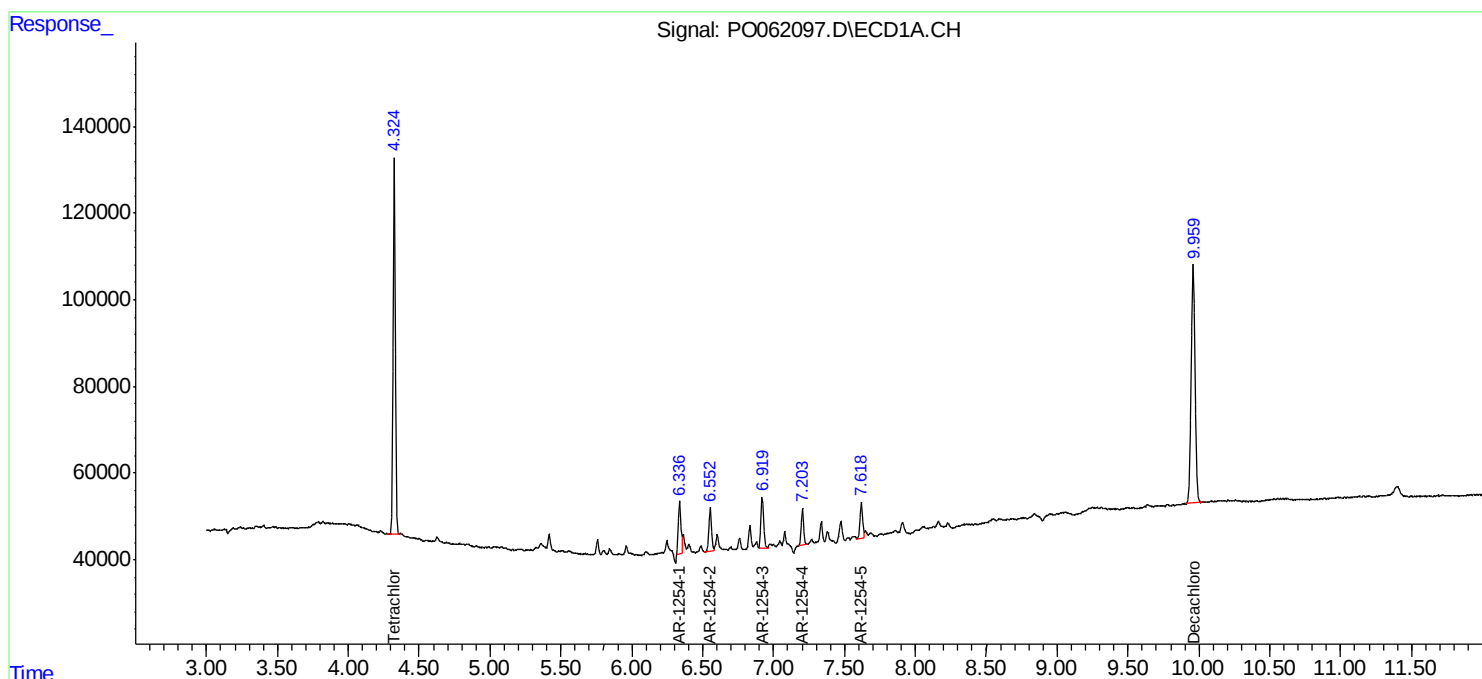

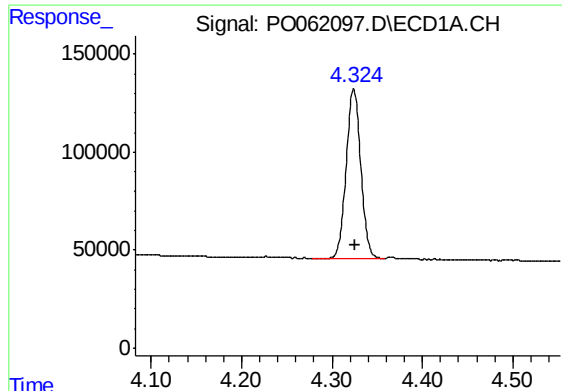


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: 0.000 min
Response: 964004
Conc: 15.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:18 PM

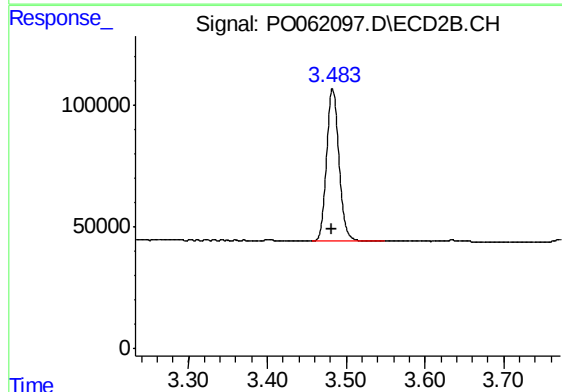


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.002 min
Response: 673804
Conc: 15.71 ng/ml

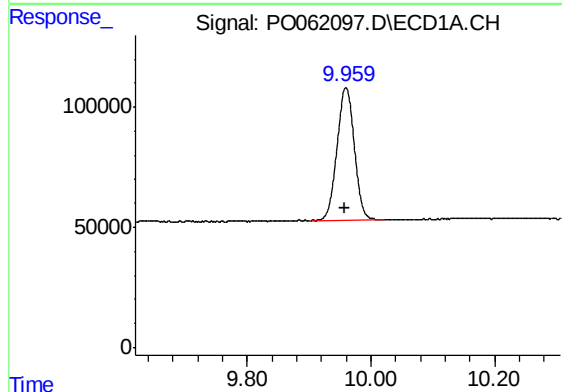


#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.003 min
Response: 1054464
Conc: 18.85 ng/ml

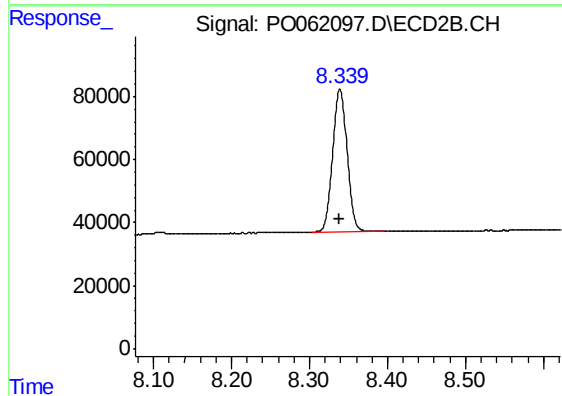

#2 Decachlorobiphenyl

R.T.: 8.339 min
Delta R.T.: 0.001 min
Response: 575290
Conc: 19.61 ng/ml

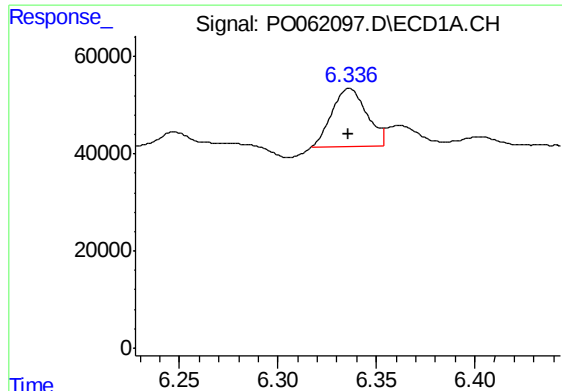


#26 AR-1254-1

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 147667
Conc: 55.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:18 PM

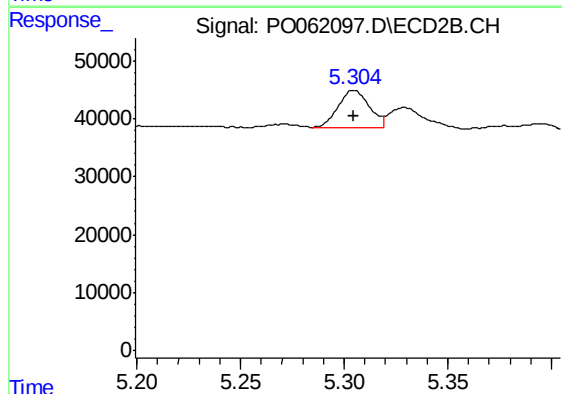


#26 AR-1254-1

R.T.: 5.305 min
Delta R.T.: 0.000 min
Response: 67541
Conc: 27.62 ng/ml

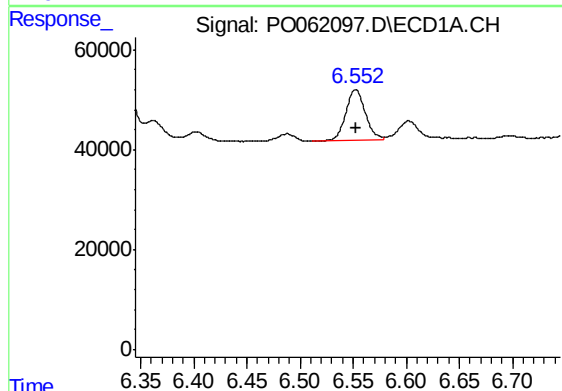


#27 AR-1254-2

R.T.: 6.552 min
Delta R.T.: 0.000 min
Response: 127761
Conc: 31.25 ng/ml

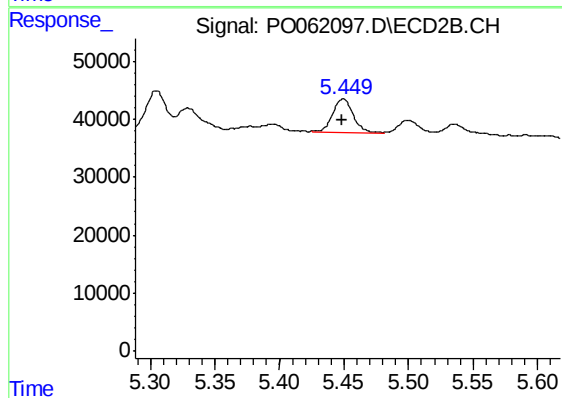

#27 AR-1254-2

R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 61899
Conc: 29.23 ng/ml

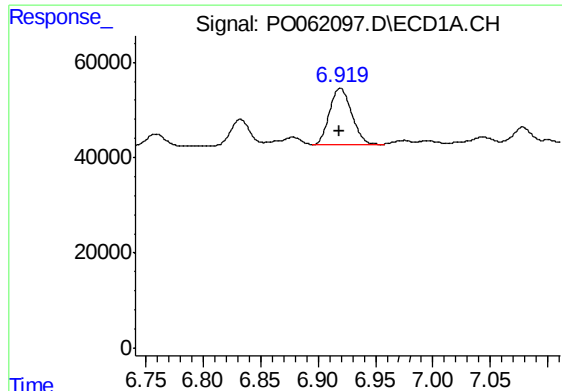


#28 AR-1254-3

R.T.: 6.919 min
Delta R.T.: 0.000 min
Response: 157270
Conc: 37.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019


Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:18 PM

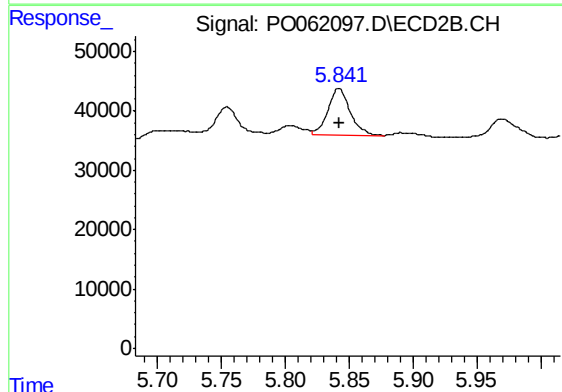


#28 AR-1254-3

R.T.: 5.842 min
Delta R.T.: 0.000 min
Response: 93228
Conc: 28.61 ng/ml

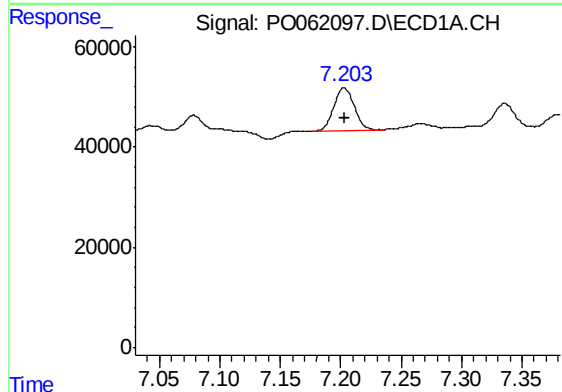


#29 AR-1254-4

R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 101468
Conc: 33.67 ng/ml m

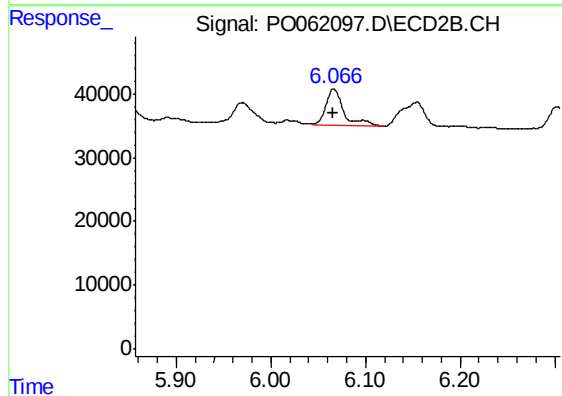

#29 AR-1254-4

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 73969
Conc: 38.30 ng/ml

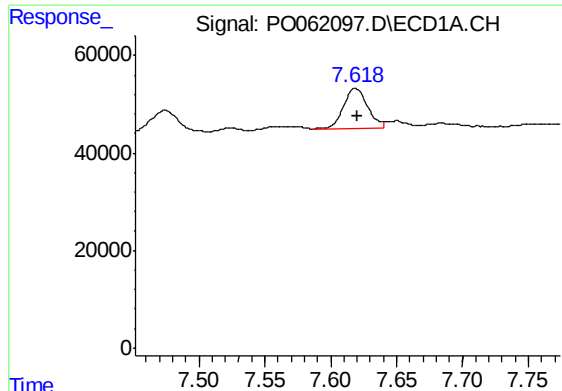


#30 AR-1254-5

R.T.: 7.618 min
Delta R.T.: -0.002 min
Response: 106323
Conc: 33.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019

Manual Integrations
APPROVED

Ankita
10/18/2019 5:49:18 PM

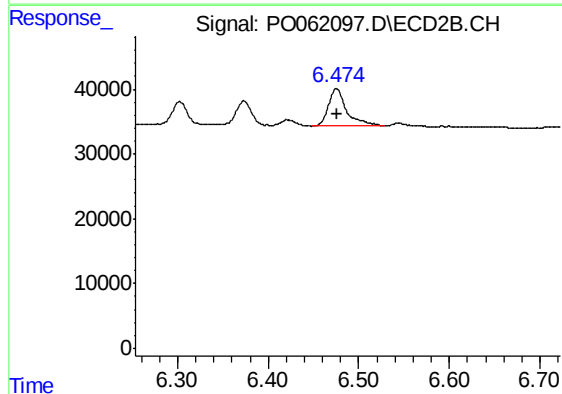

#30 AR-1254-5

R.T.: 6.475 min
Delta R.T.: 0.000 min
Response: 82470
Conc: 31.22 ng/ml