

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101719\
Data File : P0062121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2019 22:43
Operator : HP/AJ
Sample : TEST SPIKE
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST SPIKE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 05:03:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.325	3.485	11659721	7382488	188.524	172.159
2) SA Decachlor...	9.958	8.338	16631084	8087407	297.235	275.631

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101719\
Data File : P0062121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2019 22:43
Operator : HP/AJ
Sample : TEST SPIKE
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST SPIKE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 05:03:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

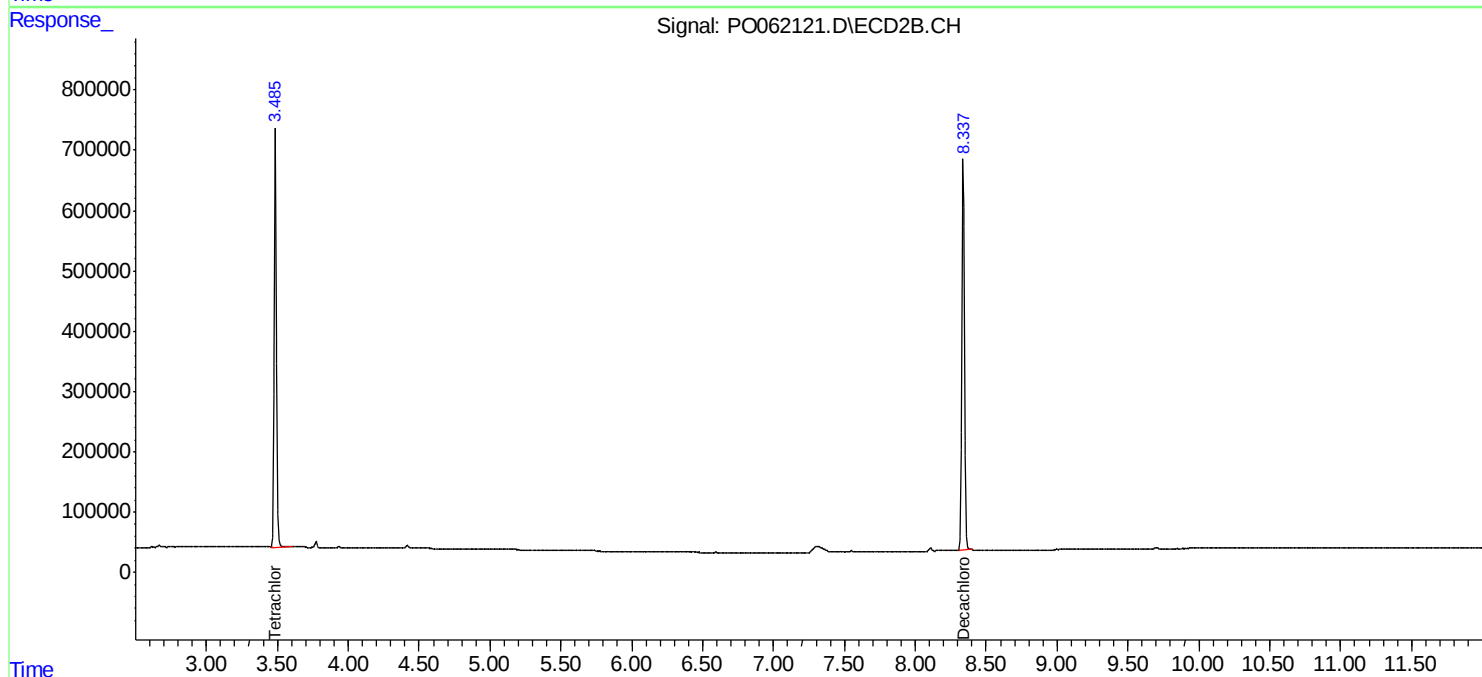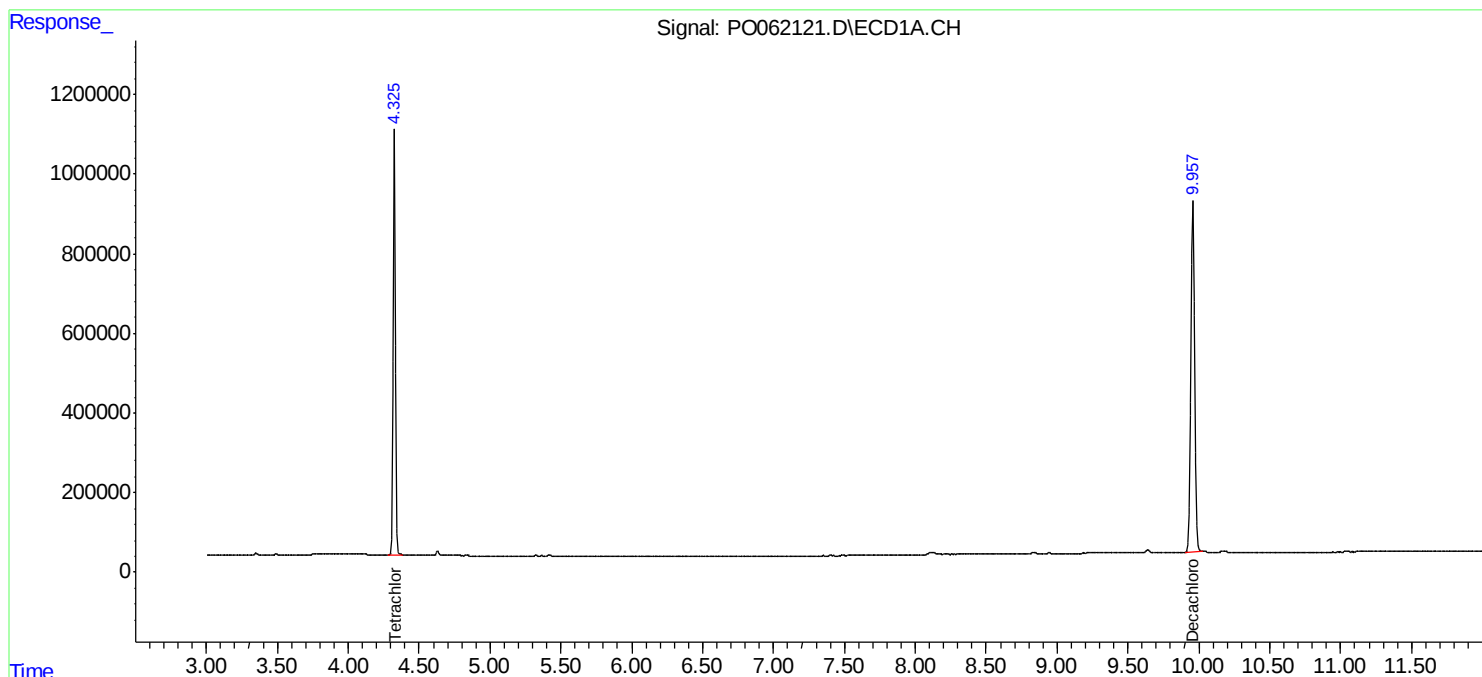


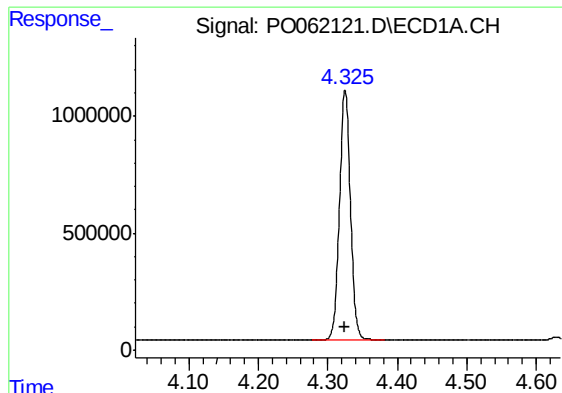

#1 Tetrachloro-m-xylene


R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 11659721
Conc: 188.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST SPIKE

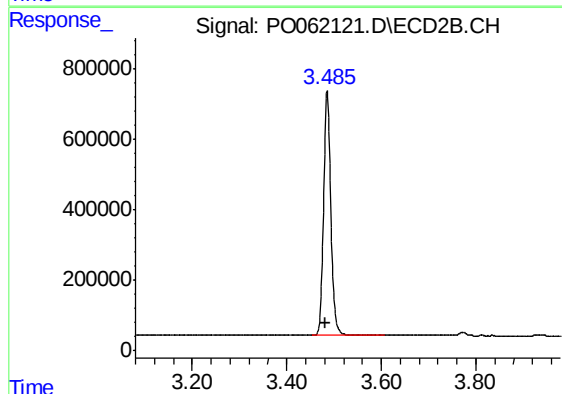


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: 0.004 min
Response: 7382488
Conc: 172.16 ng/ml

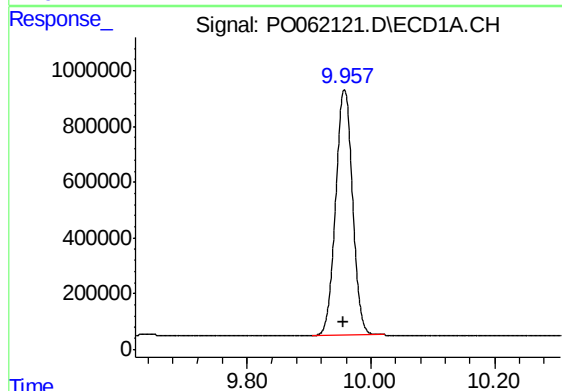

#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.001 min
Response: 16631084
Conc: 297.23 ng/ml

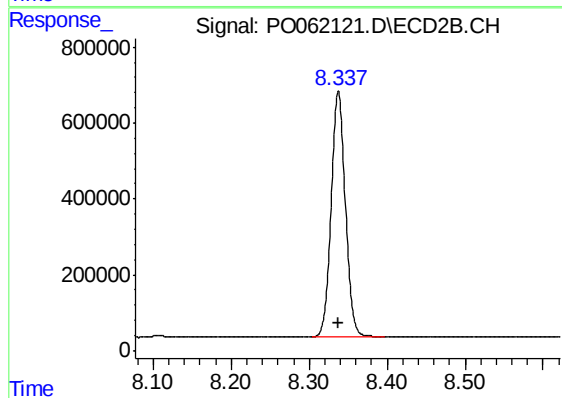

#2 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: 0.000 min
Response: 8087407
Conc: 275.63 ng/ml