

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102319\
 Data File : P0063059.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2019 14:40
 Operator : HP/AJ
 Sample : K5485-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-24B-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 00:49:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.477	1228746	861894	19.867	20.099
2)	SA Decachlor...	9.938	8.327	885305	479247	15.822	16.333
Target Compounds							
10)	L2 AR-1221-3	0.000	3.891	0	68633	N.D.	58.322 #
11)	L3 AR-1232-1	0.000	3.891	0	68633	N.D.	44.293 #
20)	L4 AR-1242-5	0.000	5.263	0	30055	N.D.	25.187 #
26)	L6 AR-1254-1	0.000	5.263	0	30055	N.D.	12.289 #
27)	L6 AR-1254-2	6.541	5.465	133070	69971	32.548	33.038
28)	L6 AR-1254-3	6.915	5.852	115433	115761	27.589	35.530 #
30)	L6 AR-1254-5	7.606	6.466	9326	46646	2.976	17.661 #
31)	L7 AR-1260-1	0.000	5.959	0	50164	N.D.	23.609 #
32)	L7 AR-1260-2	7.319	6.148	166916	58157	48.656	22.918 #
33)	L7 AR-1260-3	7.740	0.000	67452	0	25.491	N.D. #
34)	L7 AR-1260-4	0.000	6.712	0	40725	N.D.	23.194 #
35)	L7 AR-1260-5	8.171	0.000	29090	0	5.556	N.D. #
36)	L8 AR-1262-1	7.740	0.000	67452	0	16.432	N.D. #
37)	L8 AR-1262-2	8.171	0.000	29090	0	4.511	N.D. #
43)	L9 AR-1268-3	0.000	7.539	0	28072	N.D.	8.056 #
45)	L9 AR-1268-5	9.621	8.096	97554	55688	5.413	6.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063059.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2019 14:40
Operator : HP/AJ
Sample : K5485-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-24B-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 00:49:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

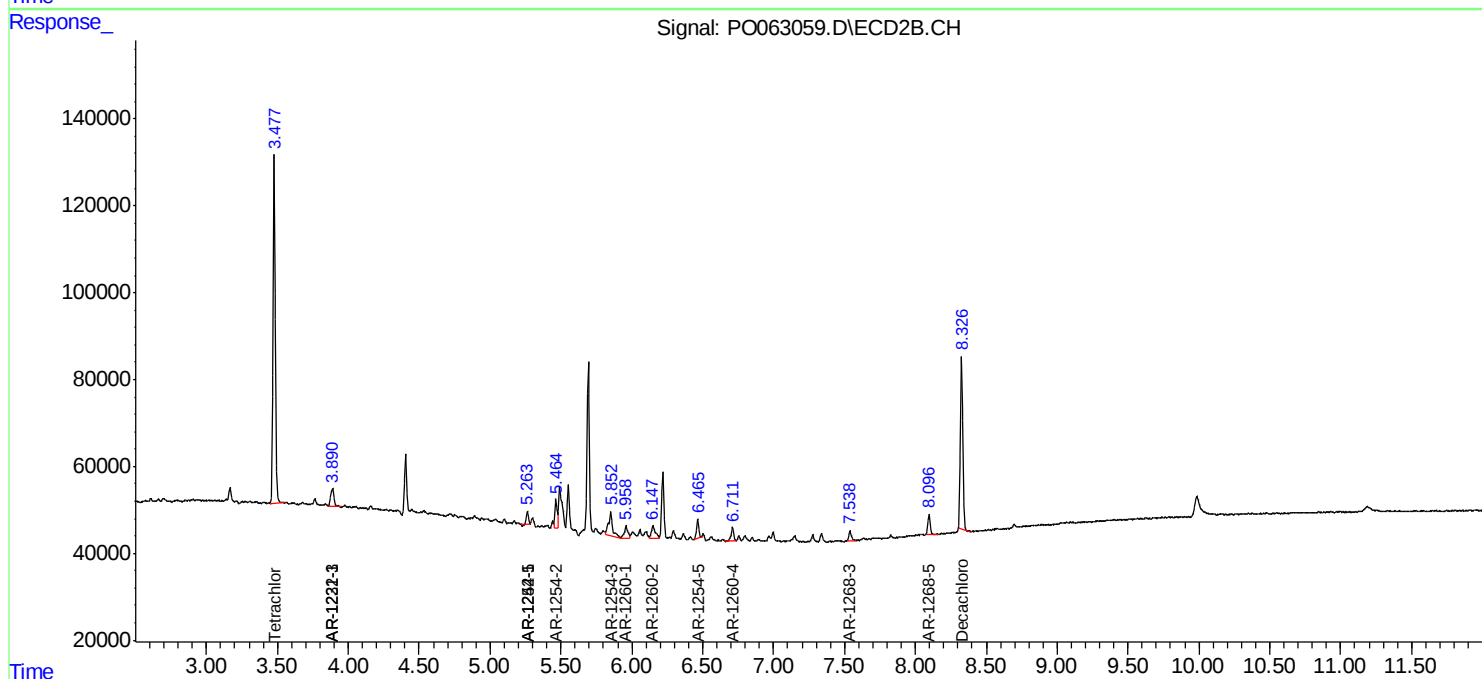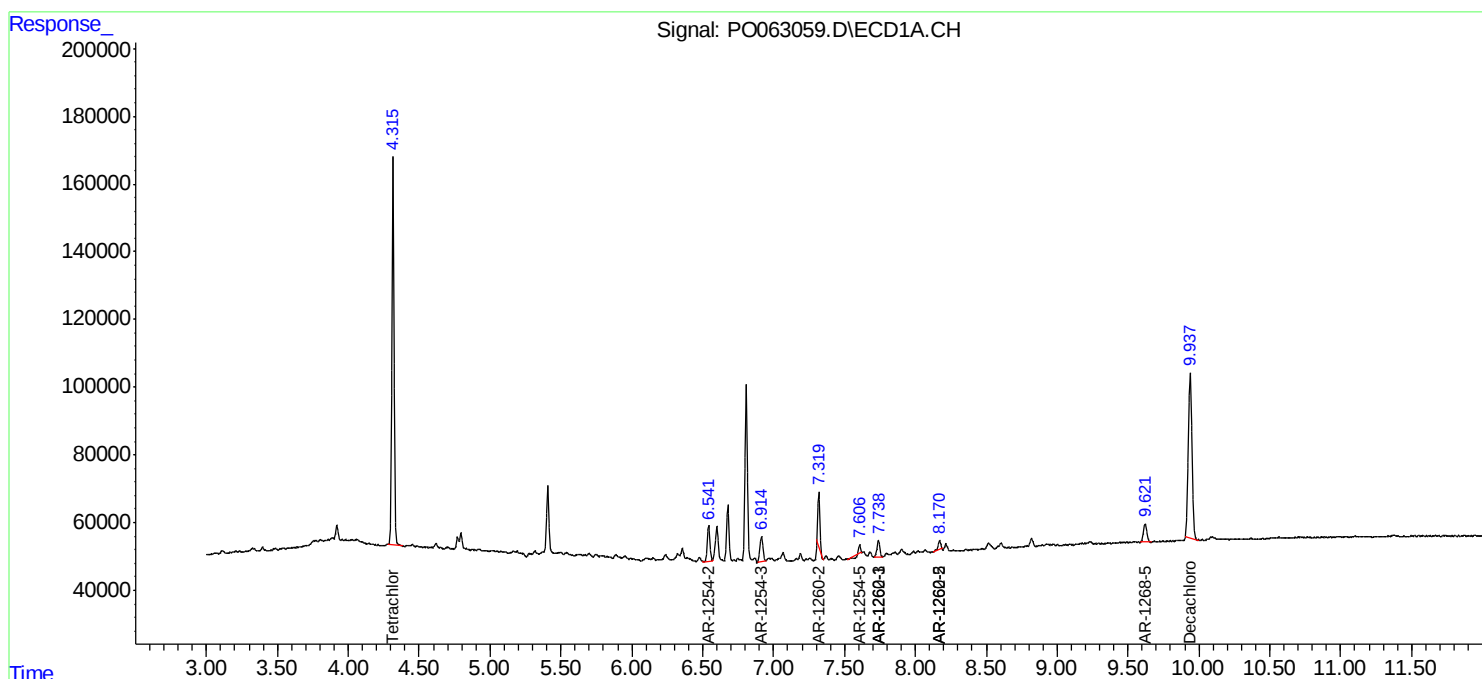


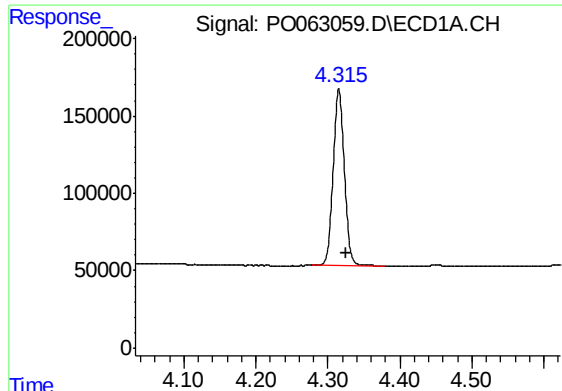

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: -0.010 min
Response: 1228746
Conc: 19.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

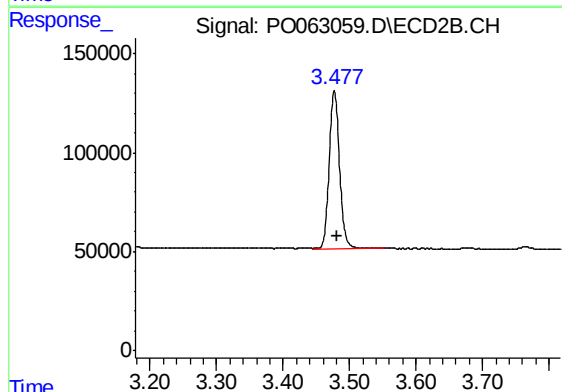


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.004 min
Response: 861894
Conc: 20.10 ng/ml

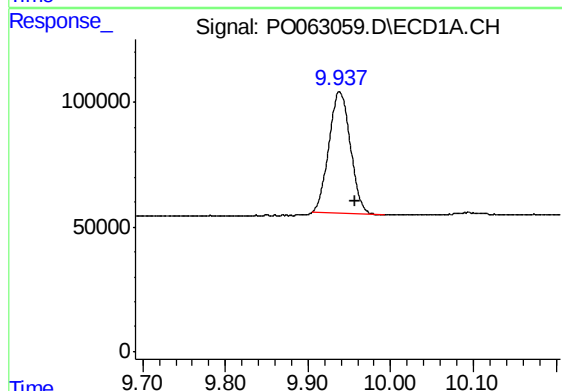


#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: -0.018 min
Response: 885305
Conc: 15.82 ng/ml

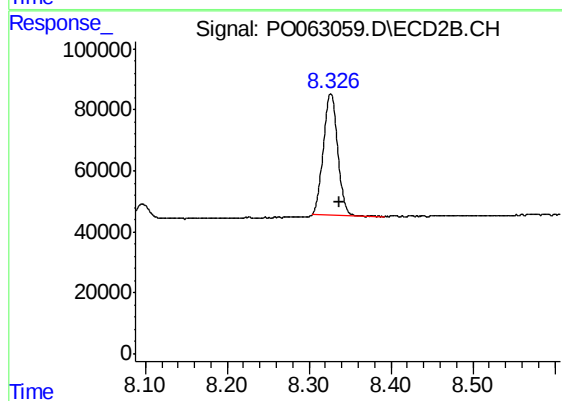

#2 Decachlorobiphenyl


R.T.: 8.327 min
Delta R.T.: -0.011 min
Response: 479247
Conc: 16.33 ng/ml

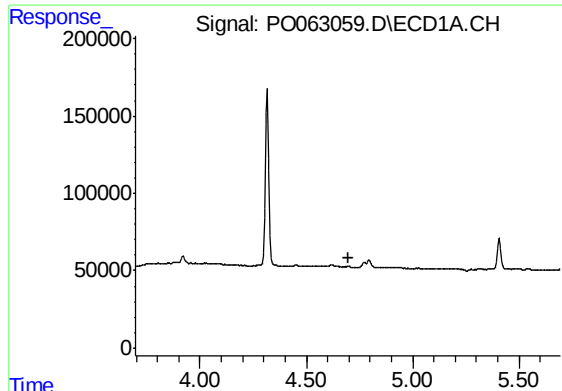

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.696 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

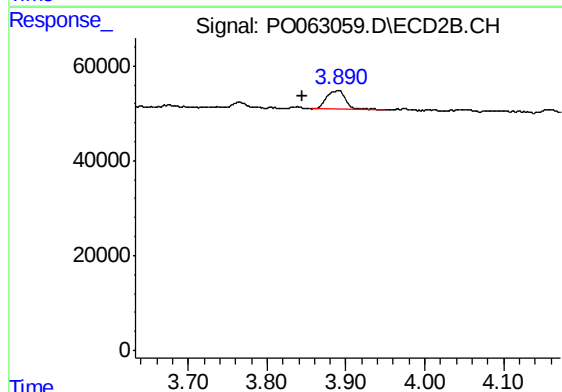


#10 AR-1221-3

R.T.: 3.891 min
Delta R.T.: 0.046 min
Response: 68633
Conc: 58.32 ng/ml

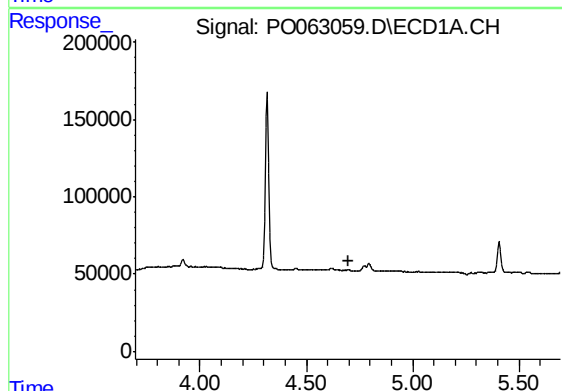


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 4.696 min
Response: 0
Conc: N.D.

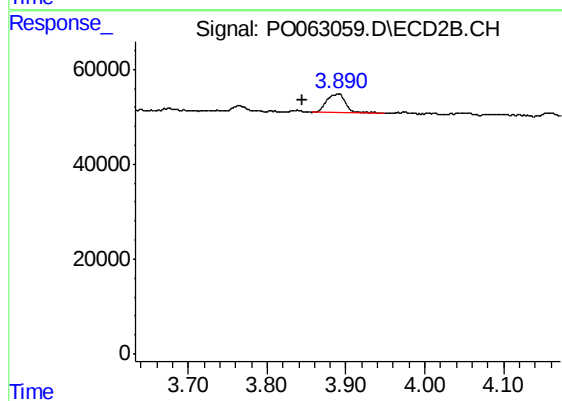

#11 AR-1232-1


R.T.: 3.891 min
Delta R.T.: 0.046 min
Response: 68633
Conc: 44.29 ng/ml

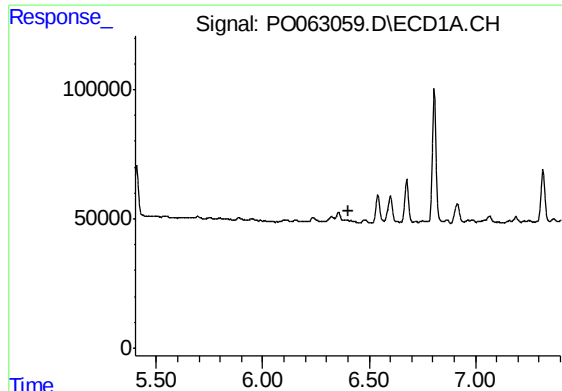

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.401 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

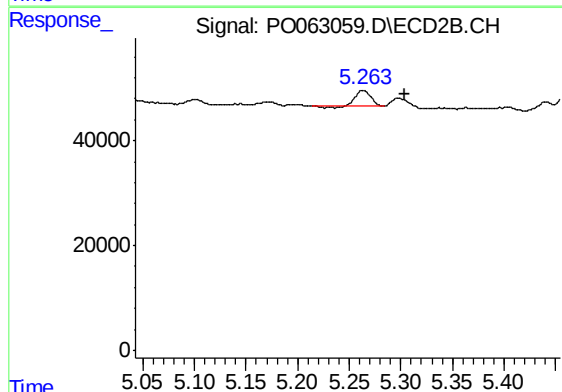


#20 AR-1242-5

R.T.: 5.263 min
Delta R.T.: -0.041 min
Response: 30055
Conc: 25.19 ng/ml

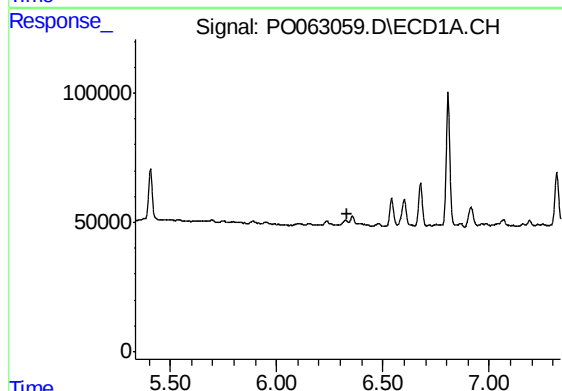


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.336 min
Response: 0
Conc: N.D.

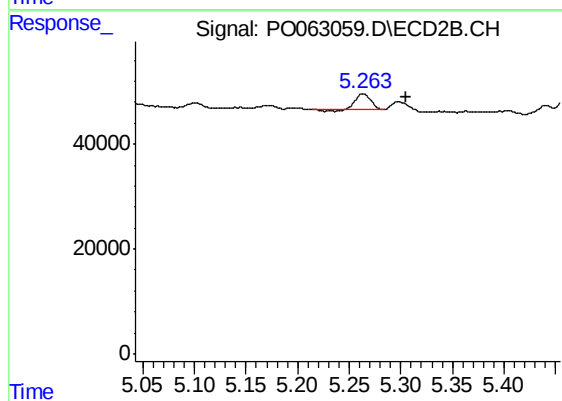

#26 AR-1254-1


R.T.: 5.263 min
Delta R.T.: -0.041 min
Response: 30055
Conc: 12.29 ng/ml

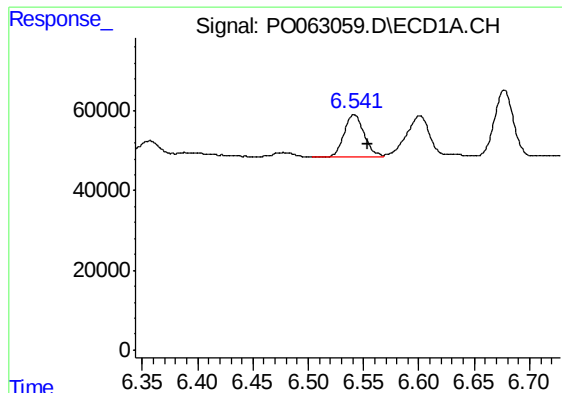

#27 AR-1254-2


R.T.: 6.541 min
Delta R.T.: -0.012 min
Response: 133070
Conc: 32.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

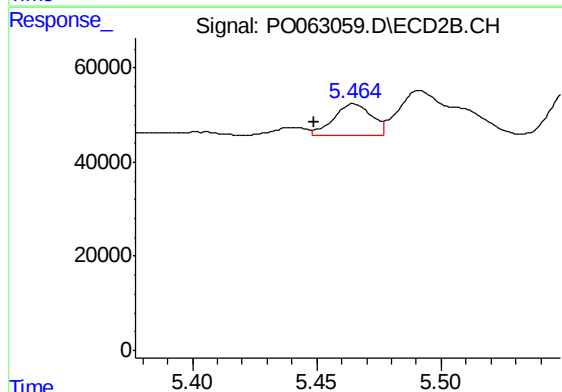


#27 AR-1254-2

R.T.: 5.465 min
Delta R.T.: 0.016 min
Response: 69971
Conc: 33.04 ng/ml

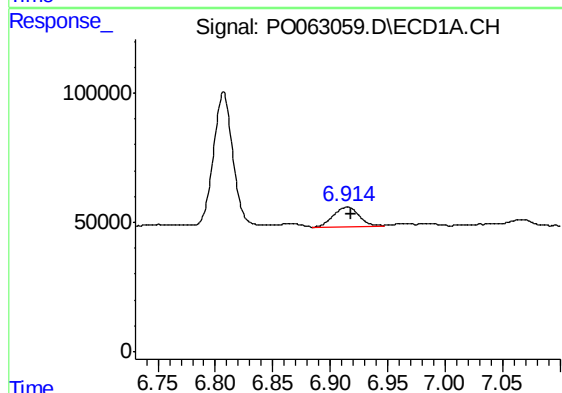


#28 AR-1254-3

R.T.: 6.915 min
Delta R.T.: -0.004 min
Response: 115433
Conc: 27.59 ng/ml

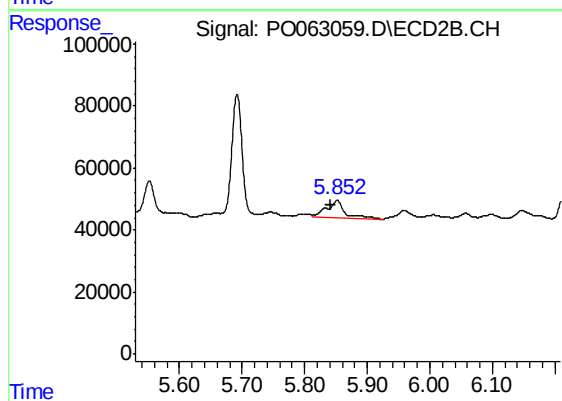

#28 AR-1254-3


R.T.: 5.852 min
Delta R.T.: 0.010 min
Response: 115761
Conc: 35.53 ng/ml

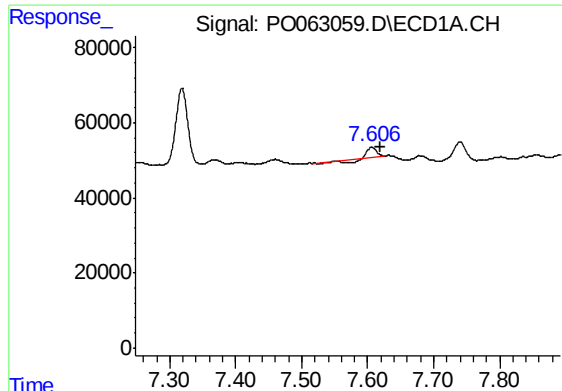

#30 AR-1254-5


R.T.: 7.606 min
Delta R.T.: -0.014 min
Response: 9326
Conc: 2.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

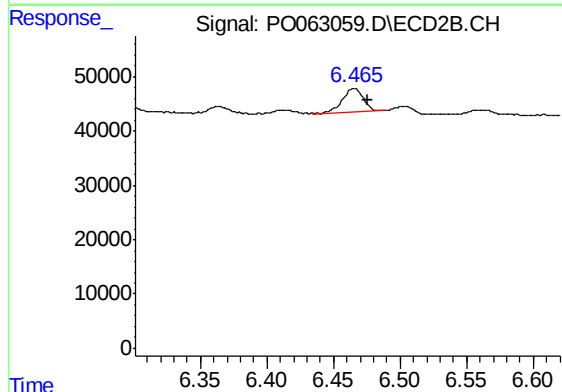


#30 AR-1254-5

R.T.: 6.466 min
Delta R.T.: -0.010 min
Response: 46646
Conc: 17.66 ng/ml

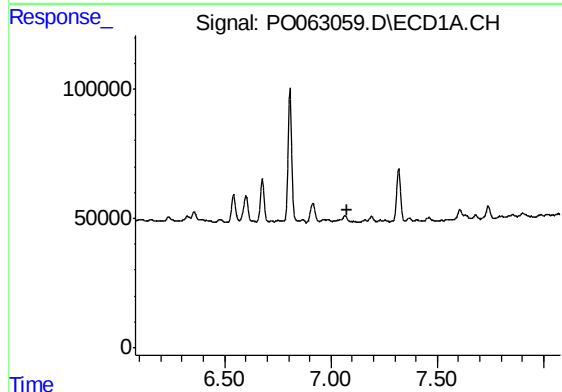


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.080 min
Response: 0
Conc: N.D.

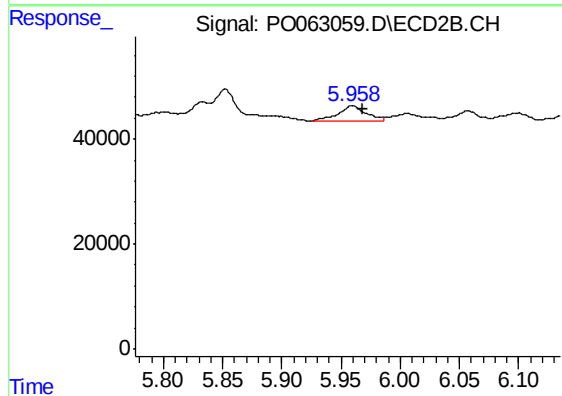

#31 AR-1260-1


R.T.: 5.959 min
Delta R.T.: -0.009 min
Response: 50164
Conc: 23.61 ng/ml

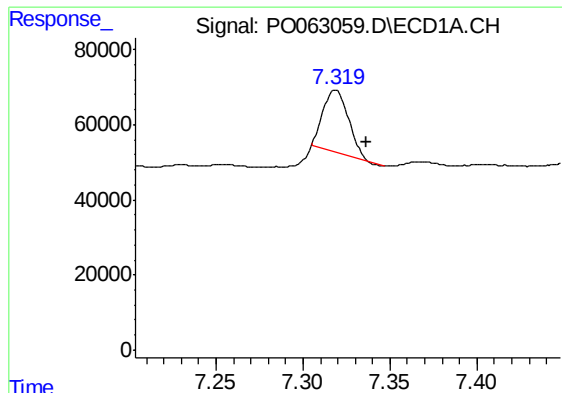

#32 AR-1260-2


R.T.: 7.319 min
Delta R.T.: -0.018 min
Response: 166916
Conc: 48.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

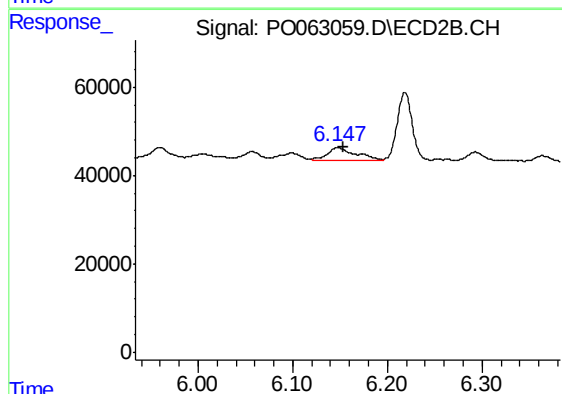


#32 AR-1260-2

R.T.: 6.148 min
Delta R.T.: -0.006 min
Response: 58157
Conc: 22.92 ng/ml

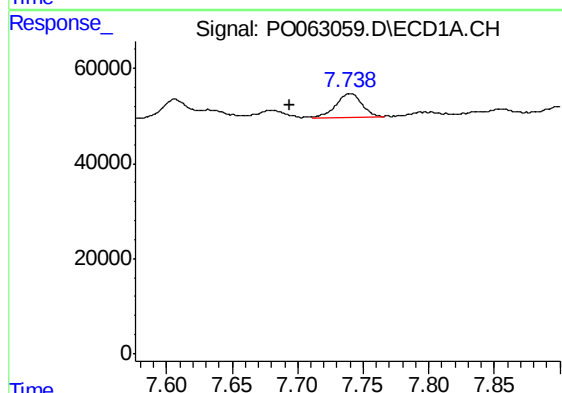


#33 AR-1260-3

R.T.: 7.740 min
Delta R.T.: 0.046 min
Response: 67452
Conc: 25.49 ng/ml

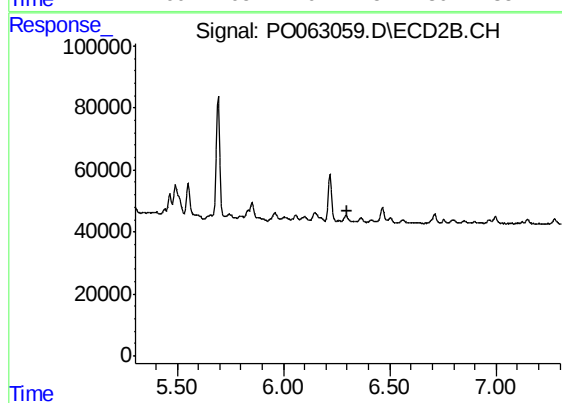

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.303 min
Response: 0
Conc: N.D.

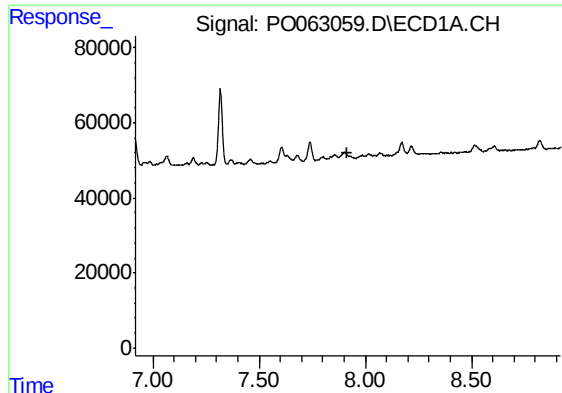

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

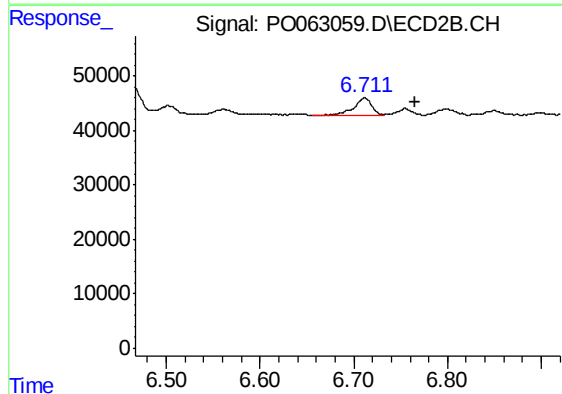


#34 AR-1260-4

R.T.: 6.712 min
Delta R.T.: -0.054 min
Response: 40725
Conc: 23.19 ng/ml

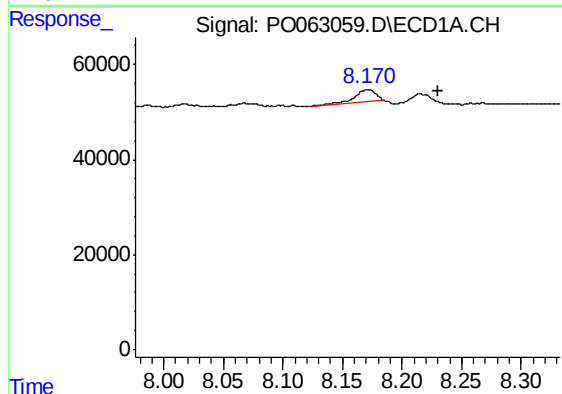


#35 AR-1260-5

R.T.: 8.171 min
Delta R.T.: -0.059 min
Response: 29090
Conc: 5.56 ng/ml

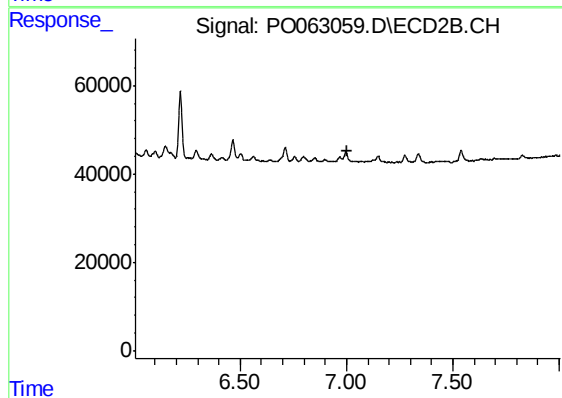

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.006 min
Response: 0
Conc: N.D.

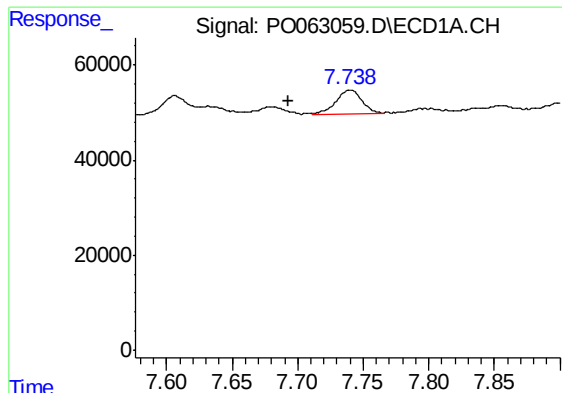

#36 AR-1262-1


R.T.: 7.740 min
Delta R.T.: 0.047 min
Response: 67452
Conc: 16.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

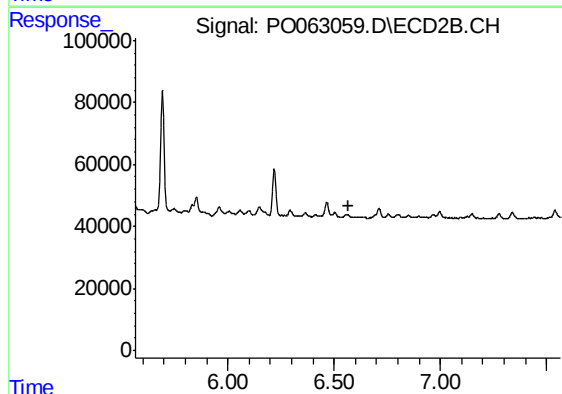


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.565 min
Response: 0
Conc: N.D.

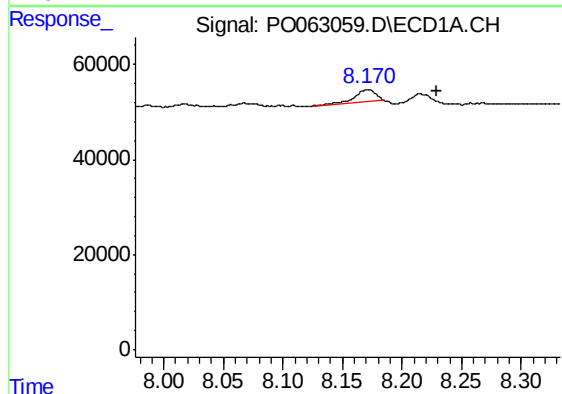


#37 AR-1262-2

R.T.: 8.171 min
Delta R.T.: -0.058 min
Response: 29090
Conc: 4.51 ng/ml

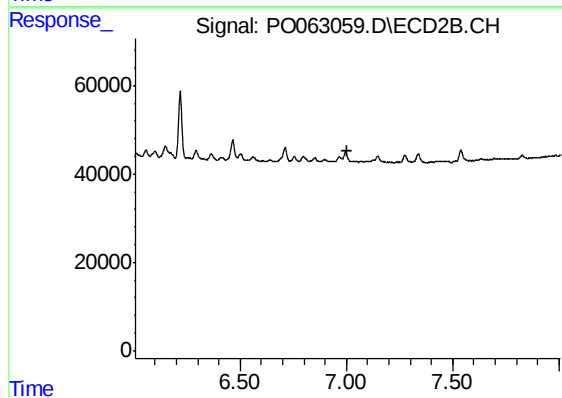

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

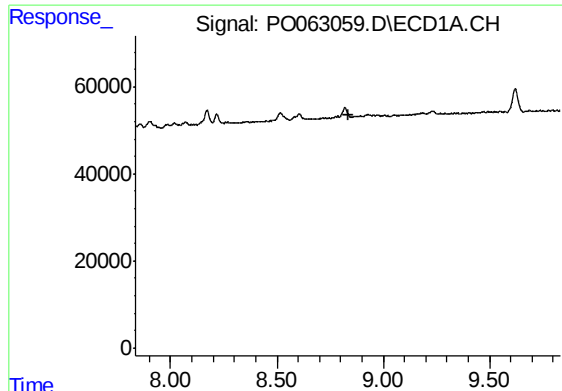

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-24B-D

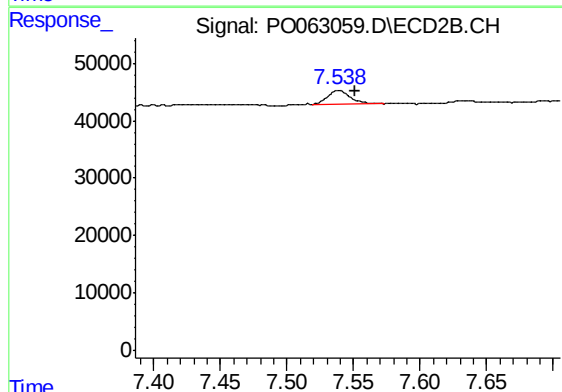


#43 AR-1268-3

R.T.: 7.539 min
Delta R.T.: -0.012 min
Response: 28072
Conc: 8.06 ng/ml

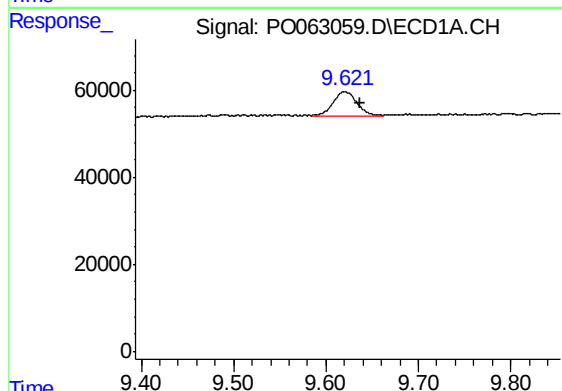

#45 AR-1268-5

R.T.: 9.621 min
Delta R.T.: -0.017 min
Response: 97554
Conc: 5.41 ng/ml

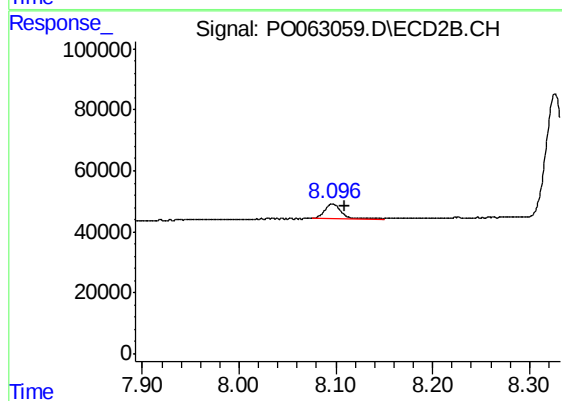

#45 AR-1268-5

R.T.: 8.096 min
Delta R.T.: -0.012 min
Response: 55688
Conc: 6.02 ng/ml