

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102319\
 Data File : P0063063.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2019 15:45
 Operator : HP/AJ
 Sample : K5493-01RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SLOAN-ROLL-OFF-COMPRE

Manual Integrations
 APPROVED

Ankita
 10/24/2019 11:47:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:17:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.315	3.476	871068	619968	14.084	14.458m
2) SA Decachlor...	9.937	8.326	342263	198387	6.117	6.761

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063063.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2019 15:45
Operator : HP/AJ
Sample : K5493-01RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SLOAN-ROLL-OFF-COMPRE


Manual Integrations
APPROVED

Ankita
10/24/2019 11:47:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:17:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

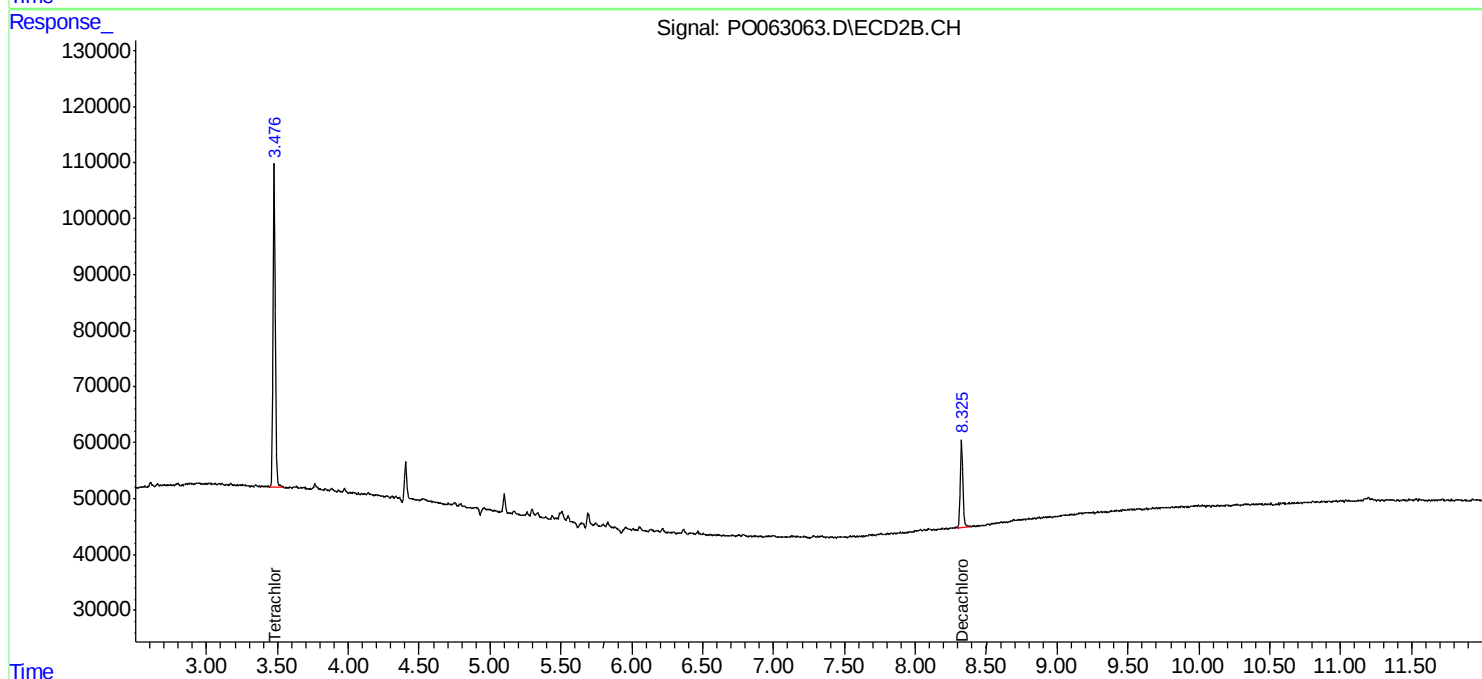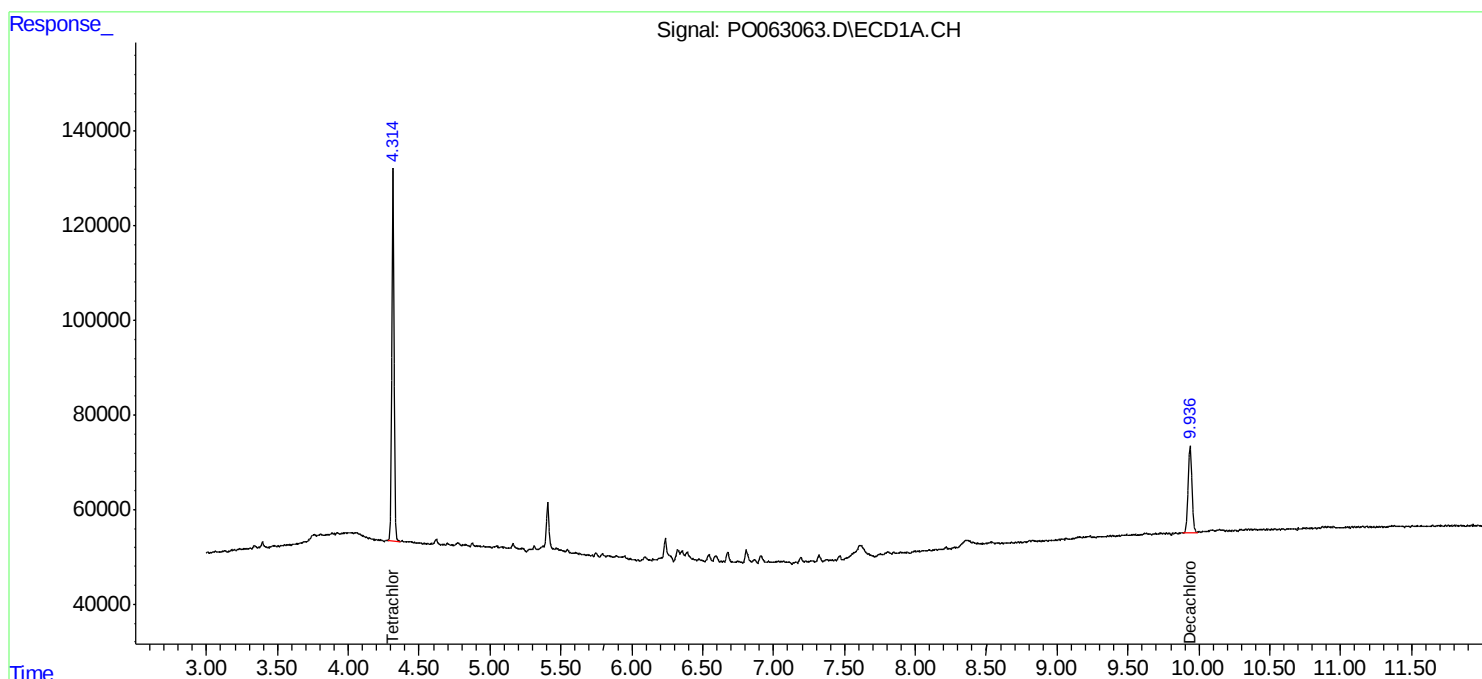

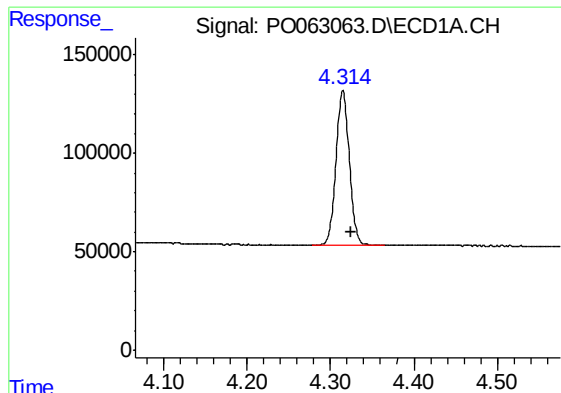


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: -0.010 min
Response: 871068
Conc: 14.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
SLOAN-ROLL-OFF-COMPRE


Manual Integrations
APPROVED

Ankita
10/24/2019 11:47:24 AM

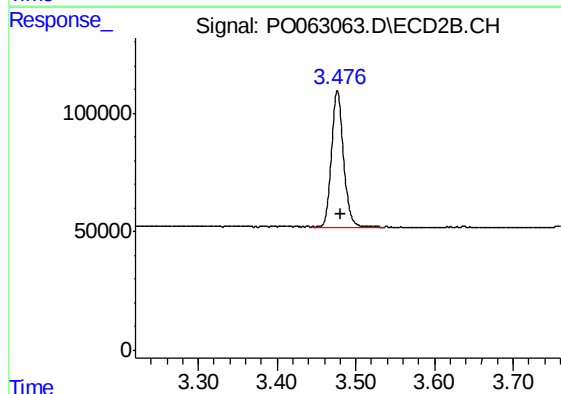


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.005 min
Response: 619968
Conc: 14.46 ng/ml m

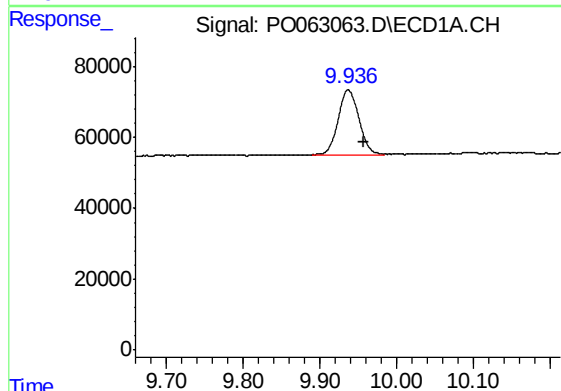

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.020 min
Response: 342263
Conc: 6.12 ng/ml

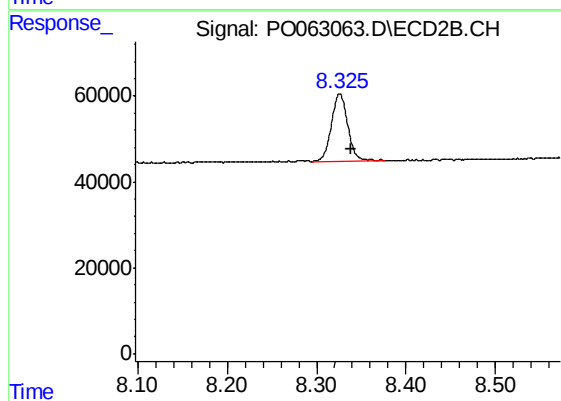

#2 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.012 min
Response: 198387
Conc: 6.76 ng/ml