

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102319\
 Data File : P0063071.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2019 18:08
 Operator : HP/AJ
 Sample : K5505-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 55-ST-22

Manual Integrations
 APPROVED

Ankita
 10/24/2019 11:47:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:20:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.317	3.480	1076618	714467	17.408m	16.661
2)	SA Decachlor...	9.938	8.326	822180	436689	14.694	14.883

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063071.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2019 18:08
Operator : HP/AJ
Sample : K5505-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
55-ST-22


Manual Integrations
APPROVED

Ankita
10/24/2019 11:47:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:20:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

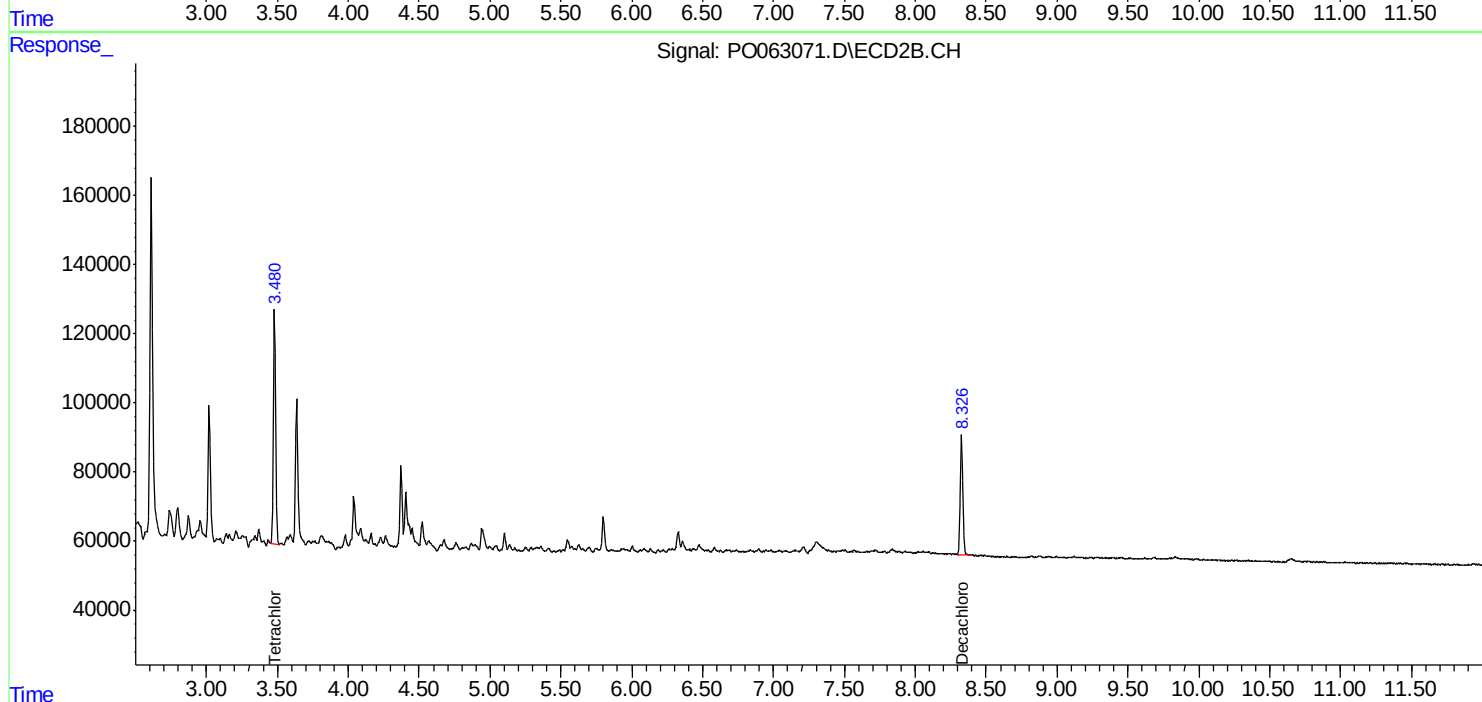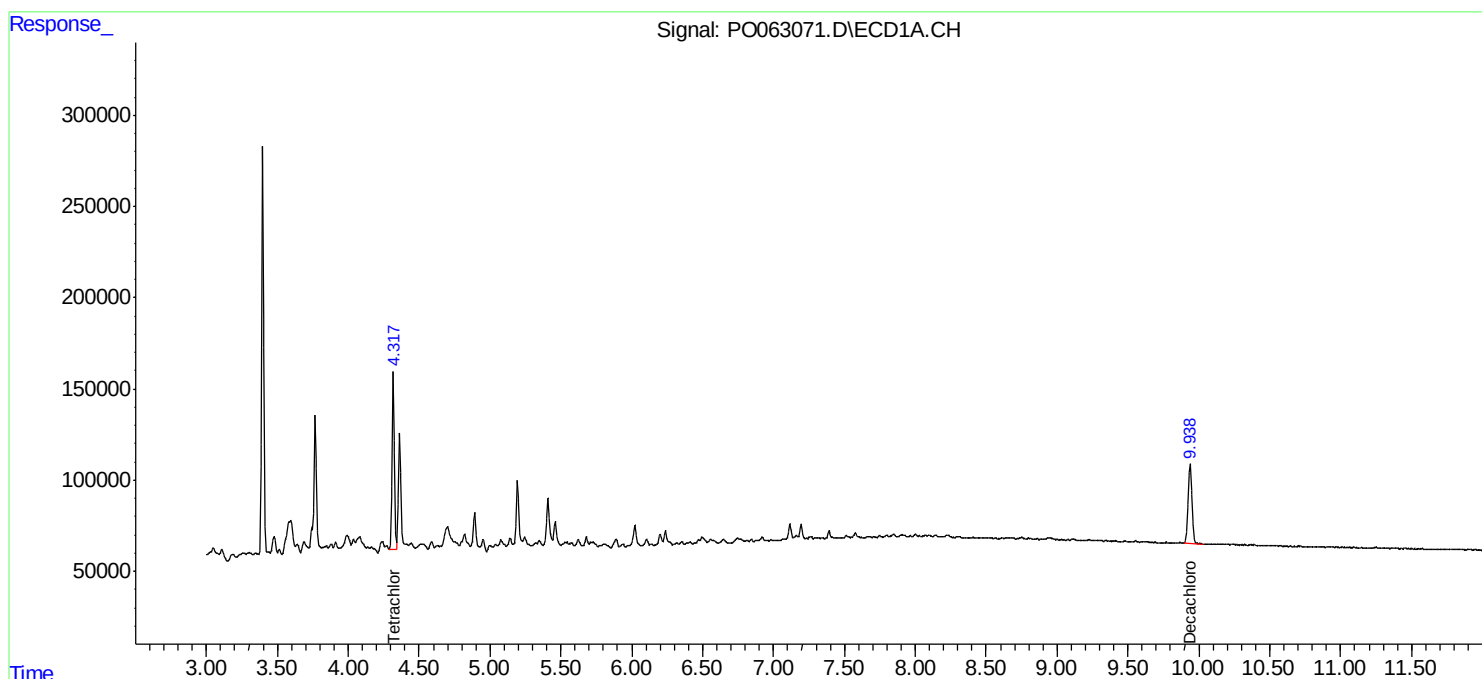

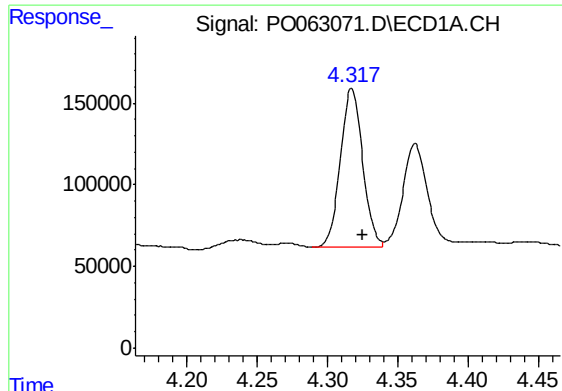


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: -0.008 min
Response: 1076618
Conc: 17.41 ng/ml m

Instrument :
ECD_O
ClientSampleId :
55-ST-22


Manual Integrations
APPROVED

Ankita
10/24/2019 11:47:46 AM

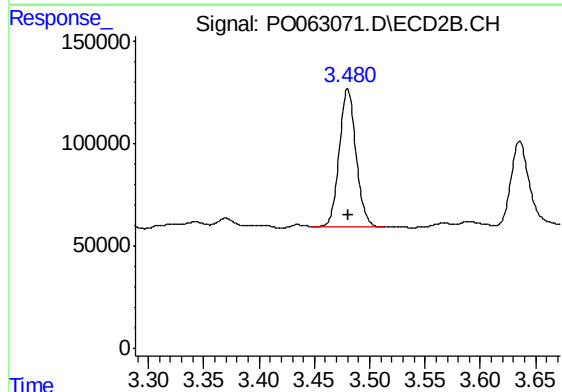


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: -0.001 min
Response: 714467
Conc: 16.66 ng/ml

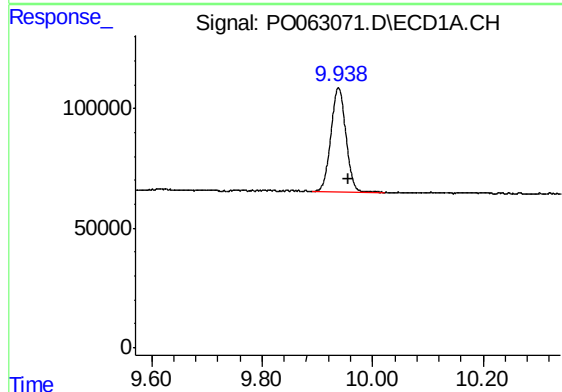

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: -0.018 min
Response: 822180
Conc: 14.69 ng/ml

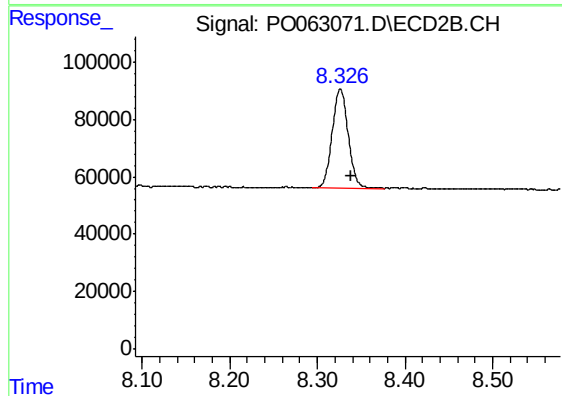

#2 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.012 min
Response: 436689
Conc: 14.88 ng/ml