

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102319\
 Data File : P0063091.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 00:59
 Operator : HP/AJ
 Sample : K5497-13
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 167-00-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/24/2019 11:48:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 03:33:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.476	977006	704731	15.797	16.434
2)	SA Decachlor...	9.934	8.323	2782897	1488655	49.737	50.736
Target Compounds							
31)	L7 AR-1260-1	7.064	5.957	56746	57102	19.931	26.875 #
32)	L7 AR-1260-2	7.319	6.144	63851	46105	18.612m	18.169
33)	L7 AR-1260-3	7.678	6.292	58603	27208	22.147	12.049m#
34)	L7 AR-1260-4	7.921	6.752	95465	68361	34.131	38.933
35)	L7 AR-1260-5	8.214	6.994	69387	57567	13.253	15.980

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063091.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 00:59
Operator : HP/AJ
Sample : K5497-13
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
167-00-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 03:33:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

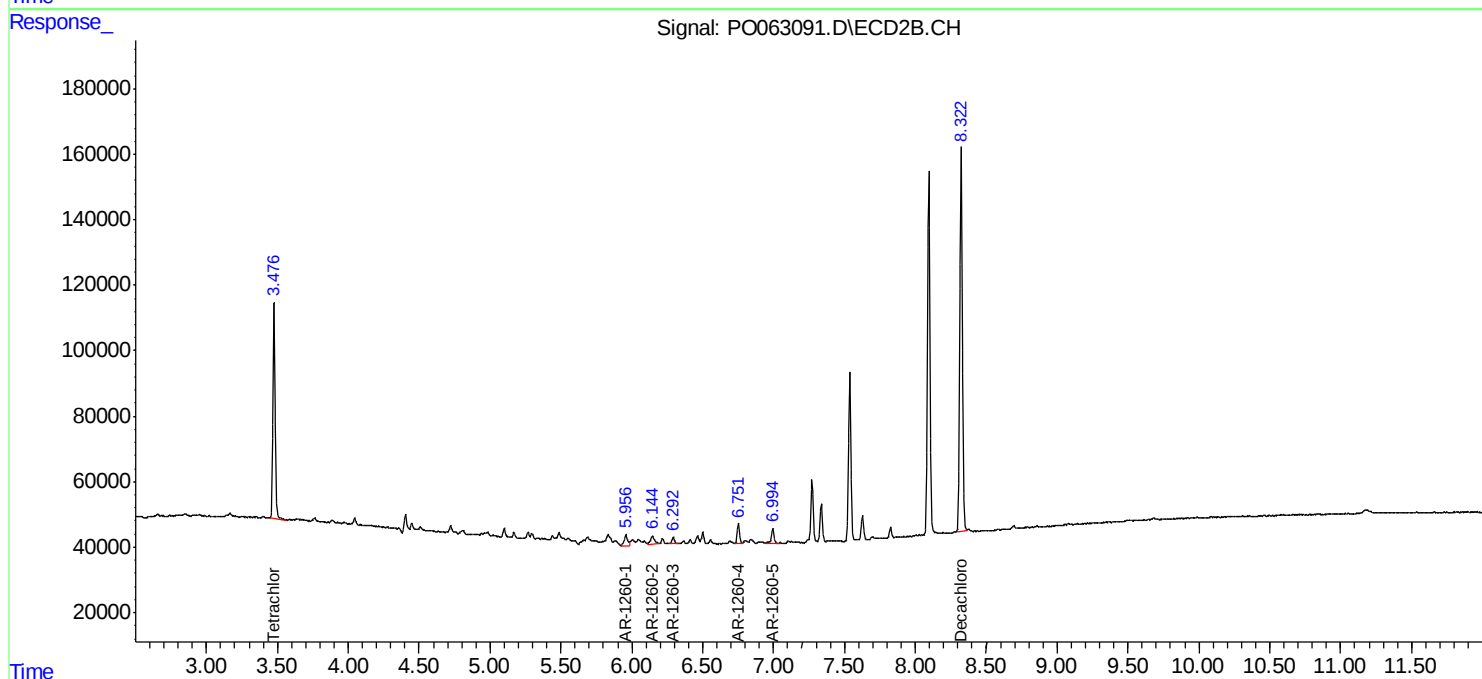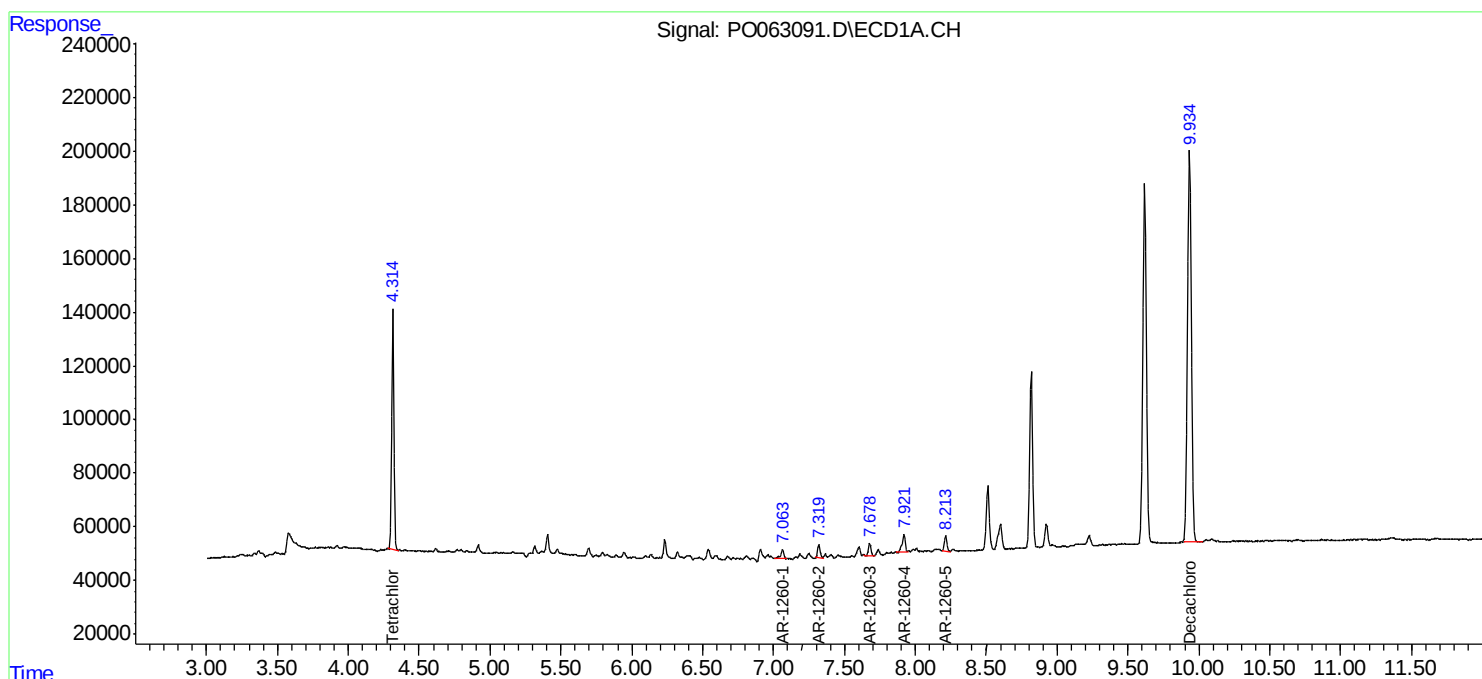

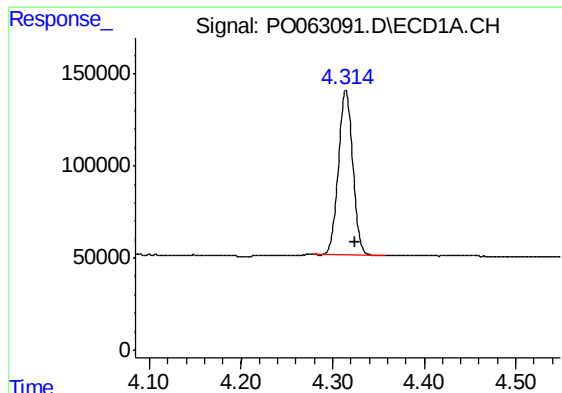


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: -0.011 min
Response: 977006
Conc: 15.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
167-00-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:46 AM

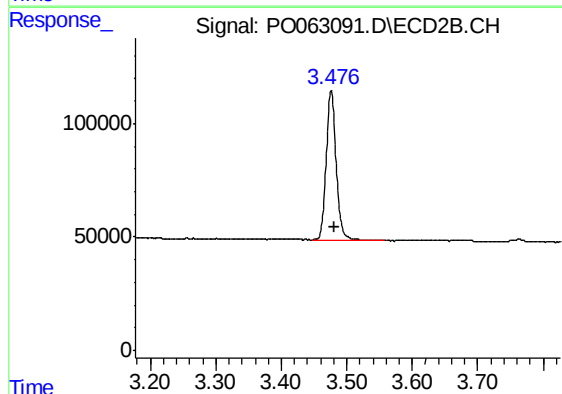


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.005 min
Response: 704731
Conc: 16.43 ng/ml

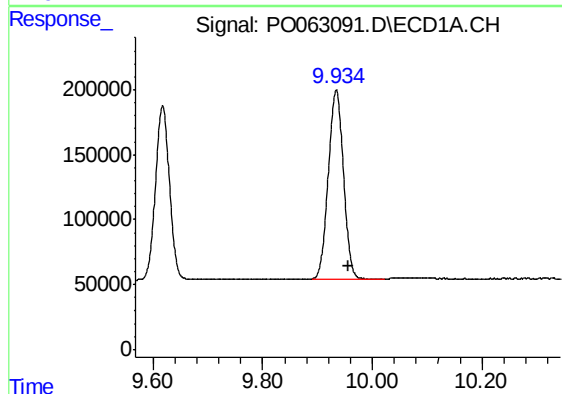


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: -0.022 min
Response: 2782897
Conc: 49.74 ng/ml

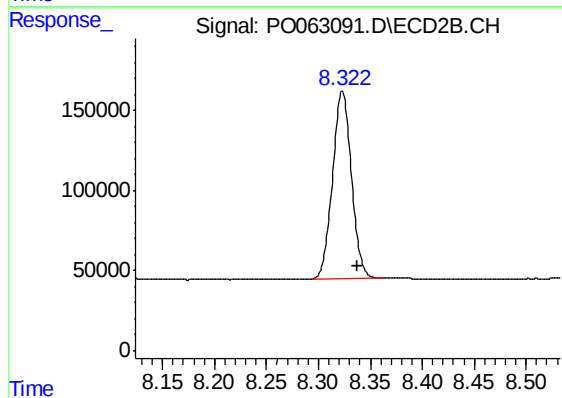

#2 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.015 min
Response: 1488655
Conc: 50.74 ng/ml

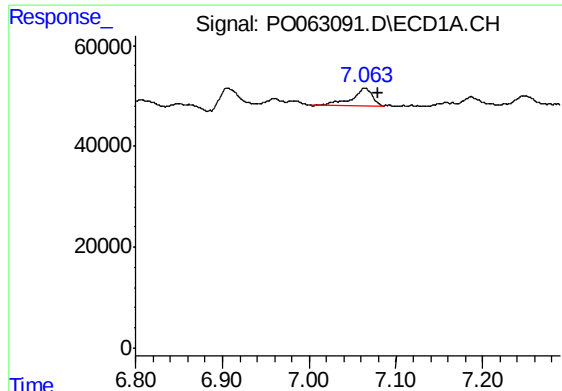


#31 AR-1260-1

R.T.: 7.064 min
Delta R.T.: -0.015 min
Response: 56746
Conc: 19.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
167-00-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:46 AM

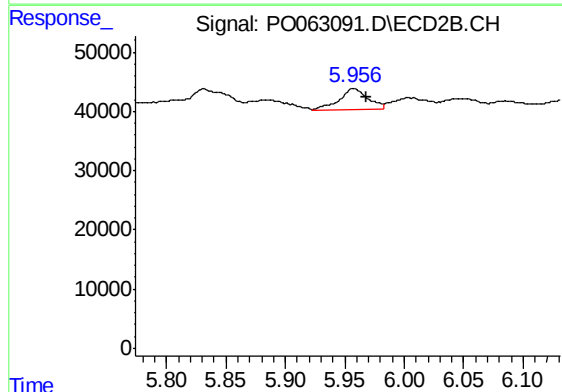


#31 AR-1260-1

R.T.: 5.957 min
Delta R.T.: -0.011 min
Response: 57102
Conc: 26.87 ng/ml

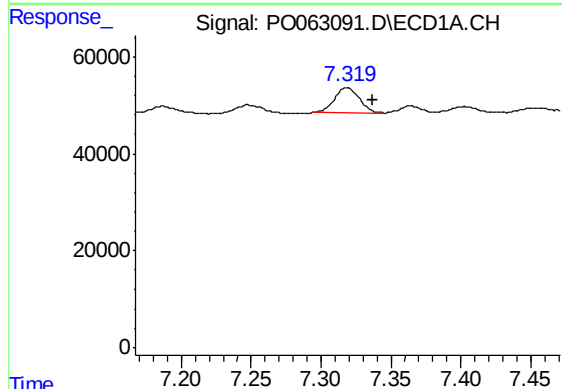


#32 AR-1260-2

R.T.: 7.319 min
Delta R.T.: -0.018 min
Response: 63851
Conc: 18.61 ng/ml m

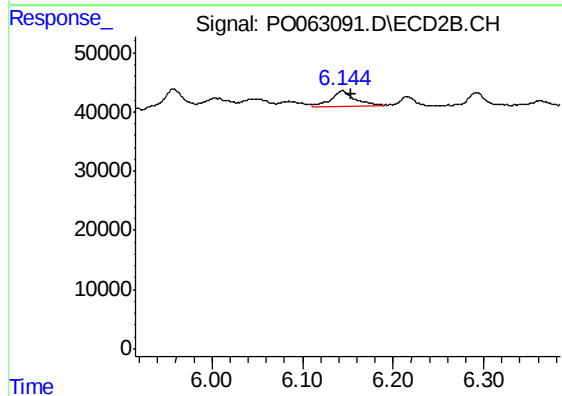

#32 AR-1260-2

R.T.: 6.144 min
Delta R.T.: -0.010 min
Response: 46105
Conc: 18.17 ng/ml

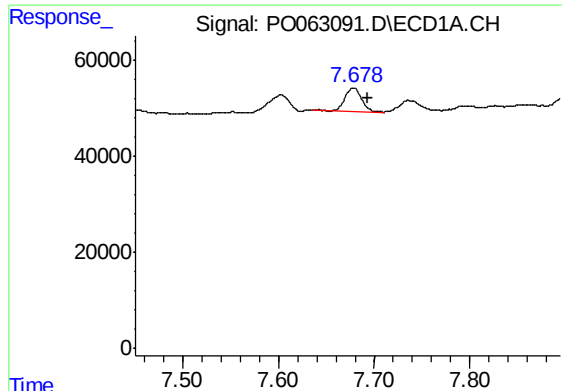


#33 AR-1260-3

R.T.: 7.678 min
Delta R.T.: -0.015 min
Response: 58603
Conc: 22.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
167-00-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:46 AM

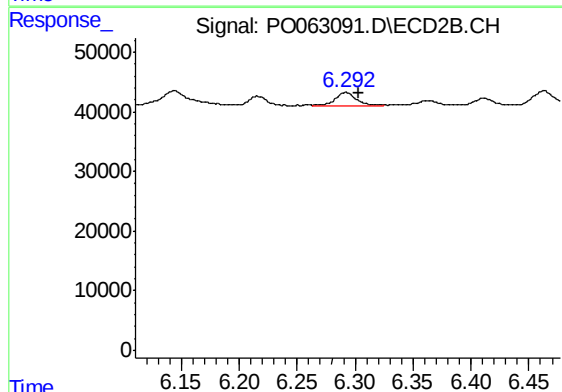


#33 AR-1260-3

R.T.: 6.292 min
Delta R.T.: -0.011 min
Response: 27208
Conc: 12.05 ng/ml m

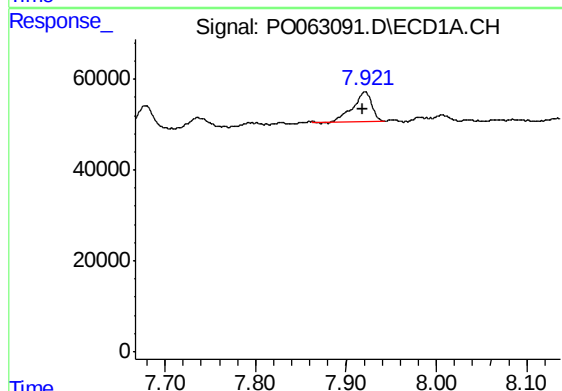


#34 AR-1260-4

R.T.: 7.921 min
Delta R.T.: 0.003 min
Response: 95465
Conc: 34.13 ng/ml

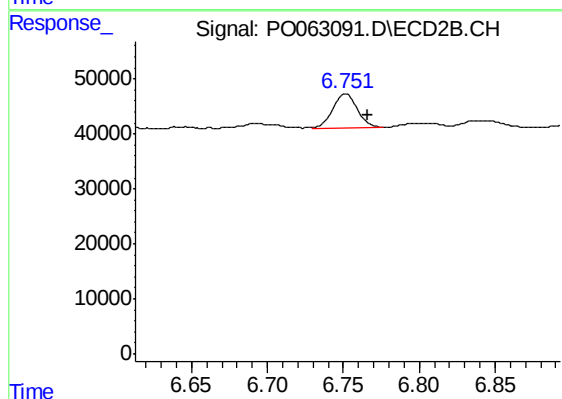

#34 AR-1260-4

R.T.: 6.752 min
Delta R.T.: -0.014 min
Response: 68361
Conc: 38.93 ng/ml

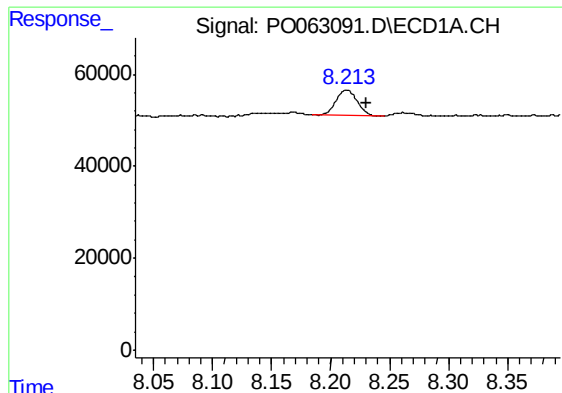


#35 AR-1260-5

R.T.: 8.214 min
Delta R.T.: -0.016 min
Response: 69387
Conc: 13.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
167-00-(0-1)

Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:46 AM

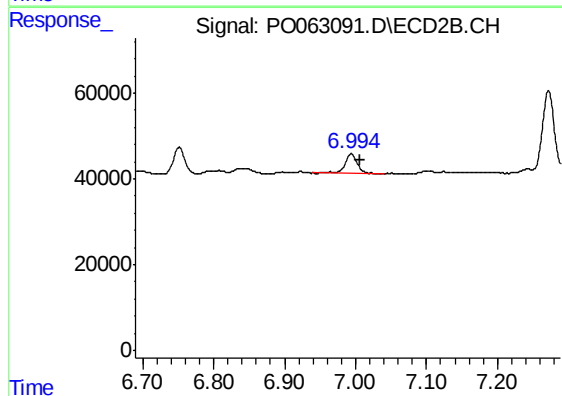

#35 AR-1260-5

R.T.: 6.994 min
Delta R.T.: -0.012 min
Response: 57567
Conc: 15.98 ng/ml