

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
 Data File : P0063093.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 1:32
 Operator : HP/AJ
 Sample : K5498-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 196-58-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/24/2019 11:48:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 03:34:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.477	1115772	796058	18.041	18.564
2)	SA Decachlor...	9.934	8.324	683294	385646	12.212	13.143
Target Compounds							
31)	L7 AR-1260-1	7.064	5.958	77745	60917	27.306m	28.671
32)	L7 AR-1260-2	7.318	6.144	133714	48144	38.978m	18.972 #
33)	L7 AR-1260-3	7.677	6.292	50592	41981	19.119	18.591
34)	L7 AR-1260-4	7.902	6.754	60557	29911	21.650m	17.035
35)	L7 AR-1260-5	8.213	6.996	75734	59965	14.465	16.646

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063093.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 1:32
Operator : HP/AJ
Sample : K5498-09
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
196-58-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 03:34:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

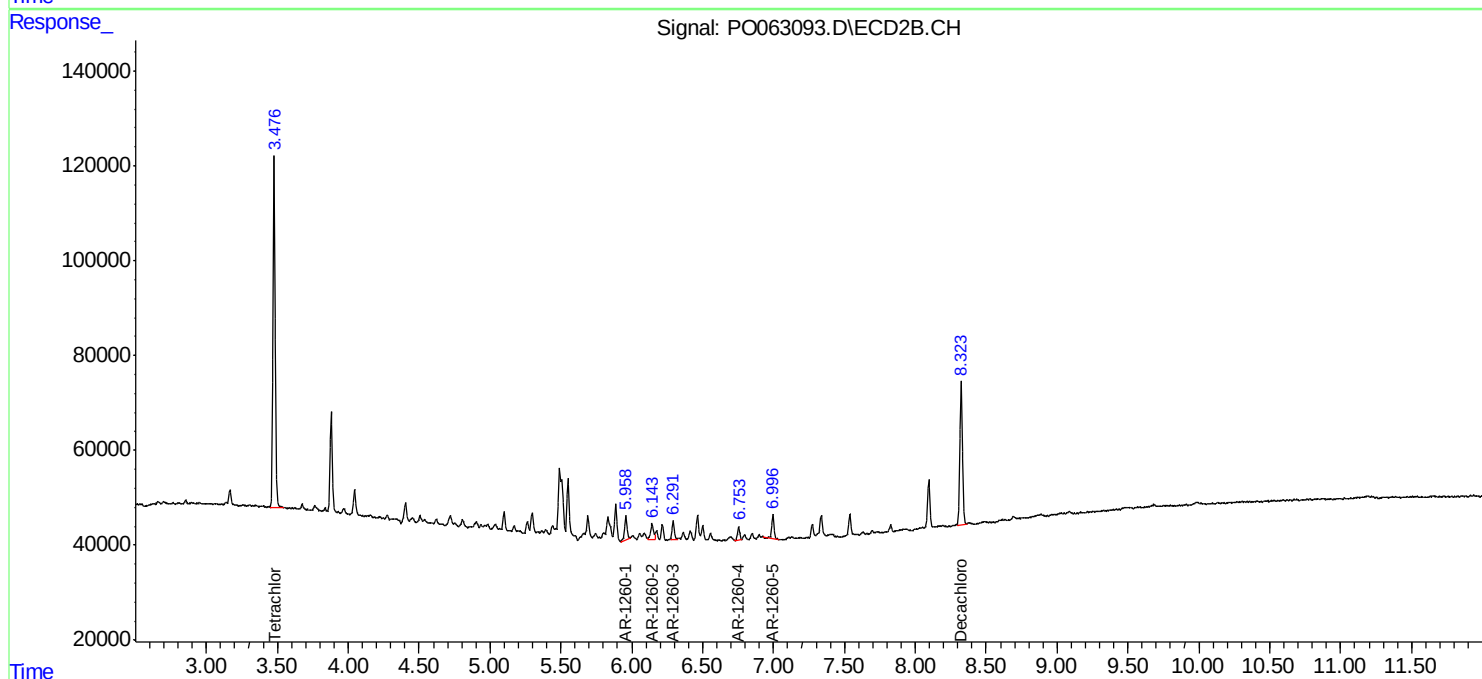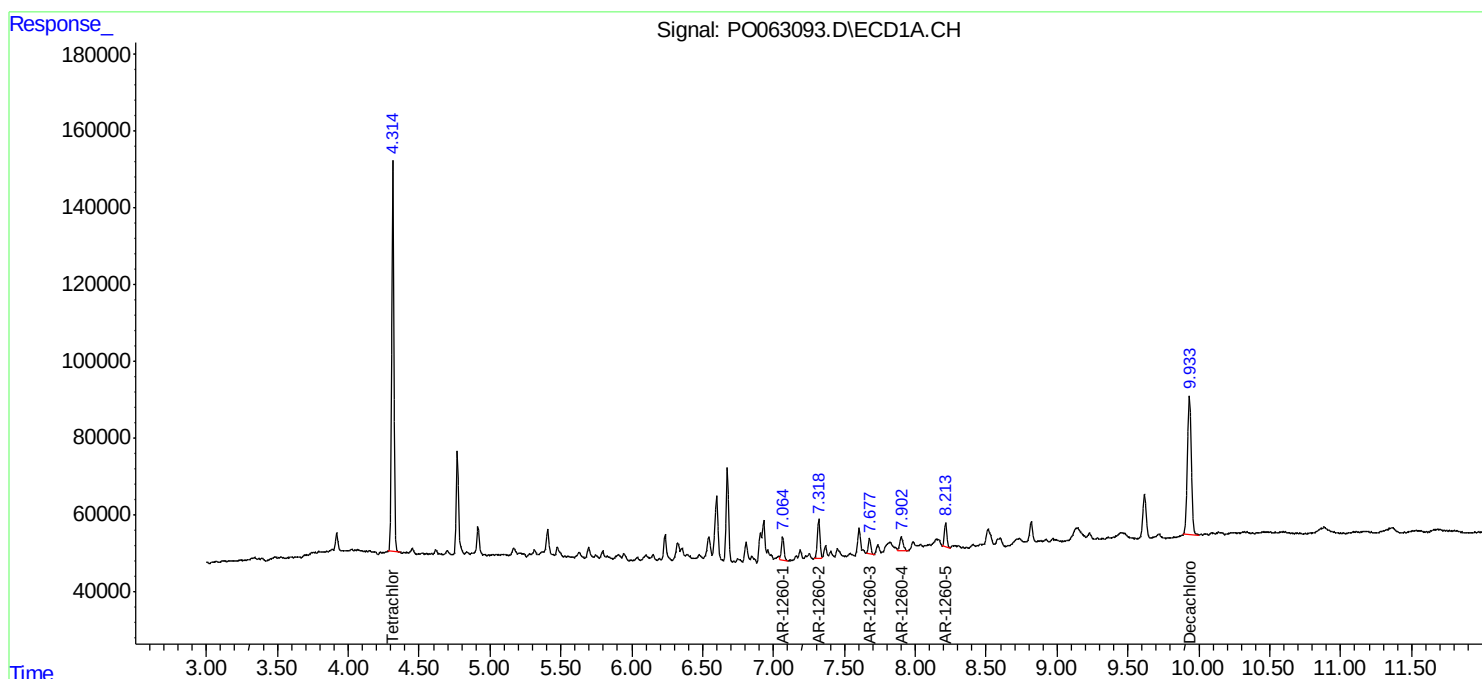

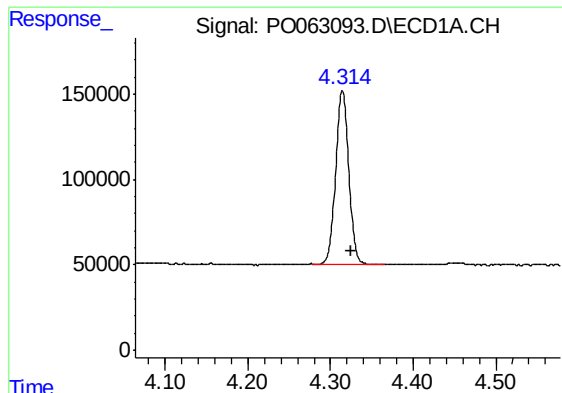


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: -0.011 min
Response: 1115772
Conc: 18.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
196-58-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:50 AM

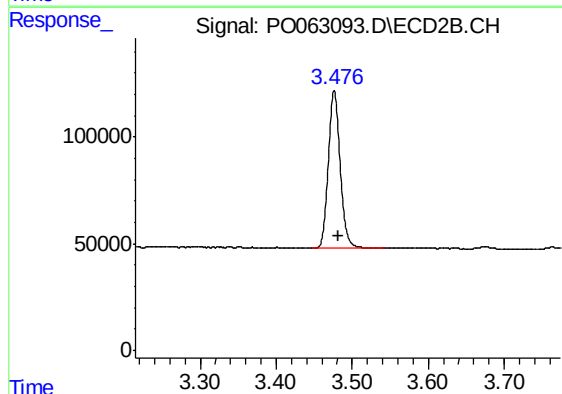


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.005 min
Response: 796058
Conc: 18.56 ng/ml

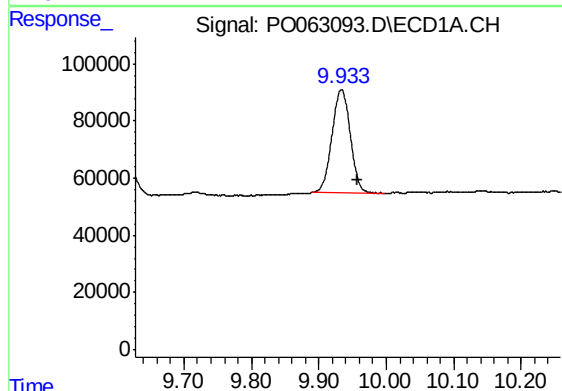


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: -0.023 min
Response: 683294
Conc: 12.21 ng/ml

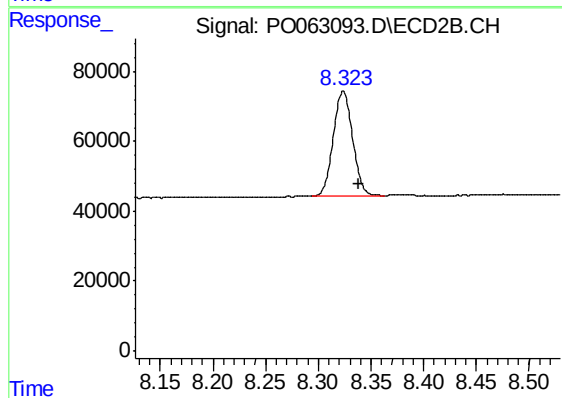

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.014 min
Response: 385646
Conc: 13.14 ng/ml

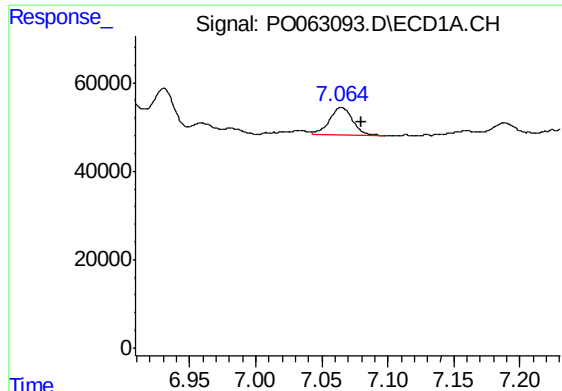


#31 AR-1260-1

R.T.: 7.064 min
Delta R.T.: -0.016 min
Response: 77745
Conc: 27.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
196-58-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:50 AM

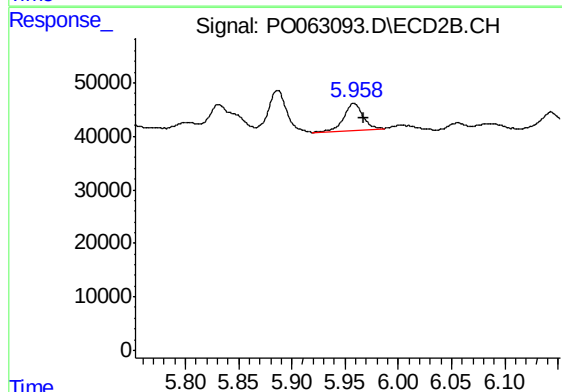


#31 AR-1260-1

R.T.: 5.958 min
Delta R.T.: -0.010 min
Response: 60917
Conc: 28.67 ng/ml

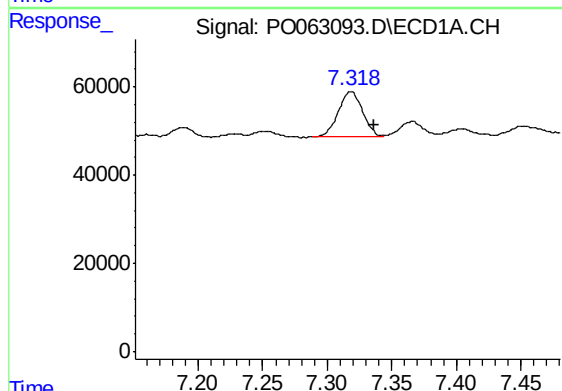


#32 AR-1260-2

R.T.: 7.318 min
Delta R.T.: -0.019 min
Response: 133714
Conc: 38.98 ng/ml m

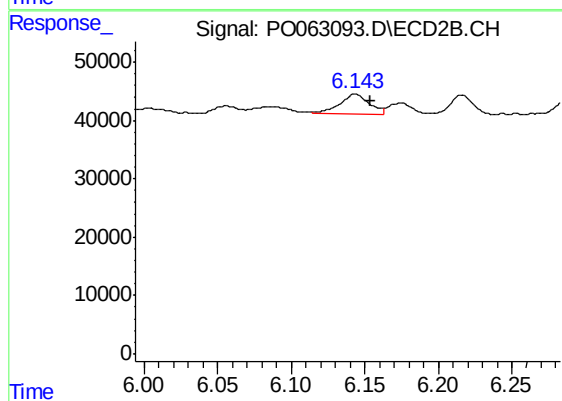

#32 AR-1260-2

R.T.: 6.144 min
Delta R.T.: -0.010 min
Response: 48144
Conc: 18.97 ng/ml

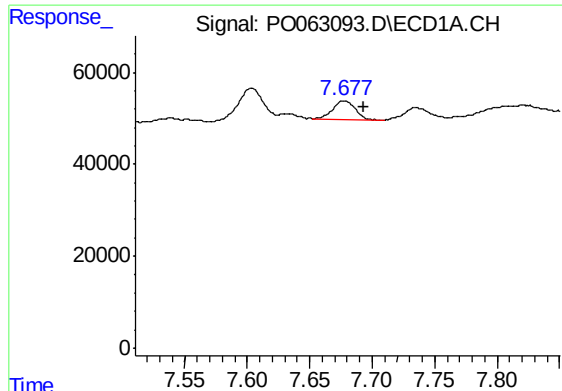


#33 AR-1260-3

R.T.: 7.677 min
Delta R.T.: -0.017 min
Response: 50592
Conc: 19.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
196-58-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:50 AM

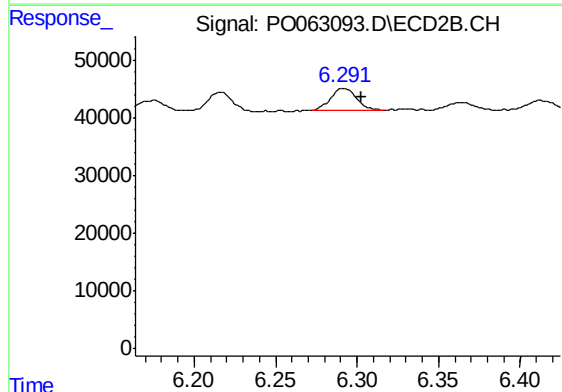


#33 AR-1260-3

R.T.: 6.292 min
Delta R.T.: -0.011 min
Response: 41981
Conc: 18.59 ng/ml

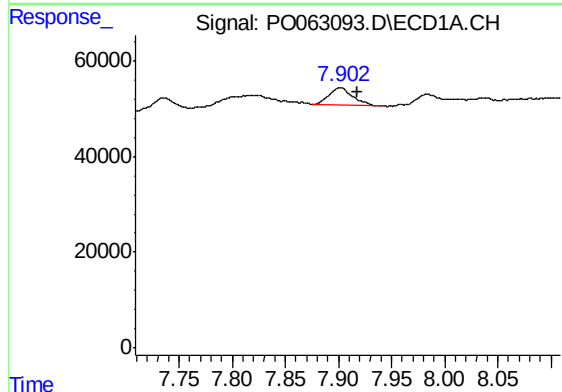


#34 AR-1260-4

R.T.: 7.902 min
Delta R.T.: -0.016 min
Response: 60557
Conc: 21.65 ng/ml m

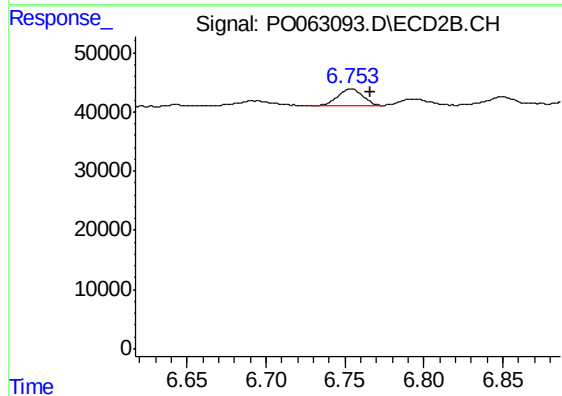

#34 AR-1260-4

R.T.: 6.754 min
Delta R.T.: -0.012 min
Response: 29911
Conc: 17.04 ng/ml

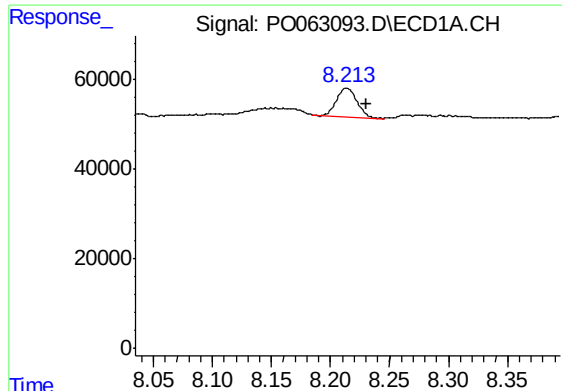


#35 AR-1260-5

R.T.: 8.213 min
Delta R.T.: -0.017 min
Response: 75734
Conc: 14.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
196-58-(0-1)

Manual Integrations
APPROVED

Ankita
10/24/2019 11:48:50 AM

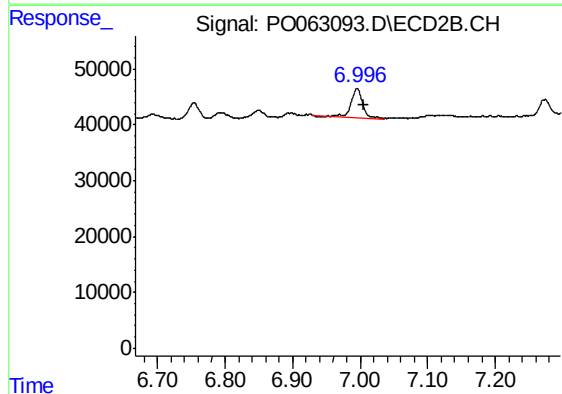

#35 AR-1260-5

R.T.: 6.996 min
Delta R.T.: -0.011 min
Response: 59965
Conc: 16.65 ng/ml