

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102319\
 Data File : P0063098.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 4:00
 Operator : HP/AJ
 Sample : K5498-11
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 191-36-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/24/2019 11:50:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 09:03:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.476	1188699	836534	19.220m	19.508
2)	SA Decachlor...	9.933	8.322	1033321	574185	18.468	19.569
Target Compounds							
31)	L7 AR-1260-1	7.065	5.961	321554	345621	112.940	162.665m#
32)	L7 AR-1260-2	7.316	6.144	606400	111654	176.765m	43.999 #
33)	L7 AR-1260-3	7.677	6.291	154796	115804	58.499	51.284
34)	L7 AR-1260-4	7.899	6.753	185897	84382	66.462m	48.058 #
35)	L7 AR-1260-5	8.213	6.995	240265	205182	45.891	56.956

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063098.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 4:00
Operator : HP/AJ
Sample : K5498-11
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
191-36-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 09:03:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

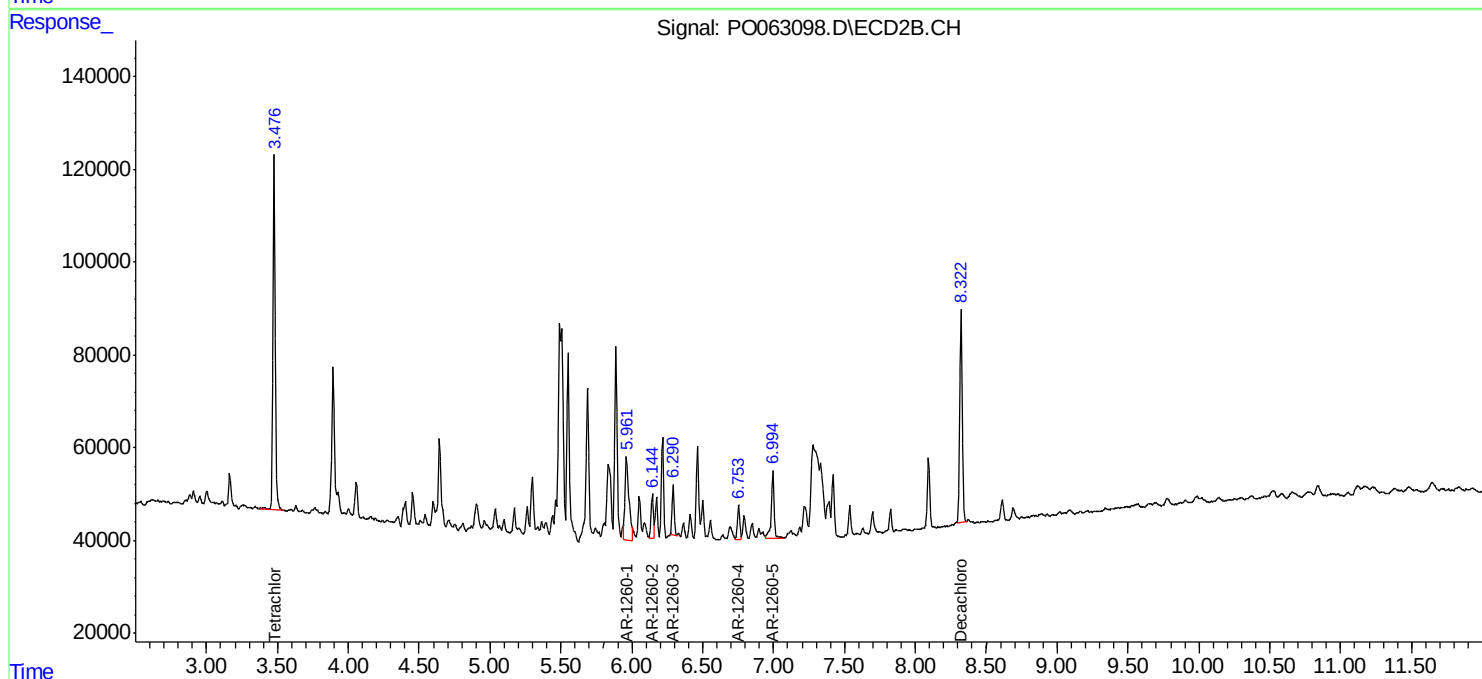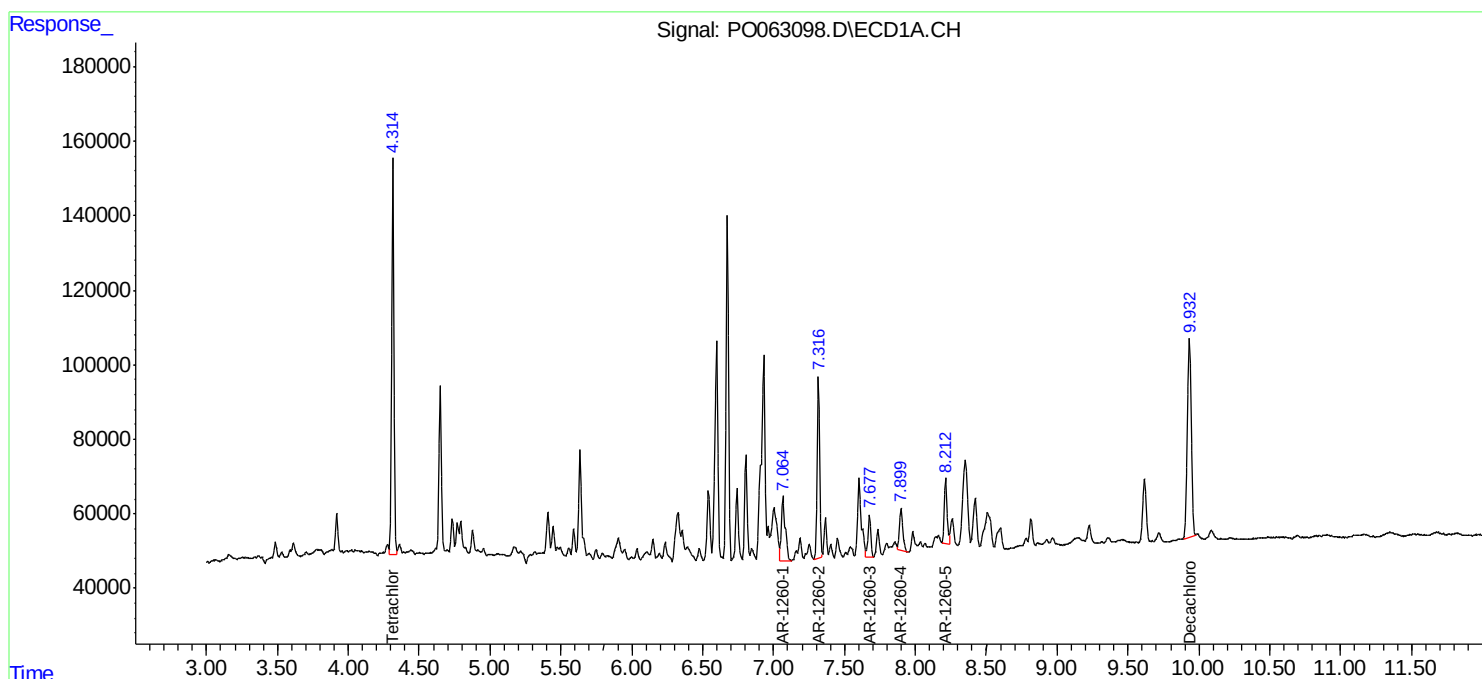

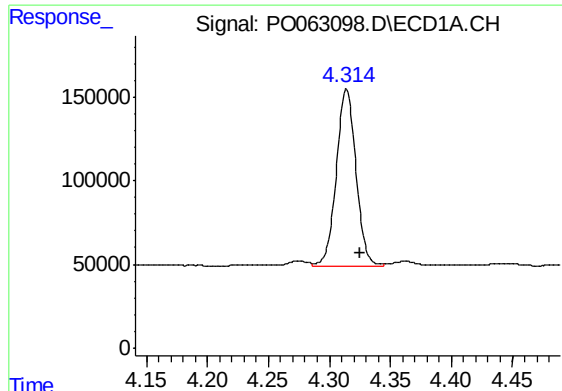


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: -0.011 min
Response: 1188699
Conc: 19.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
191-36-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:17 AM

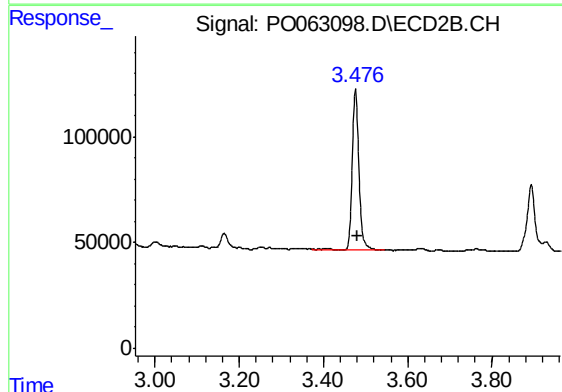


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.005 min
Response: 836534
Conc: 19.51 ng/ml

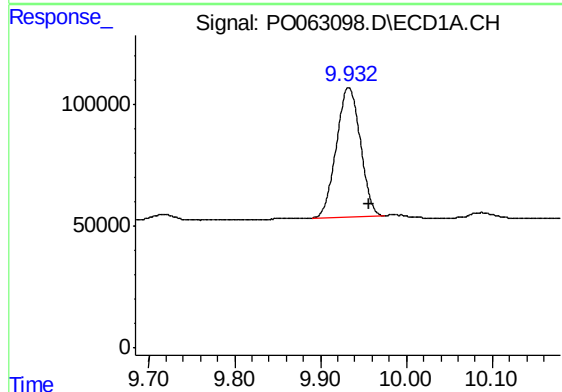


#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.024 min
Response: 1033321
Conc: 18.47 ng/ml

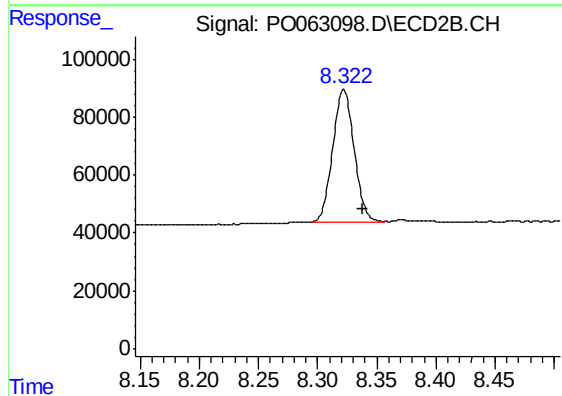

#2 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.016 min
Response: 574185
Conc: 19.57 ng/ml

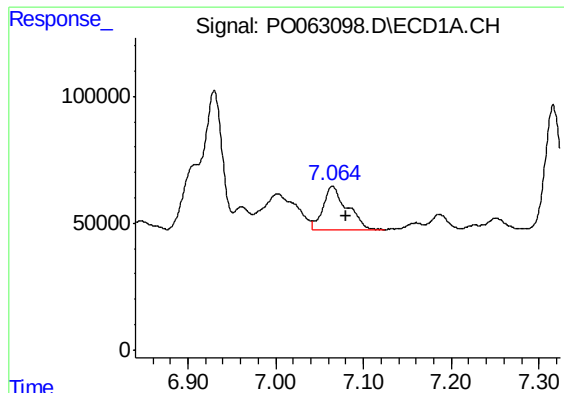


#31 AR-1260-1

R.T.: 7.065 min
Delta R.T.: -0.015 min
Response: 321554
Conc: 112.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
191-36-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:17 AM

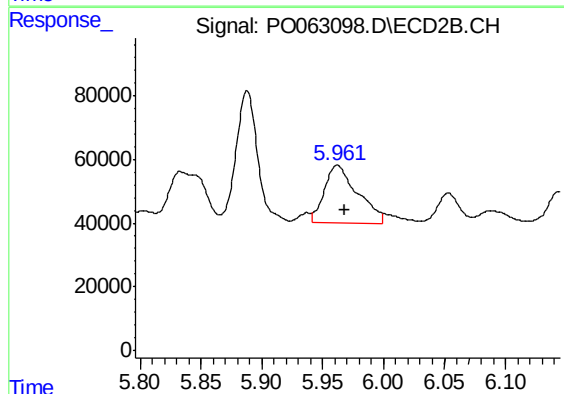


#31 AR-1260-1

R.T.: 5.961 min
Delta R.T.: -0.007 min
Response: 345621
Conc: 162.67 ng/ml m

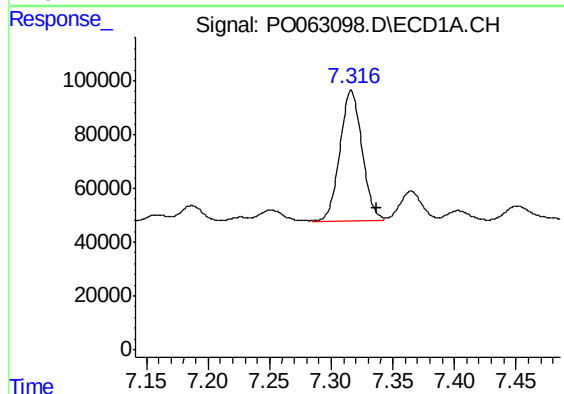


#32 AR-1260-2

R.T.: 7.316 min
Delta R.T.: -0.021 min
Response: 606400
Conc: 176.76 ng/ml m

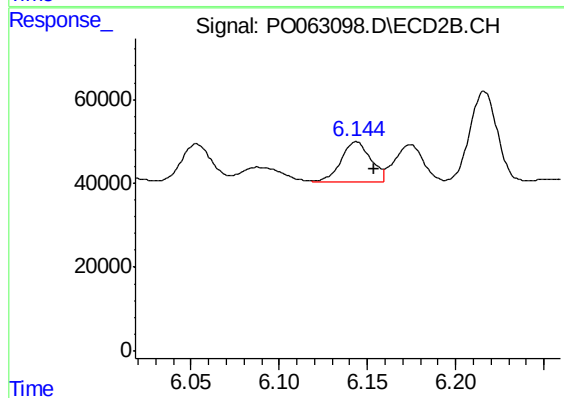

#32 AR-1260-2

R.T.: 6.144 min
Delta R.T.: -0.010 min
Response: 111654
Conc: 44.00 ng/ml

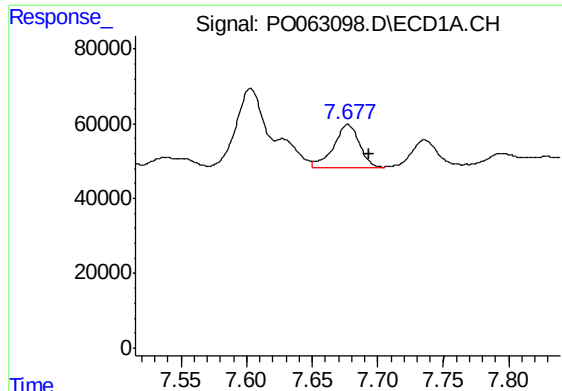


#33 AR-1260-3

R.T.: 7.677 min
Delta R.T.: -0.017 min
Response: 154796
Conc: 58.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
191-36-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:17 AM

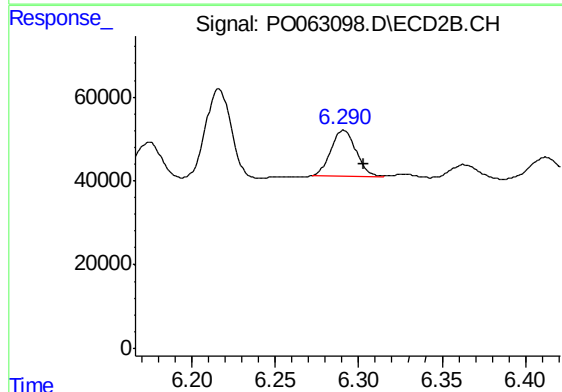


#33 AR-1260-3

R.T.: 6.291 min
Delta R.T.: -0.012 min
Response: 115804
Conc: 51.28 ng/ml

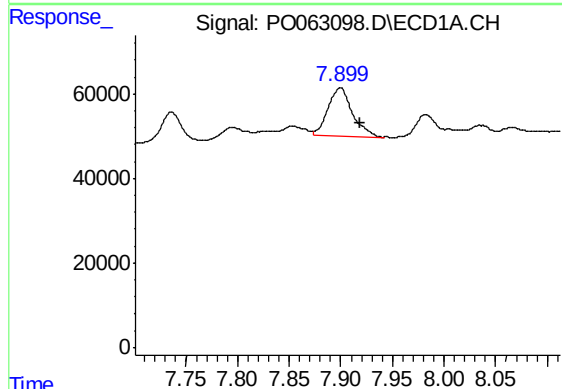


#34 AR-1260-4

R.T.: 7.899 min
Delta R.T.: -0.019 min
Response: 185897
Conc: 66.46 ng/ml m

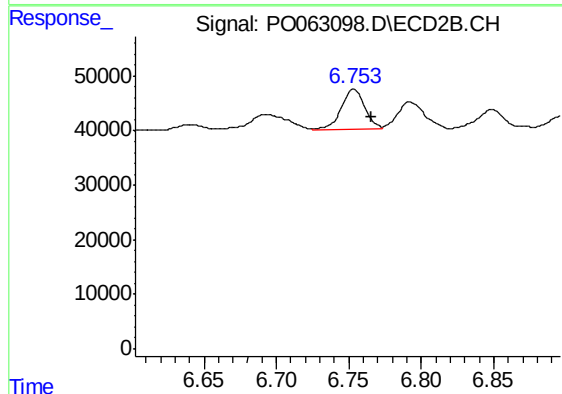

#34 AR-1260-4

R.T.: 6.753 min
Delta R.T.: -0.012 min
Response: 84382
Conc: 48.06 ng/ml

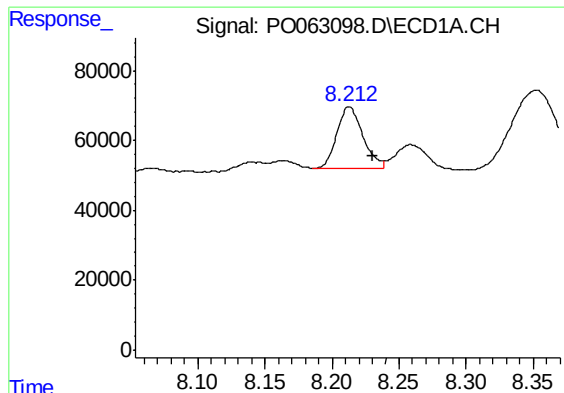


#35 AR-1260-5

R.T.: 8.213 min
Delta R.T.: -0.017 min
Response: 240265
Conc: 45.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
191-36-(0-1)

Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:17 AM

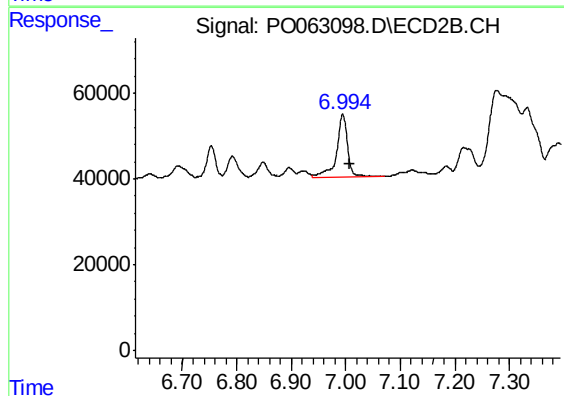

#35 AR-1260-5

R.T.: 6.995 min
Delta R.T.: -0.012 min
Response: 205182
Conc: 56.96 ng/ml