

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102319\
 Data File : P0063103.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 5:22
 Operator : HP/AJ
 Sample : K5498-01
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 189-62-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/24/2019 11:50:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 09:05:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.477	1327200	986528	21.459	23.006
2)	SA Decachlor...	9.935	8.325	1016173	530914	18.161	18.094
Target Compounds							
31)	L7 AR-1260-1	7.063	5.958	73776	33039	25.912	15.549 #
32)	L7 AR-1260-2	7.317	6.217	115529	27339	33.677m	10.773 #
33)	L7 AR-1260-3	7.677	6.291	46607	27785	17.613	12.305 #
34)	L7 AR-1260-4	7.899	6.755	71816	14463	25.676	8.237m#
35)	L7 AR-1260-5	8.212	6.995	55261	34237	10.555	9.504

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 5:22
Operator : HP/AJ
Sample : K5498-01
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
189-62-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 09:05:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

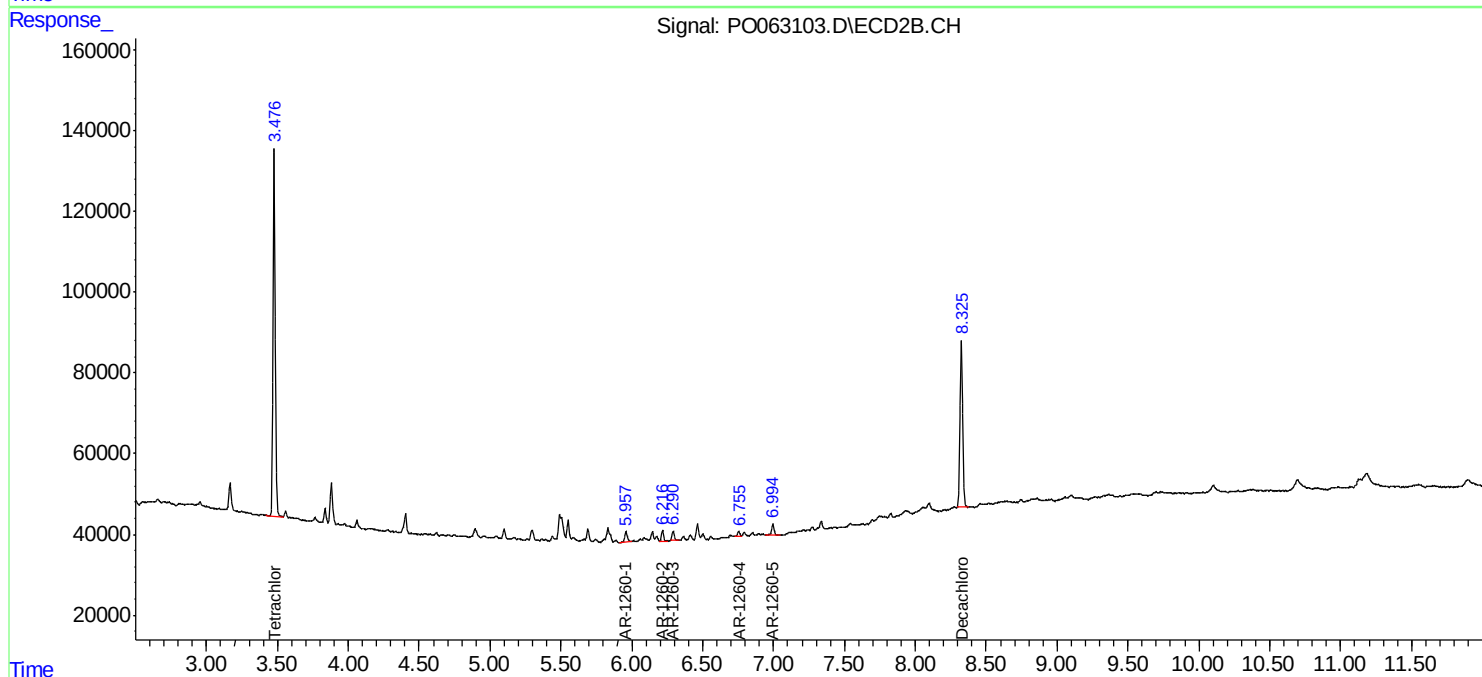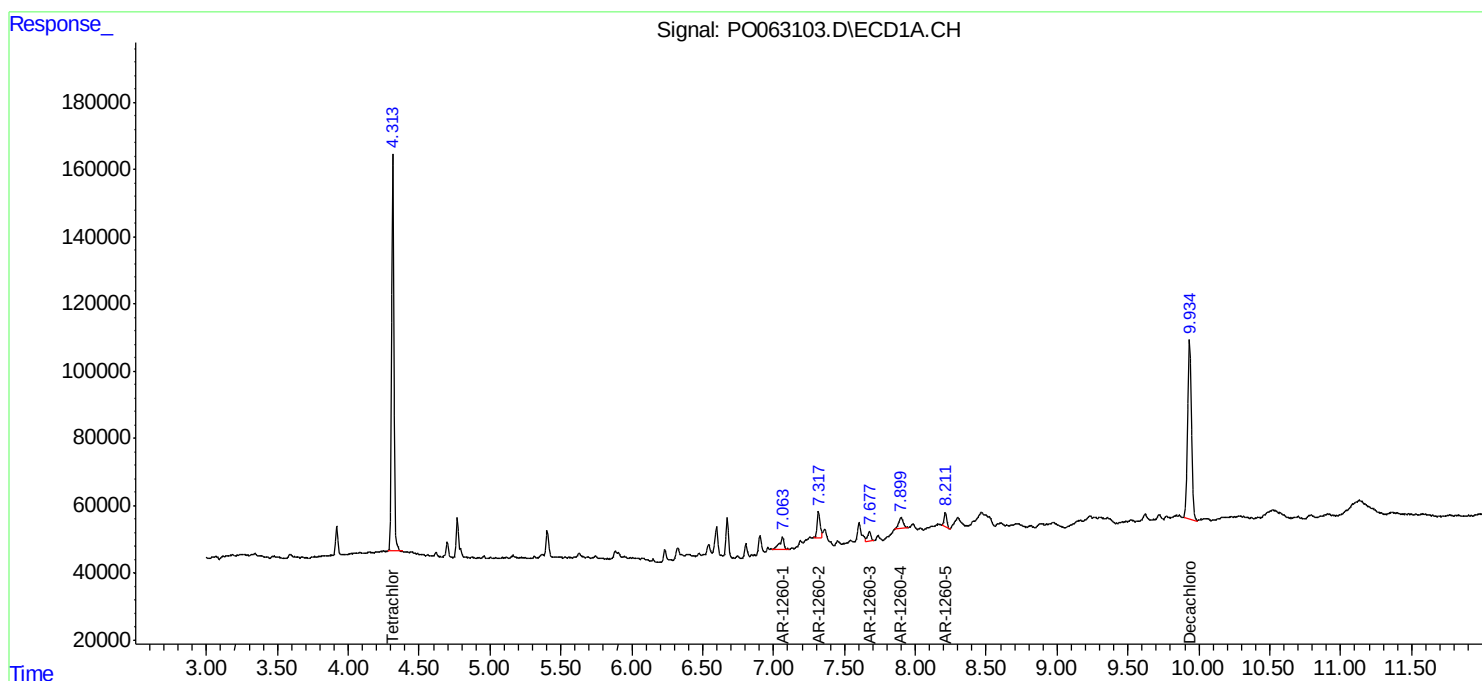

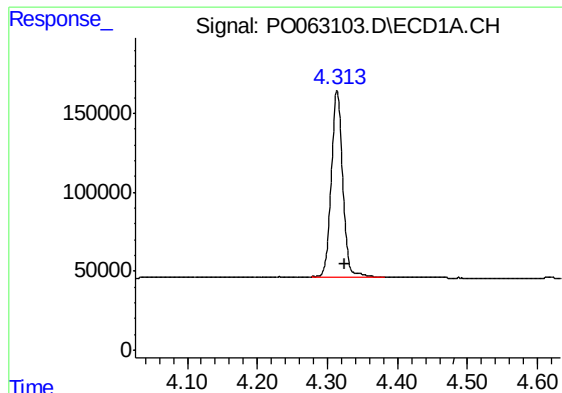


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: -0.011 min
Response: 1327200
Conc: 21.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
189-62-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:41 AM

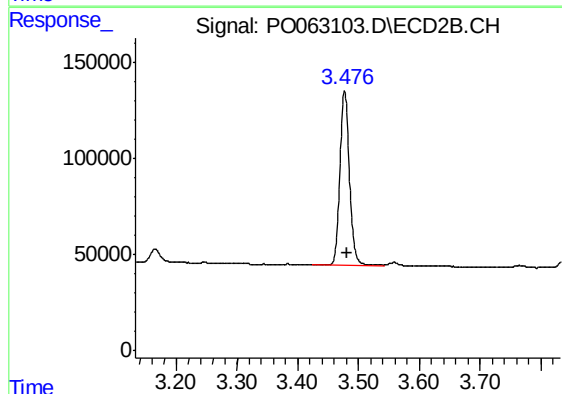


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.005 min
Response: 986528
Conc: 23.01 ng/ml

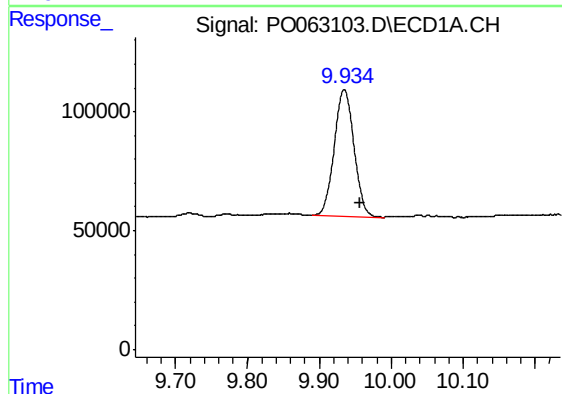


#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.022 min
Response: 1016173
Conc: 18.16 ng/ml

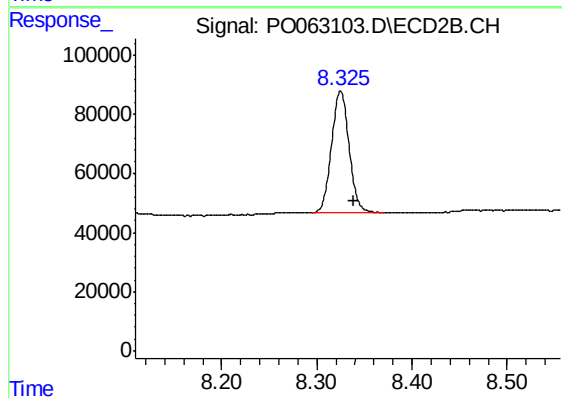

#2 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.013 min
Response: 530914
Conc: 18.09 ng/ml

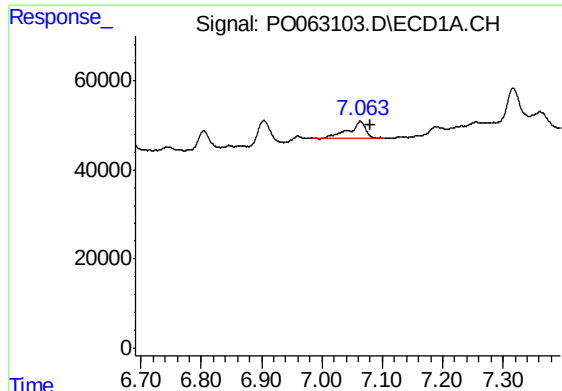


#31 AR-1260-1

R.T.: 7.063 min
Delta R.T.: -0.017 min
Response: 73776
Conc: 25.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
189-62-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:41 AM

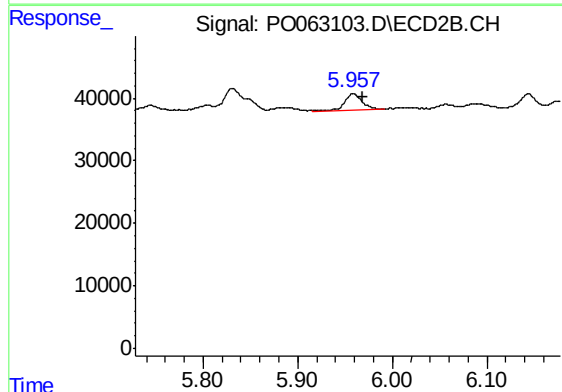


#31 AR-1260-1

R.T.: 5.958 min
Delta R.T.: -0.010 min
Response: 33039
Conc: 15.55 ng/ml

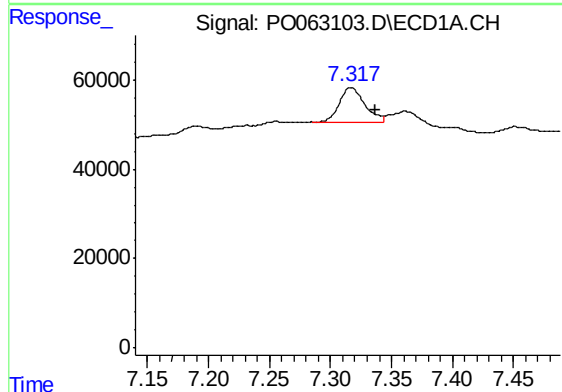


#32 AR-1260-2

R.T.: 7.317 min
Delta R.T.: -0.020 min
Response: 115529
Conc: 33.68 ng/ml m

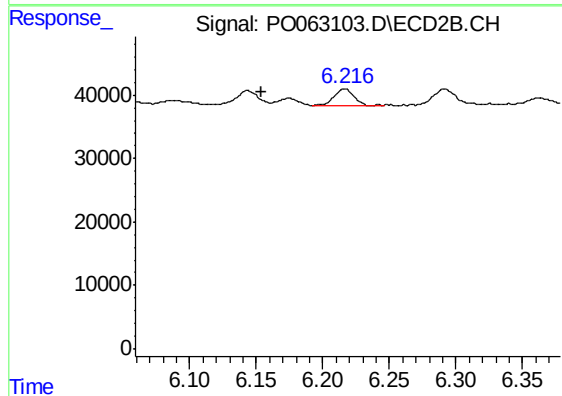

#32 AR-1260-2

R.T.: 6.217 min
Delta R.T.: 0.063 min
Response: 27339
Conc: 10.77 ng/ml

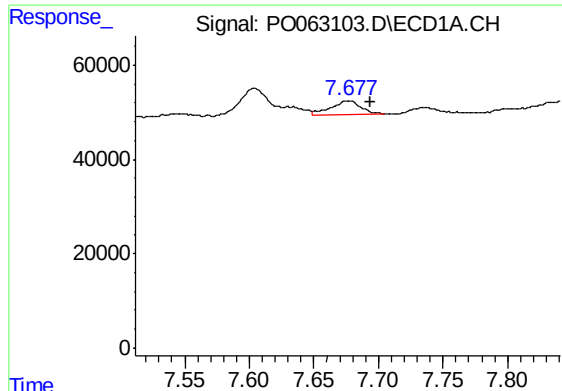


#33 AR-1260-3

R.T.: 7.677 min
Delta R.T.: -0.017 min
Response: 46607
Conc: 17.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
189-62-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:41 AM

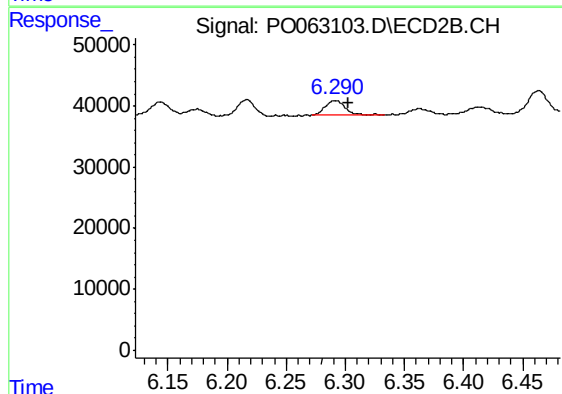


#33 AR-1260-3

R.T.: 6.291 min
Delta R.T.: -0.012 min
Response: 27785
Conc: 12.30 ng/ml

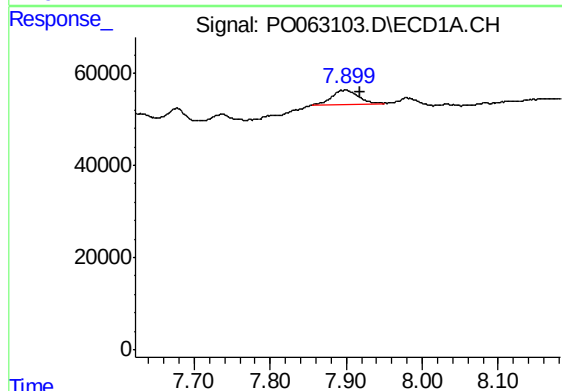


#34 AR-1260-4

R.T.: 7.899 min
Delta R.T.: -0.019 min
Response: 71816
Conc: 25.68 ng/ml

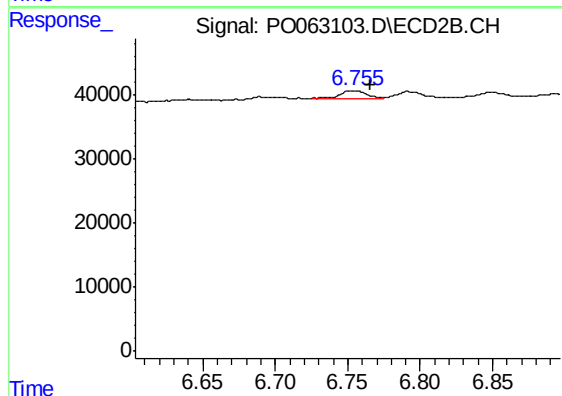

#34 AR-1260-4

R.T.: 6.755 min
Delta R.T.: -0.011 min
Response: 14463
Conc: 8.24 ng/ml m

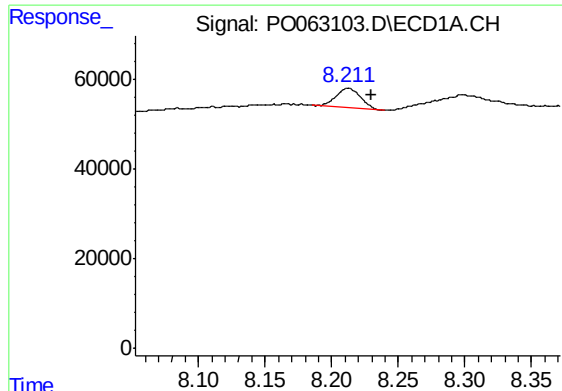


#35 AR-1260-5

R.T.: 8.212 min
Delta R.T.: -0.018 min
Response: 55261
Conc: 10.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
189-62-(0-1)

Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:41 AM

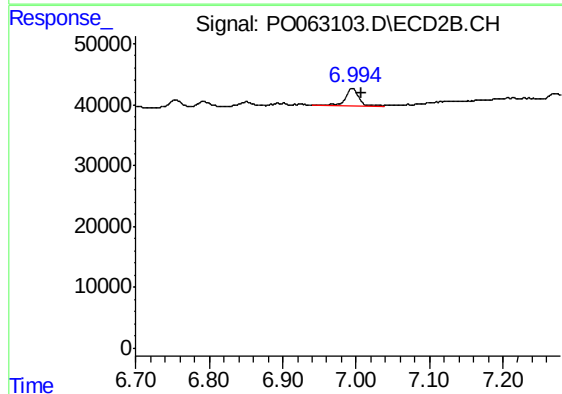

#35 AR-1260-5

R.T.: 6.995 min
Delta R.T.: -0.012 min
Response: 34237
Conc: 9.50 ng/ml