

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102319\
 Data File : P0063105.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 5:55
 Operator : HP/AJ
 Sample : K5498-05
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 190-78-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/24/2019 11:50:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 09:06:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.478	1347576	1086180	21.789	25.330
2)	SA Decachlor...	9.937	8.324	1120425	589679	20.025	20.097
Target Compounds							
31)	L7 AR-1260-1	7.065	5.959	75109	64024	26.381	30.133
32)	L7 AR-1260-2	7.318	6.129	108866	98956	31.734m	38.996
33)	L7 AR-1260-3	7.678	6.292	69335	47903	26.203	21.214
34)	L7 AR-1260-4	7.903	6.755	90011	36517	32.181	20.798 #
35)	L7 AR-1260-5	8.214	6.996	114408	84657	21.852	23.500

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102319\
Data File : PO063105.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 5:55
Operator : HP/AJ
Sample : K5498-05
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
190-78-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 09:06:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

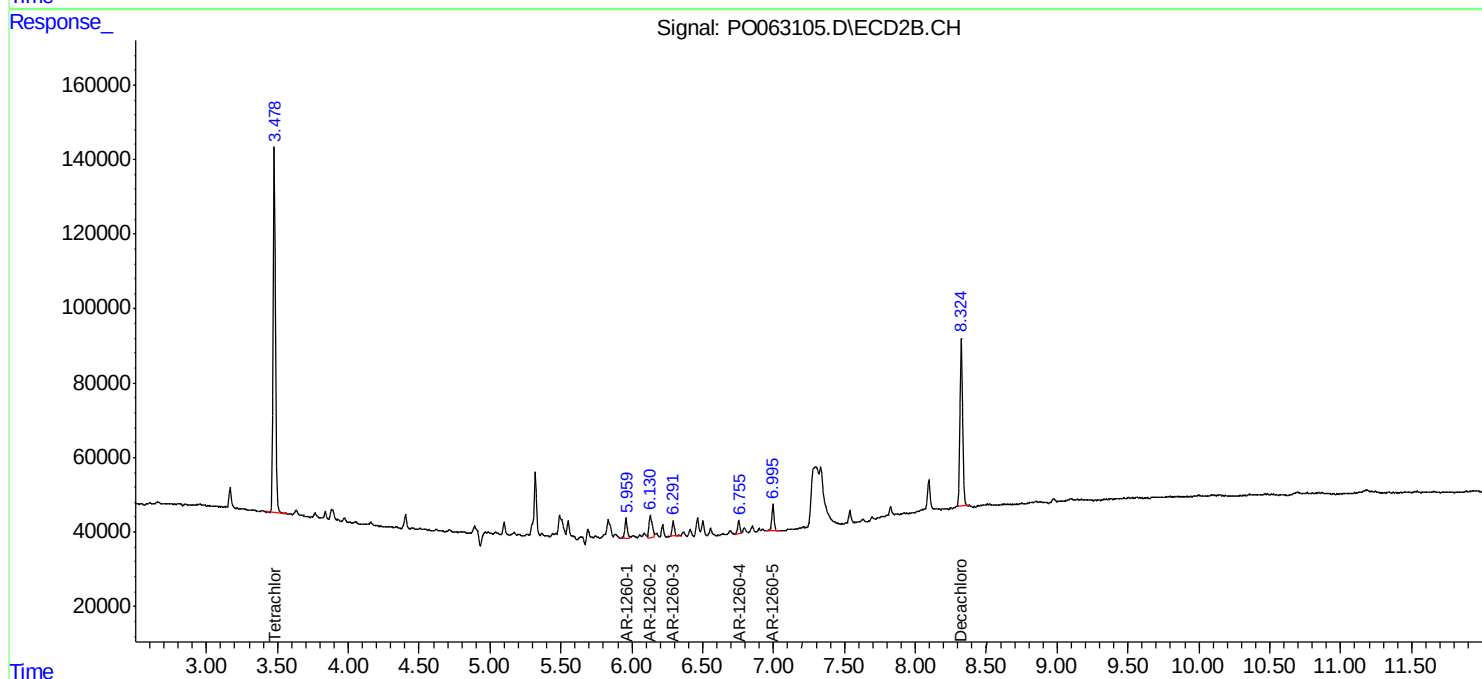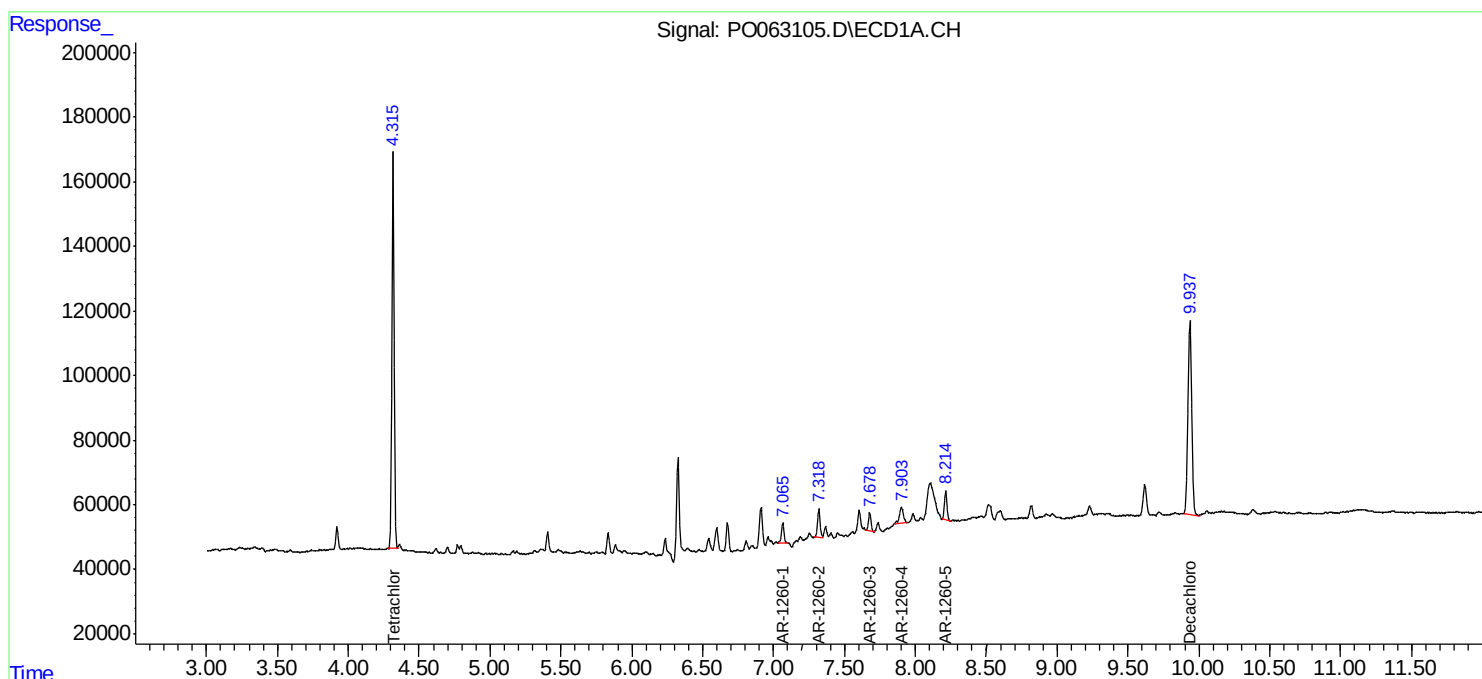

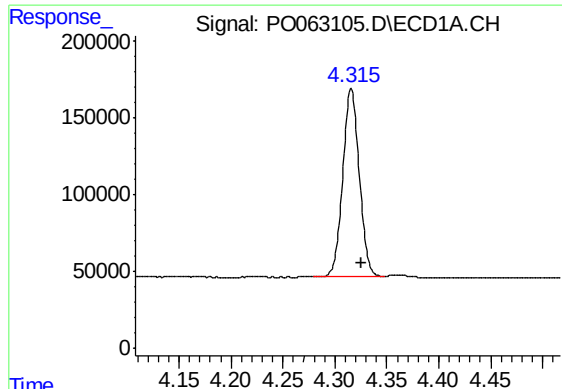


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.009 min
Response: 1347576
Conc: 21.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
190-78-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:45 AM

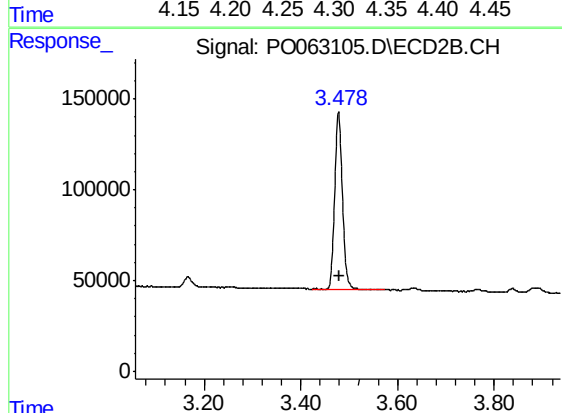


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: -0.003 min
Response: 1086180
Conc: 25.33 ng/ml

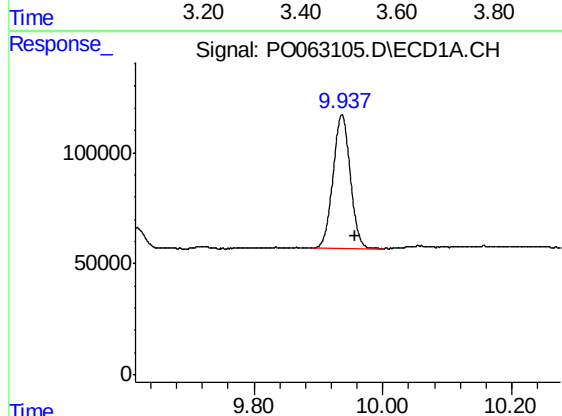


#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.020 min
Response: 1120425
Conc: 20.02 ng/ml

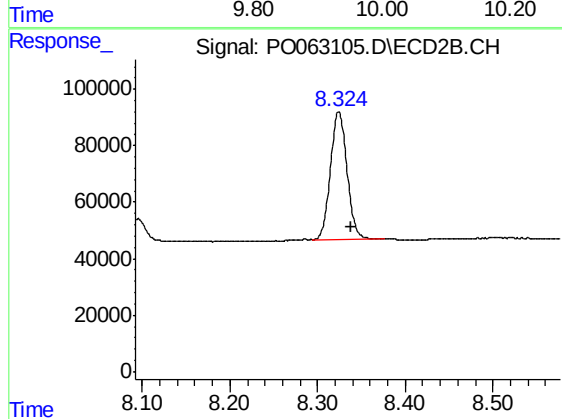

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.014 min
Response: 589679
Conc: 20.10 ng/ml

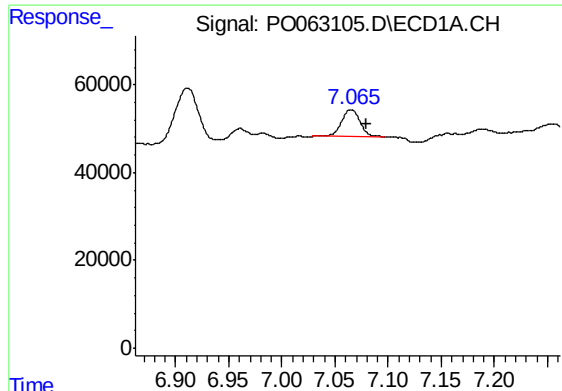


#31 AR-1260-1

R.T.: 7.065 min
Delta R.T.: -0.015 min
Response: 75109
Conc: 26.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
190-78-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:45 AM

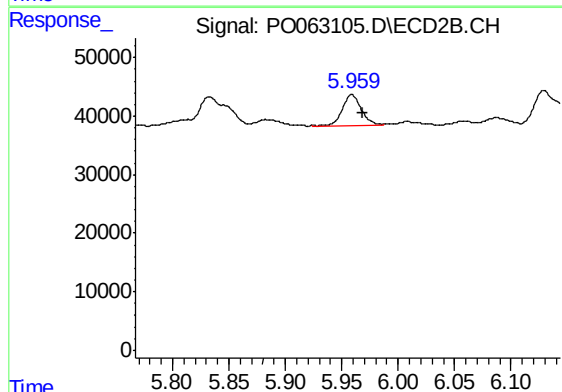


#31 AR-1260-1

R.T.: 5.959 min
Delta R.T.: -0.009 min
Response: 64024
Conc: 30.13 ng/ml

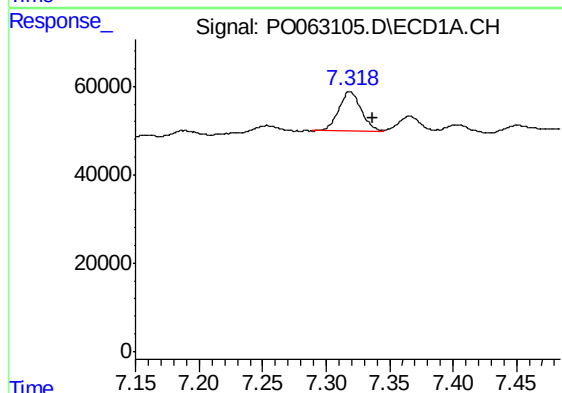


#32 AR-1260-2

R.T.: 7.318 min
Delta R.T.: -0.019 min
Response: 108866
Conc: 31.73 ng/ml m

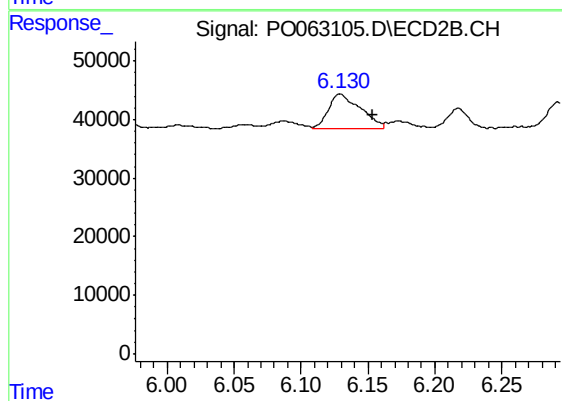

#32 AR-1260-2

R.T.: 6.129 min
Delta R.T.: -0.025 min
Response: 98956
Conc: 39.00 ng/ml

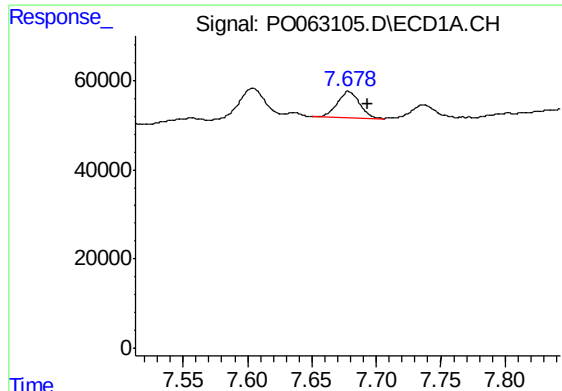


#33 AR-1260-3

R.T.: 7.678 min
Delta R.T.: -0.015 min
Response: 69335
Conc: 26.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
190-78-(0-1)


Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:45 AM

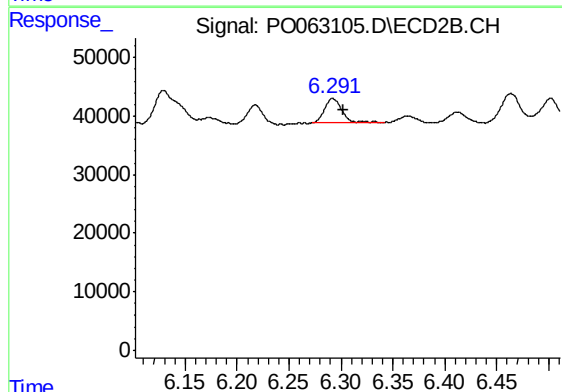


#33 AR-1260-3

R.T.: 6.292 min
Delta R.T.: -0.011 min
Response: 47903
Conc: 21.21 ng/ml

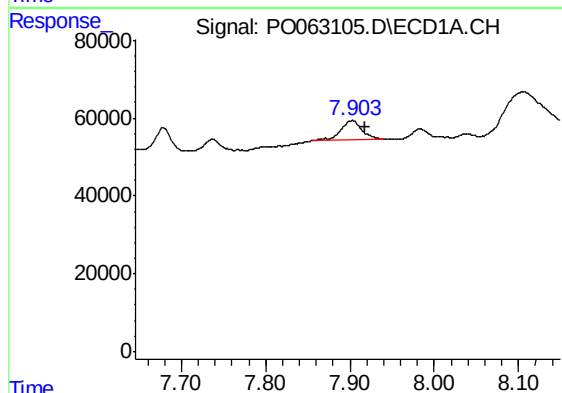


#34 AR-1260-4

R.T.: 7.903 min
Delta R.T.: -0.016 min
Response: 90011
Conc: 32.18 ng/ml

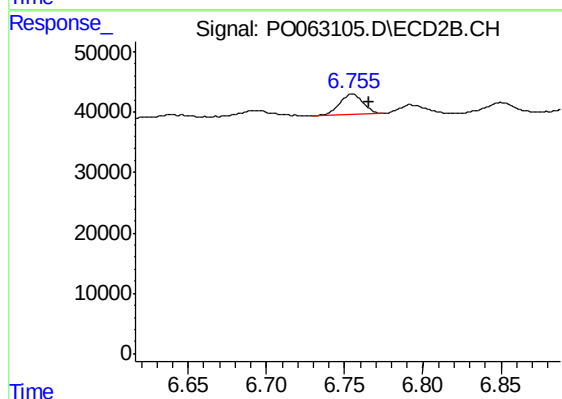

#34 AR-1260-4

R.T.: 6.755 min
Delta R.T.: -0.011 min
Response: 36517
Conc: 20.80 ng/ml

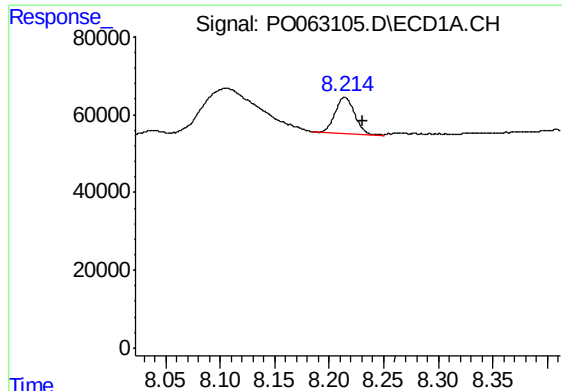


#35 AR-1260-5

R.T.: 8.214 min
Delta R.T.: -0.016 min
Response: 114408
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
190-78-(0-1)

Manual Integrations
APPROVED

Ankita
10/24/2019 11:50:45 AM

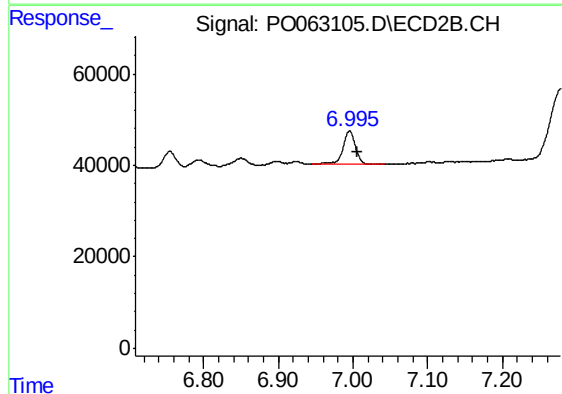

#35 AR-1260-5

R.T.: 6.996 min
Delta R.T.: -0.011 min
Response: 84657
Conc: 23.50 ng/ml