

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102419\
 Data File : P0063114.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 11:49
 Operator : HP/AJ
 Sample : K5497-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 170-48-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/25/2019 10:52:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:04:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.325	3.486	1131461	839577	18.294	19.579
2)	SA Decachlor...	9.950	8.333	1367743	727151	24.445	24.782
Target Compounds							
31)	L7 AR-1260-1	7.074	5.967	31296	61503	10.992m	28.946m#
32)	L7 AR-1260-2	7.331	6.152	73943	114448	21.554	45.100 #
33)	L7 AR-1260-3	7.688	6.301	43991	39040	16.625	17.289
34)	L7 AR-1260-4	7.911	6.763	92654	42519	33.126m	24.215 #
35)	L7 AR-1260-5	8.225	7.004	86192	75562	16.463	20.975 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102419\
Data File : PO063114.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 11:49
Operator : HP/AJ
Sample : K5497-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
170-48-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:52:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:04:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

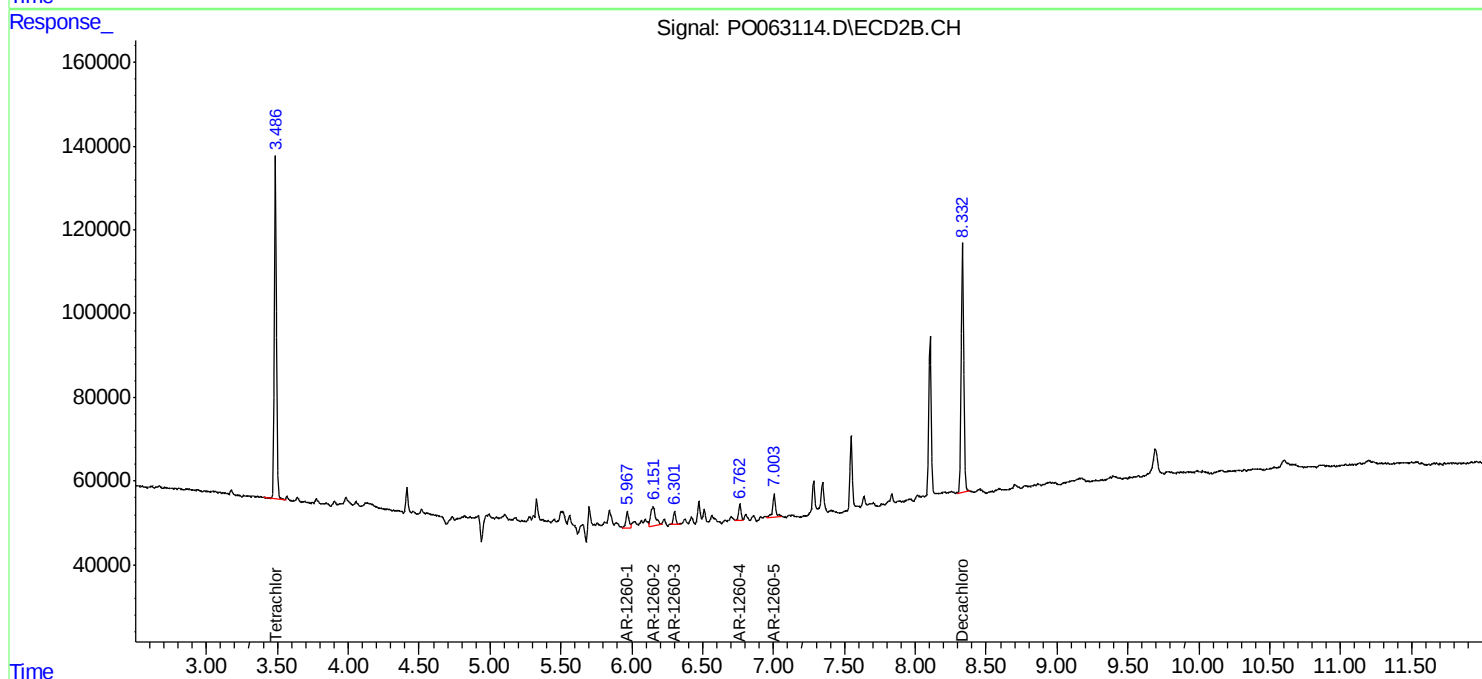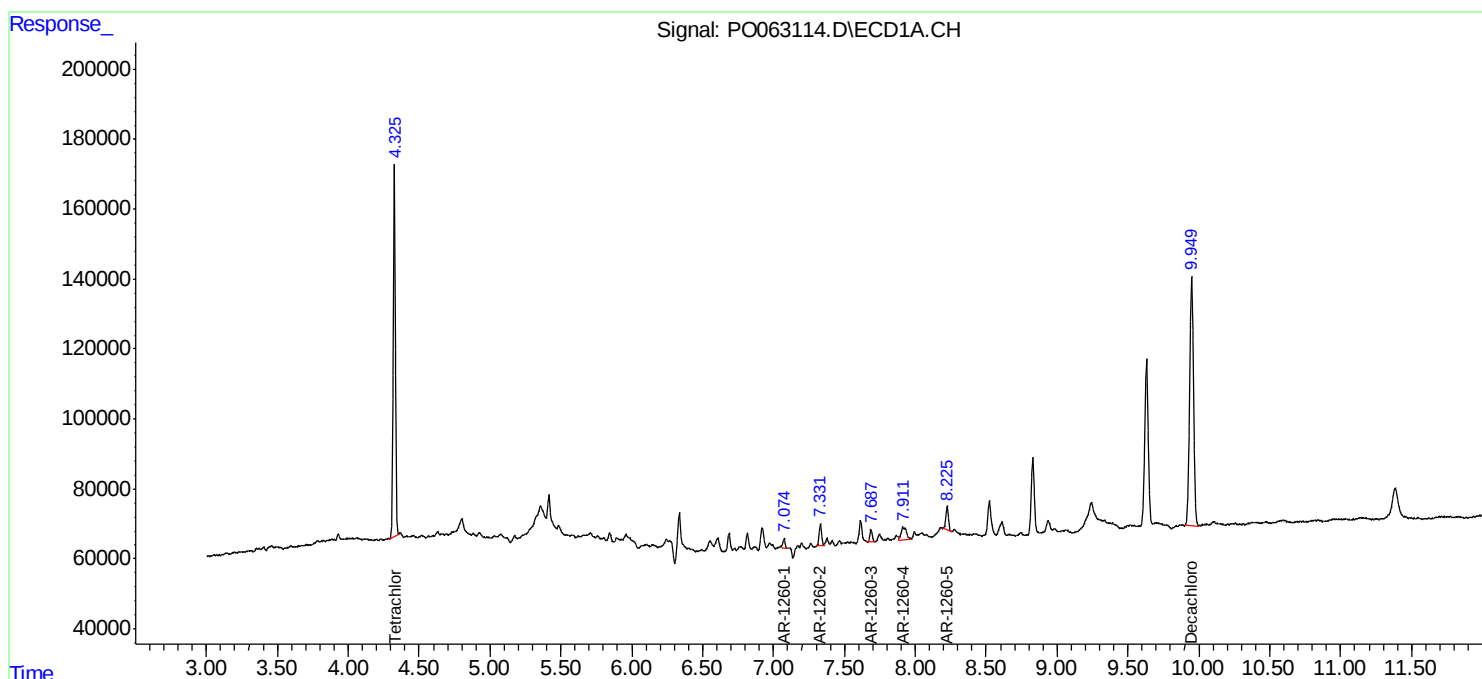

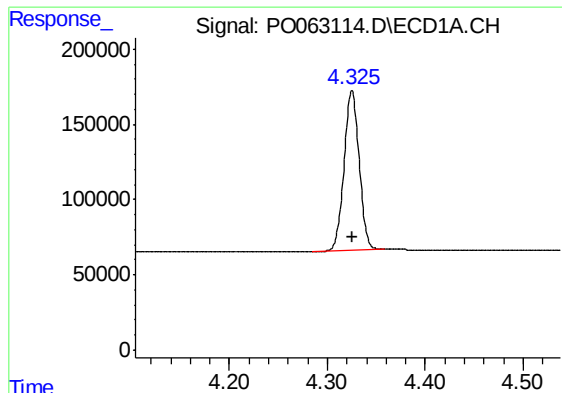


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 1131461
Conc: 18.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
170-48-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:52:22 AM

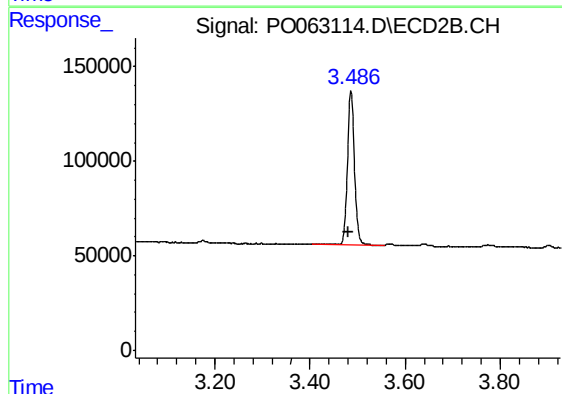


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: 0.005 min
Response: 839577
Conc: 19.58 ng/ml

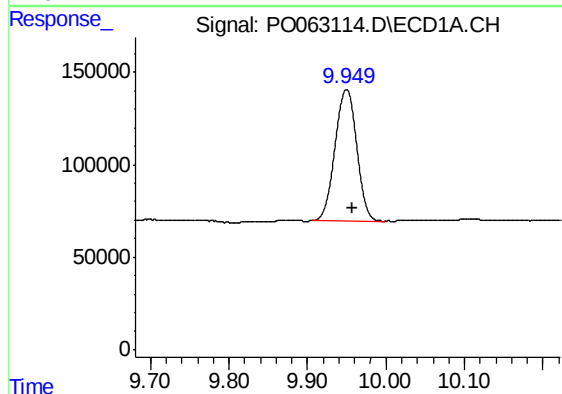


#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.007 min
Response: 1367743
Conc: 24.44 ng/ml

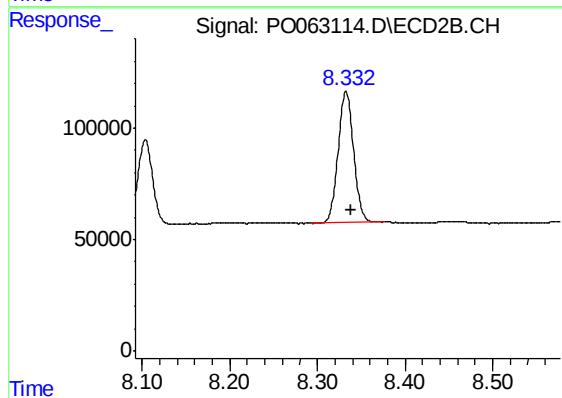

#2 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: -0.005 min
Response: 727151
Conc: 24.78 ng/ml

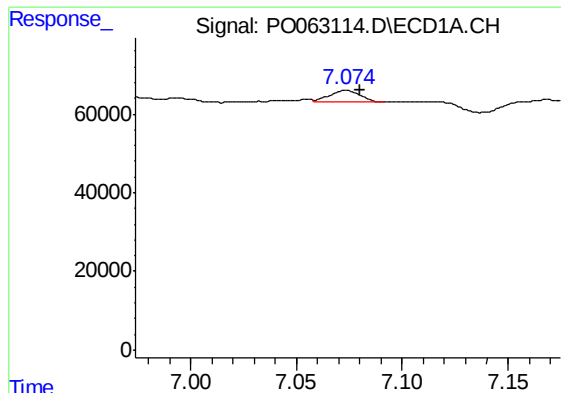


#31 AR-1260-1

R.T.: 7.074 min
Delta R.T.: -0.006 min
Response: 31296
Conc: 10.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
170-48-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:52:22 AM

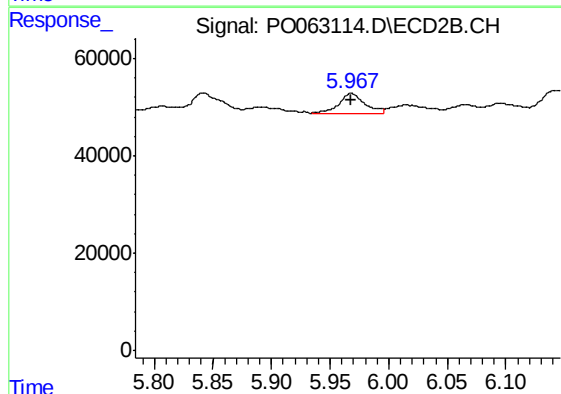


#31 AR-1260-1

R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 61503
Conc: 28.95 ng/ml m

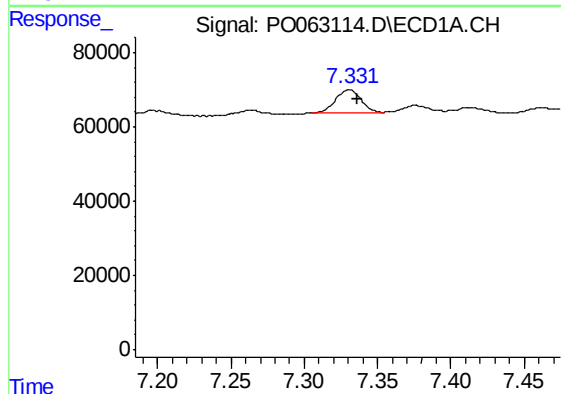


#32 AR-1260-2

R.T.: 7.331 min
Delta R.T.: -0.006 min
Response: 73943
Conc: 21.55 ng/ml

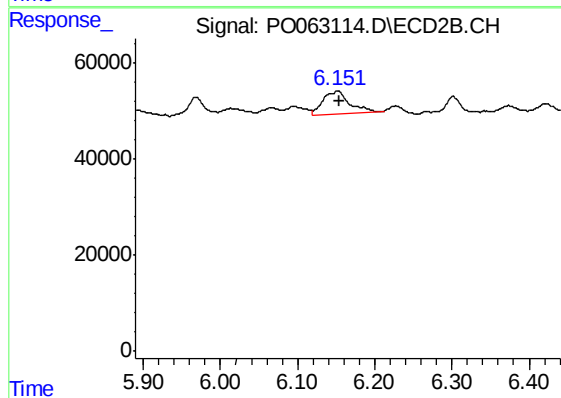

#32 AR-1260-2

R.T.: 6.152 min
Delta R.T.: -0.002 min
Response: 114448
Conc: 45.10 ng/ml

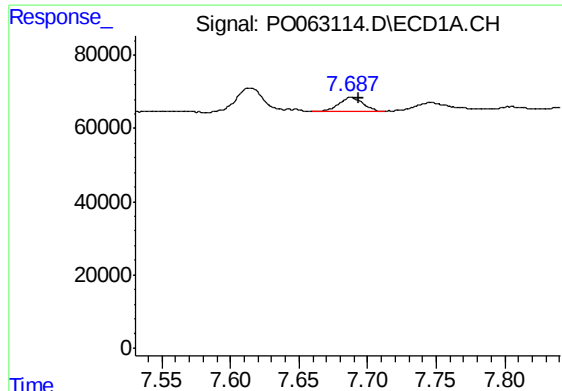


#33 AR-1260-3

R.T.: 7.688 min
Delta R.T.: -0.006 min
Response: 43991
Conc: 16.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
170-48-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:52:22 AM

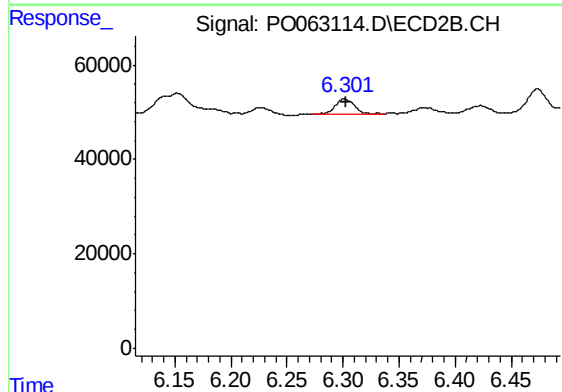


#33 AR-1260-3

R.T.: 6.301 min
Delta R.T.: -0.002 min
Response: 39040
Conc: 17.29 ng/ml

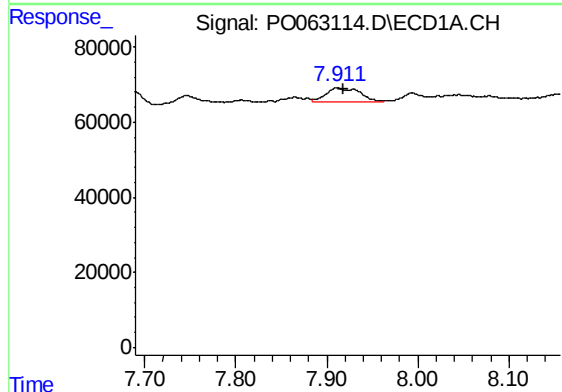


#34 AR-1260-4

R.T.: 7.911 min
Delta R.T.: -0.008 min
Response: 92654
Conc: 33.13 ng/ml m

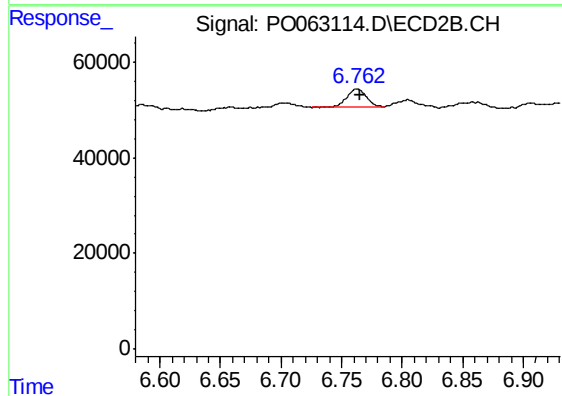

#34 AR-1260-4

R.T.: 6.763 min
Delta R.T.: -0.003 min
Response: 42519
Conc: 24.22 ng/ml

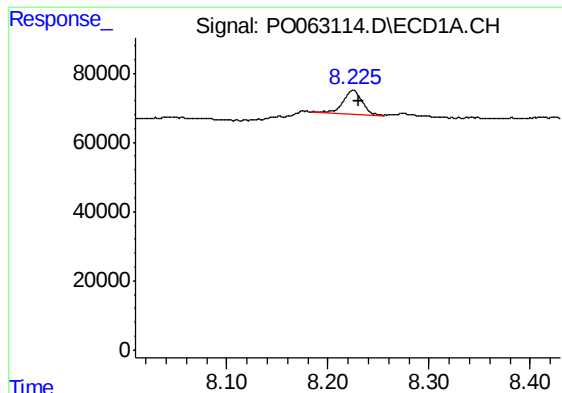


#35 AR-1260-5

R.T.: 8.225 min
Delta R.T.: -0.005 min
Response: 86192
Conc: 16.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
170-48-(0-1)

Manual Integrations
APPROVED

Ankita
10/25/2019 10:52:22 AM

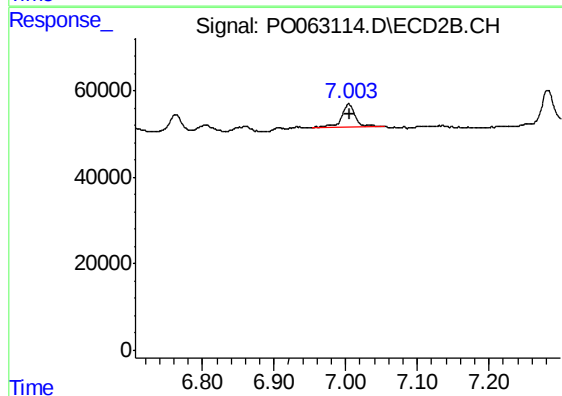

#35 AR-1260-5

R.T.: 7.004 min
Delta R.T.: -0.002 min
Response: 75562
Conc: 20.98 ng/ml