

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102419\
 Data File : P0063121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 16:22
 Operator : HP/AJ
 Sample : PB124250BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB124250BL

Manual Integrations
 APPROVED

Ankita
 10/25/2019 10:52:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:07:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.477	838640	581522	13.560m	13.561
2) SA Decachlor...	9.947	8.327	963630	522534	17.222	17.809

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102419\
Data File : PO063121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 16:22
Operator : HP/AJ
Sample : PB124250BL
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB124250BL


Manual Integrations
APPROVED

Ankita
10/25/2019 10:52:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:07:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

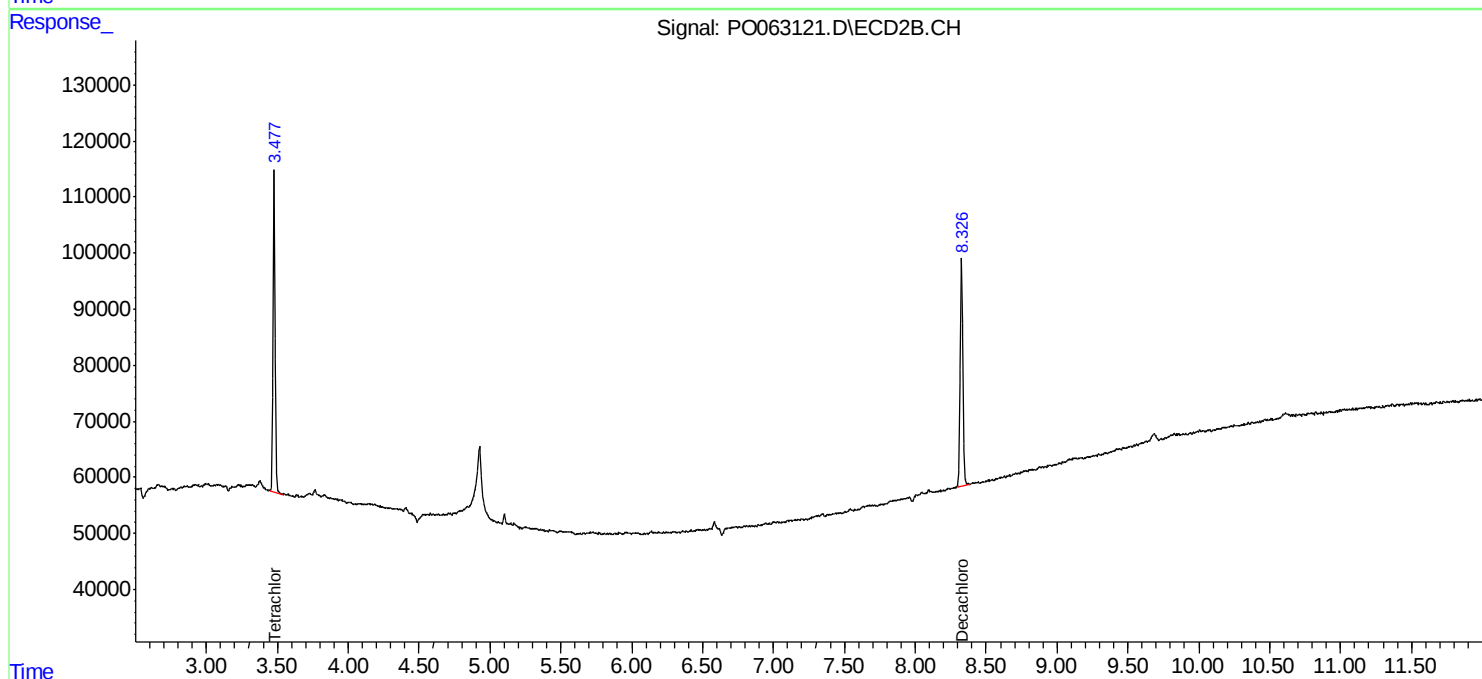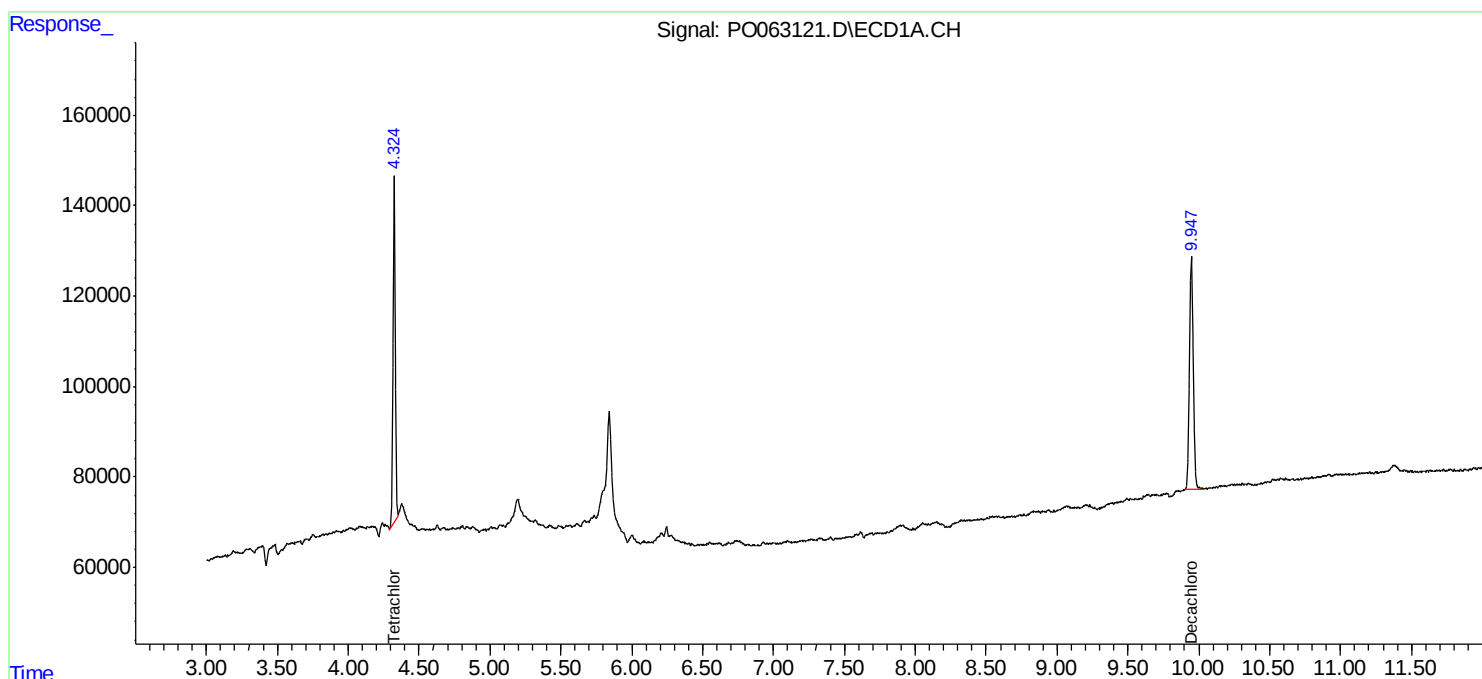

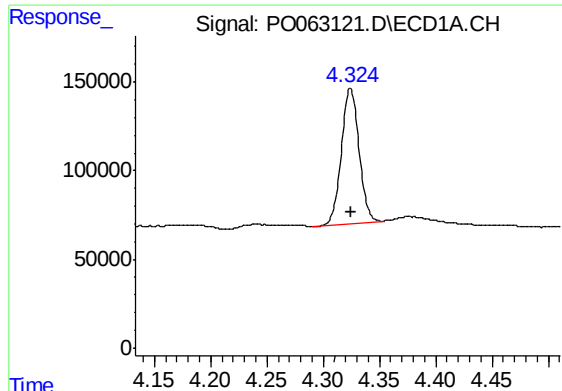


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.001 min
Response: 838640
Conc: 13.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB124250BL


Manual Integrations
APPROVED

Ankita
10/25/2019 10:52:44 AM

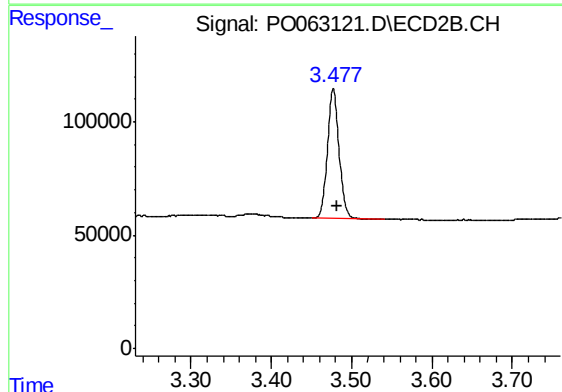


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.004 min
Response: 581522
Conc: 13.56 ng/ml

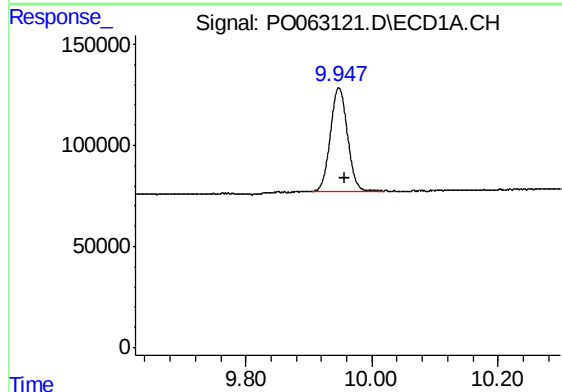

#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.009 min
Response: 963630
Conc: 17.22 ng/ml

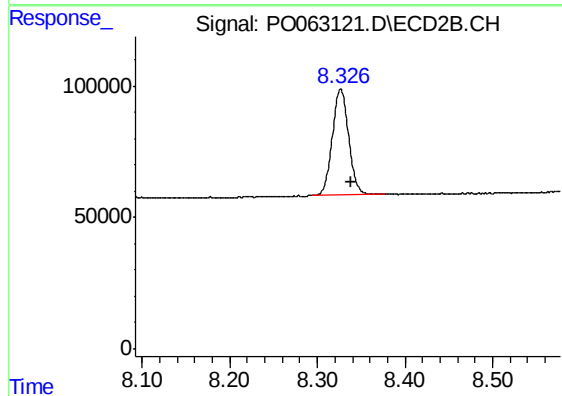

#2 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.011 min
Response: 522534
Conc: 17.81 ng/ml