

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102419\
 Data File : P0063128.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2019 18:16
 Operator : HP/AJ
 Sample : K5499-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 197-16-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/25/2019 10:53:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:10:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.313	3.476	731964	536997	11.835	12.523
2)	SA Decachlor...	9.932	8.321	474964	256496	8.489m	8.742
Target Compounds							
31)	L7 AR-1260-1	7.064	5.957	77102	61811	27.081	29.091
32)	L7 AR-1260-2	7.316	6.143	252639	56204	73.644m	22.148 #
33)	L7 AR-1260-3	7.677	6.290	48776	42421	18.433	18.786
34)	L7 AR-1260-4	7.902	6.753	56535	27306	20.212m	15.551
35)	L7 AR-1260-5	8.213	6.994	72648	68075	13.876	18.897 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102419\
Data File : PO063128.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2019 18:16
Operator : HP/AJ
Sample : K5499-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
197-16-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:53:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:10:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

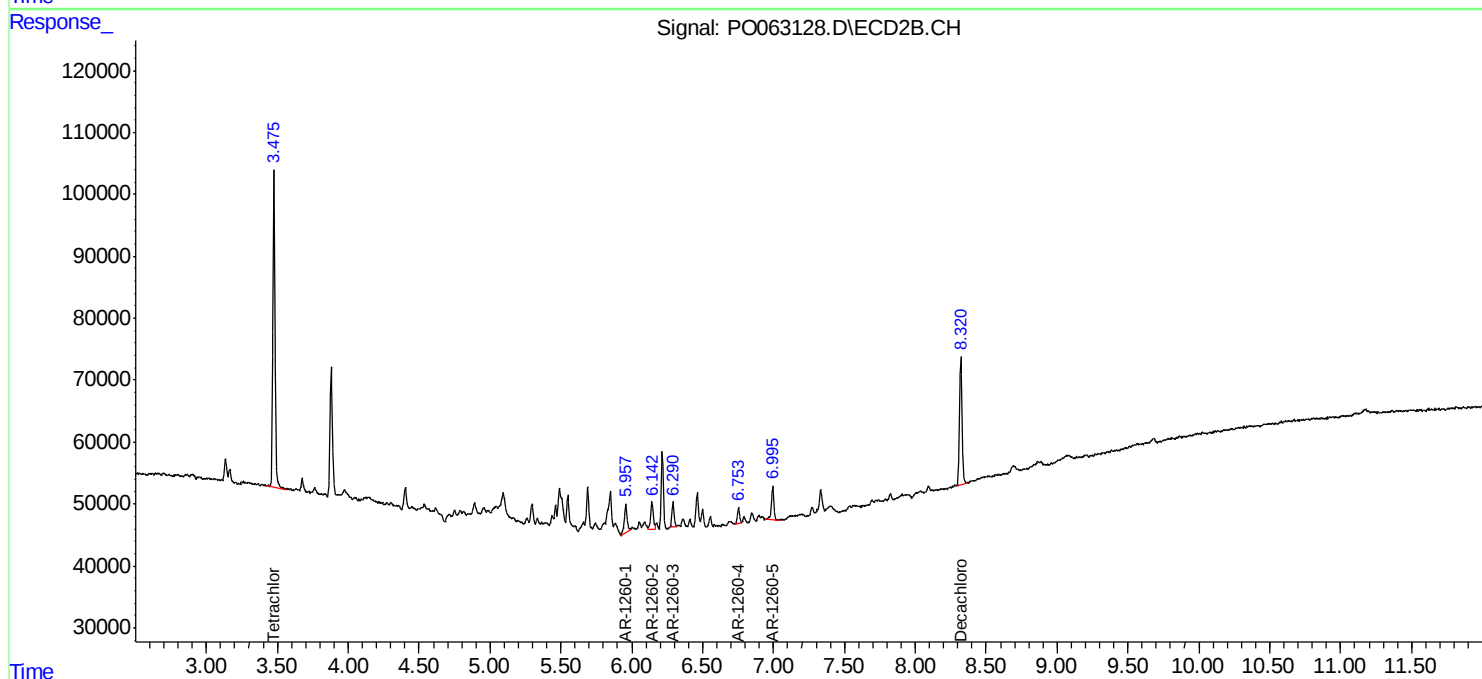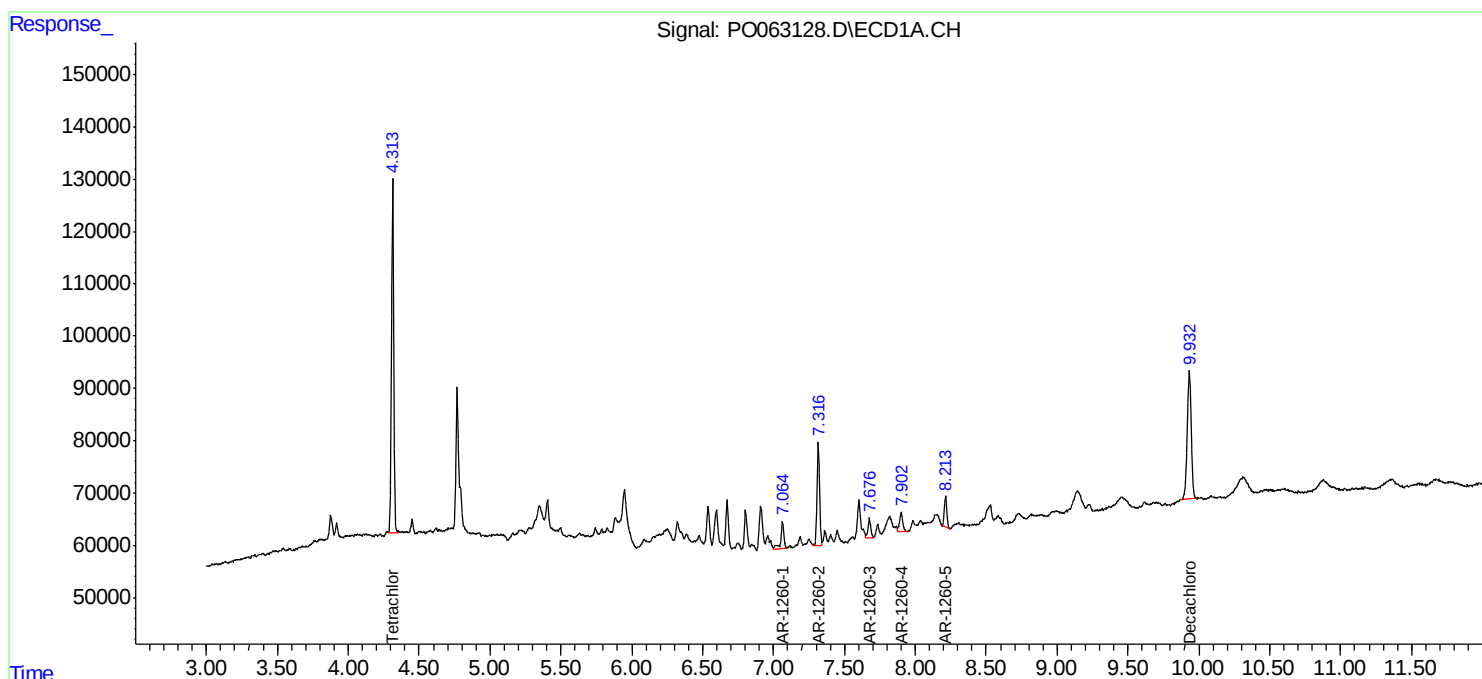

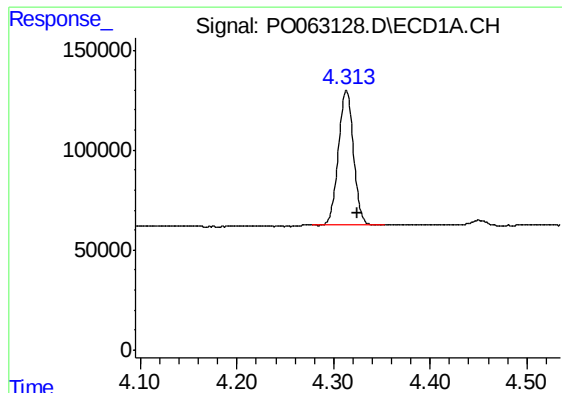


#1 Tetrachloro-m-xylene

R.T.: 4.313 min
Delta R.T.: -0.012 min
Response: 731964
Conc: 11.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
197-16-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:53:14 AM

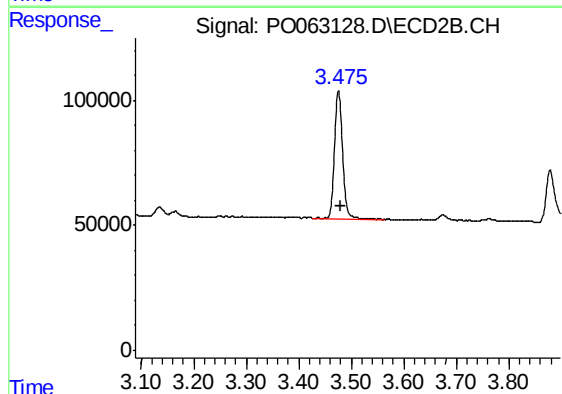


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.006 min
Response: 536997
Conc: 12.52 ng/ml

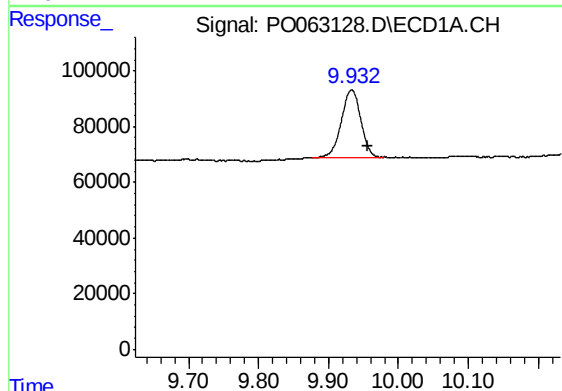


#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.024 min
Response: 474964
Conc: 8.49 ng/ml m

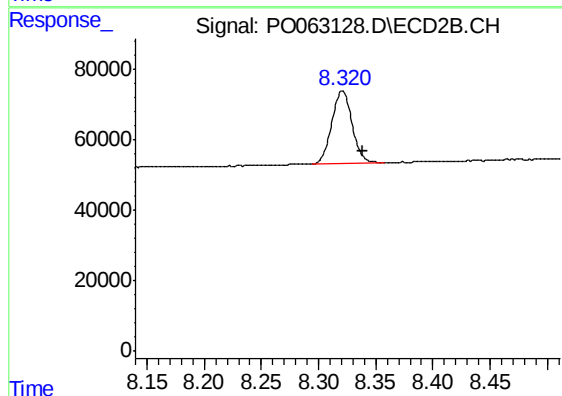

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.017 min
Response: 256496
Conc: 8.74 ng/ml

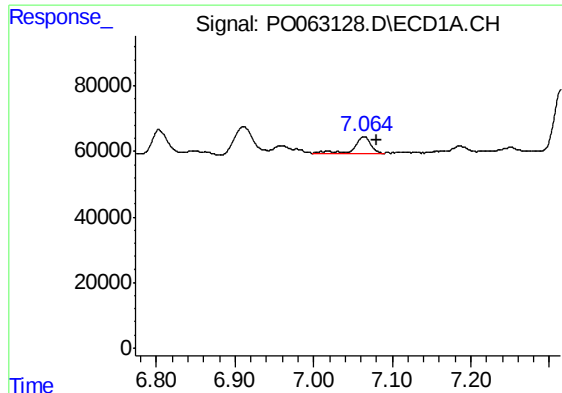


#31 AR-1260-1

R.T.: 7.064 min
Delta R.T.: -0.016 min
Response: 77102
Conc: 27.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
197-16-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:53:14 AM

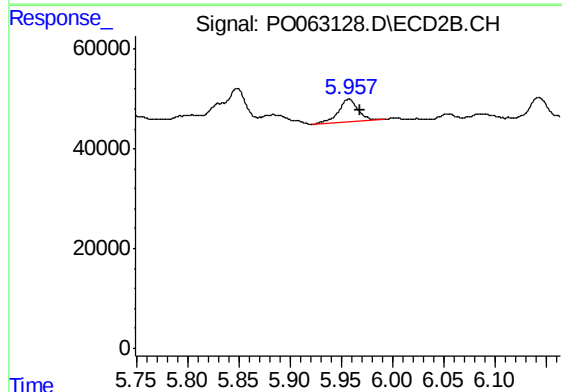


#31 AR-1260-1

R.T.: 5.957 min
Delta R.T.: -0.011 min
Response: 61811
Conc: 29.09 ng/ml

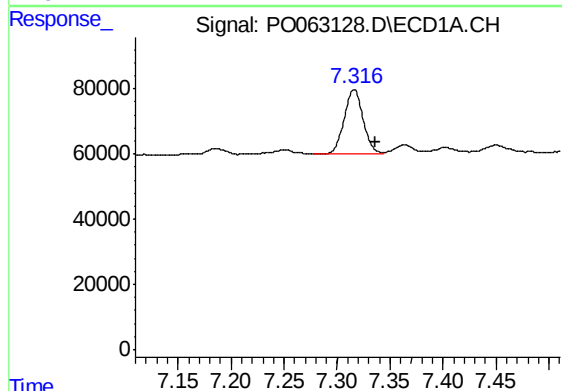


#32 AR-1260-2

R.T.: 7.316 min
Delta R.T.: -0.021 min
Response: 252639
Conc: 73.64 ng/ml m

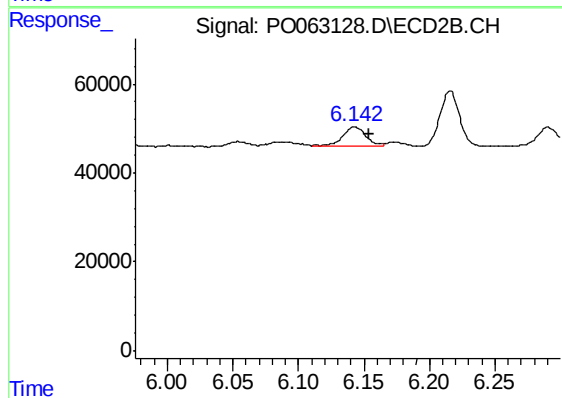

#32 AR-1260-2

R.T.: 6.143 min
Delta R.T.: -0.011 min
Response: 56204
Conc: 22.15 ng/ml

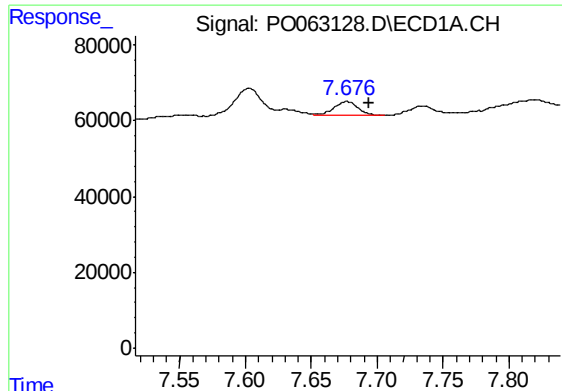


#33 AR-1260-3

R.T.: 7.677 min
Delta R.T.: -0.017 min
Response: 48776
Conc: 18.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
197-16-(0-1)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:53:14 AM

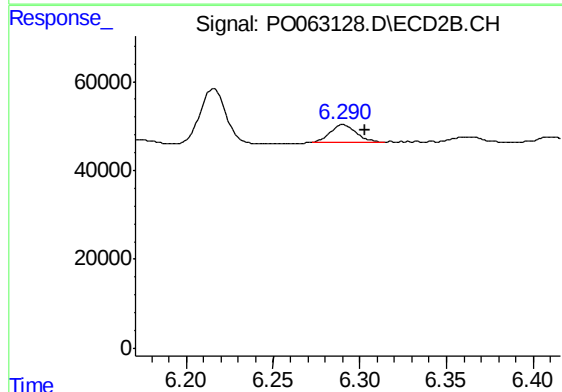


#33 AR-1260-3

R.T.: 6.290 min
Delta R.T.: -0.013 min
Response: 42421
Conc: 18.79 ng/ml

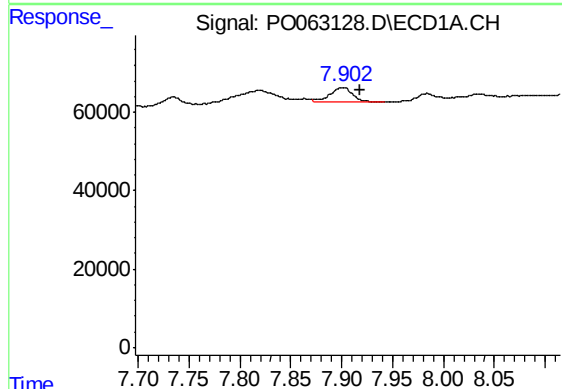


#34 AR-1260-4

R.T.: 7.902 min
Delta R.T.: -0.017 min
Response: 56535
Conc: 20.21 ng/ml m

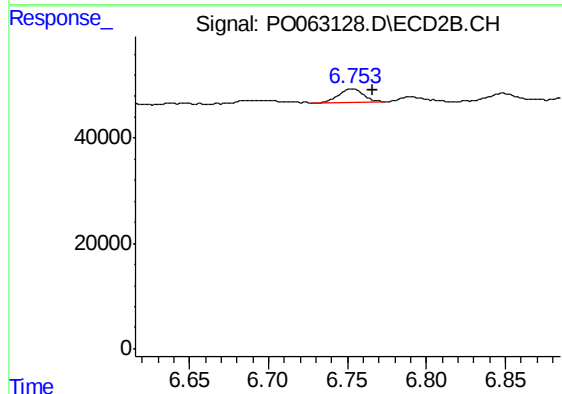

#34 AR-1260-4

R.T.: 6.753 min
Delta R.T.: -0.012 min
Response: 27306
Conc: 15.55 ng/ml

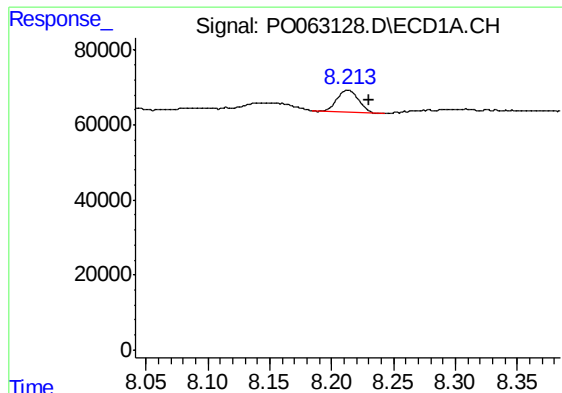


#35 AR-1260-5

R.T.: 8.213 min
Delta R.T.: -0.017 min
Response: 72648
Conc: 13.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
197-16-(0-1)

Manual Integrations
APPROVED

Ankita
10/25/2019 10:53:14 AM

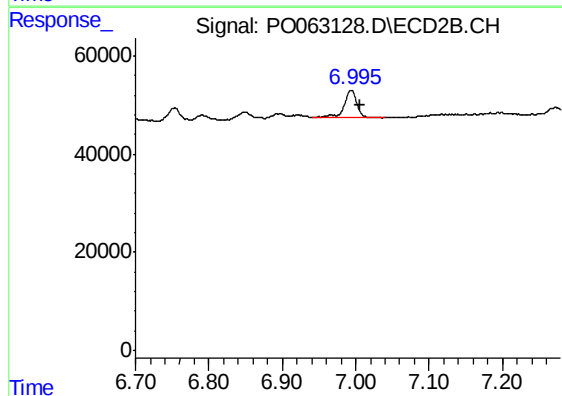

#35 AR-1260-5

R.T.: 6.994 min
Delta R.T.: -0.012 min
Response: 68075
Conc: 18.90 ng/ml