

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102519\
 Data File : P0063155.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2019 12:08
 Operator : HP/AJ
 Sample : K5502-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 179-18-(0-2.1)

Manual Integrations
 APPROVED

Ankita
 10/28/2019 10:48:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:11:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.478	938235	748913	15.170	17.465
2)	SA Decachlor...	9.935	8.322	614580	321707	10.984m	10.964

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102519\
Data File : PO063155.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2019 12:08
Operator : HP/AJ
Sample : K5502-11
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
179-18-(0-2.1)


Manual Integrations
APPROVED

Ankita
10/28/2019 10:48:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:11:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

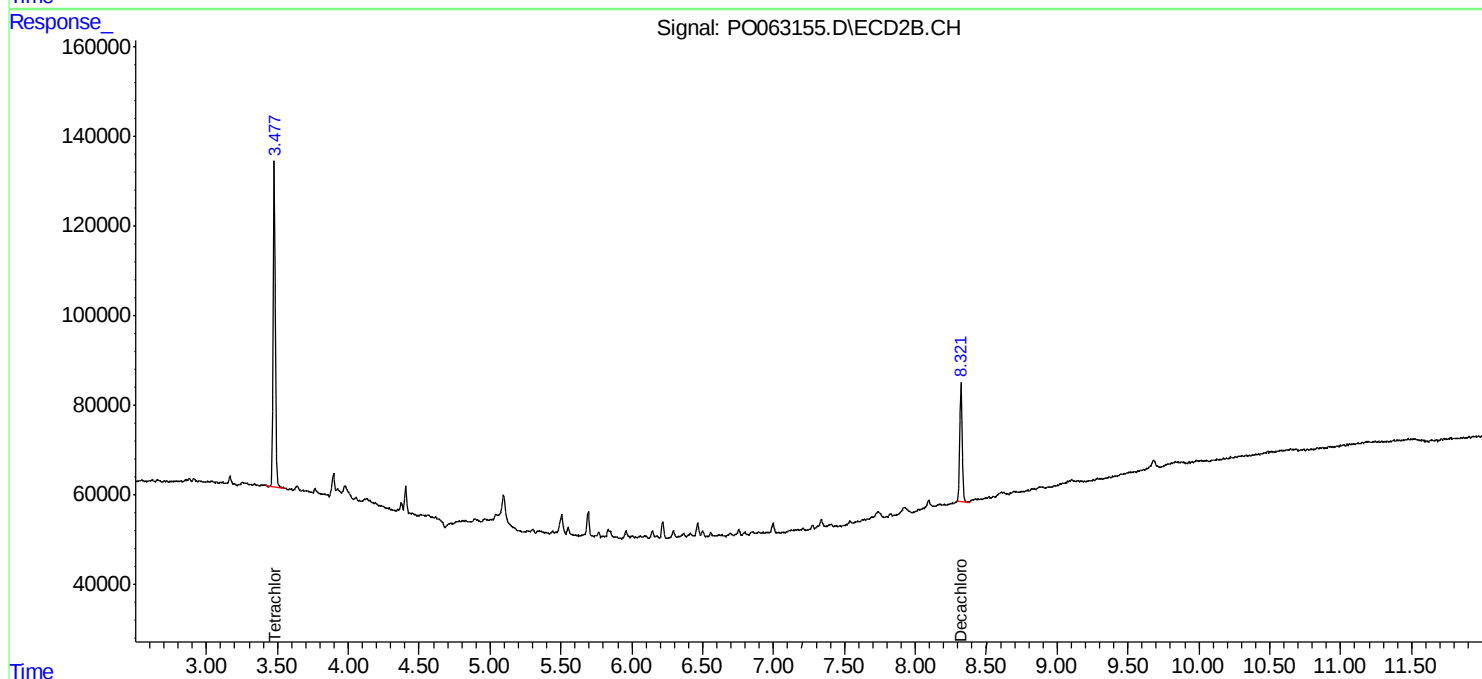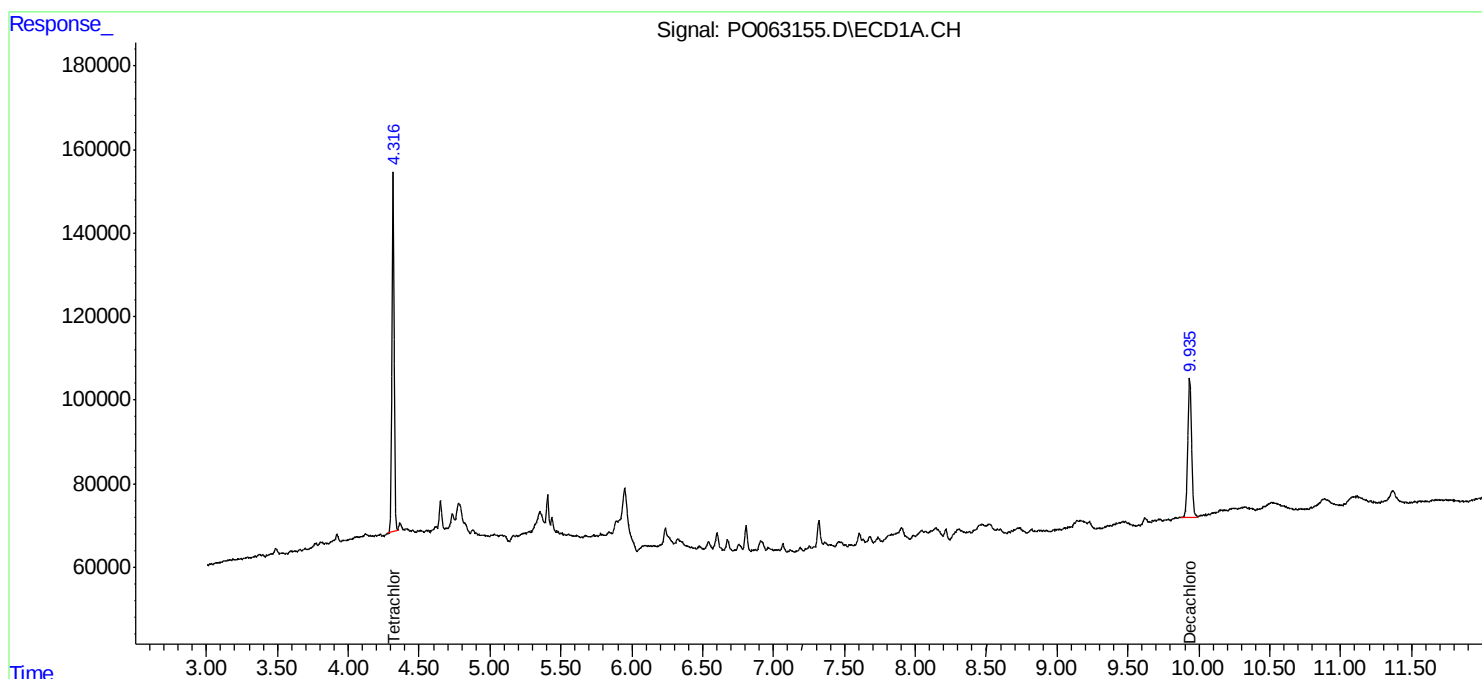

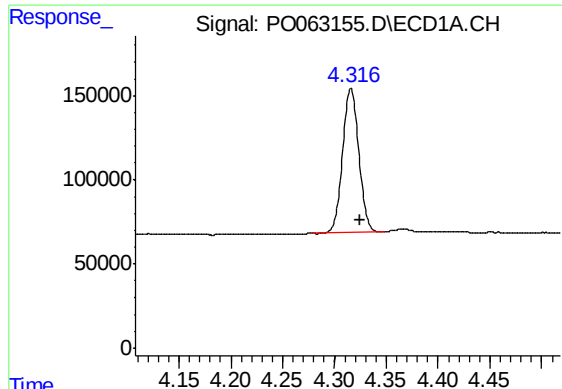


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.009 min
Response: 938235
Conc: 15.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
179-18-(0-2.1)


Manual Integrations
APPROVED

Ankita
10/28/2019 10:48:56 AM

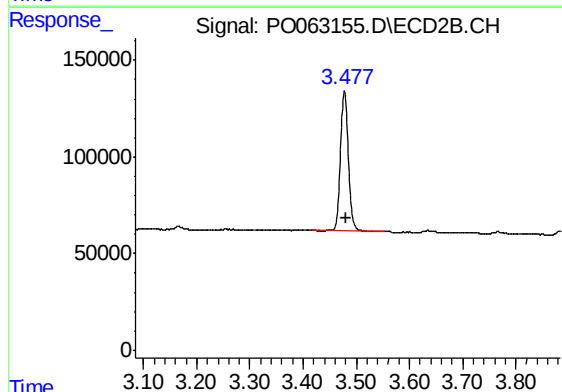


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: -0.004 min
Response: 748913
Conc: 17.46 ng/ml

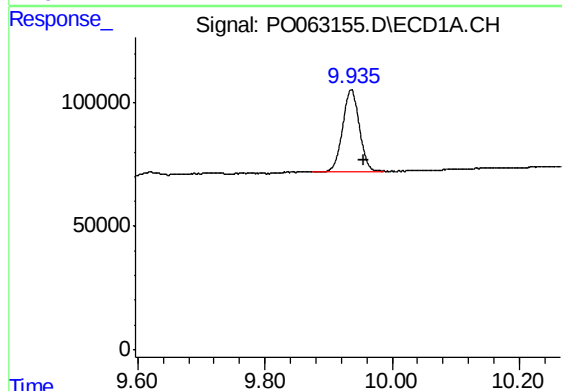

#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.021 min
Response: 614580
Conc: 10.98 ng/ml m

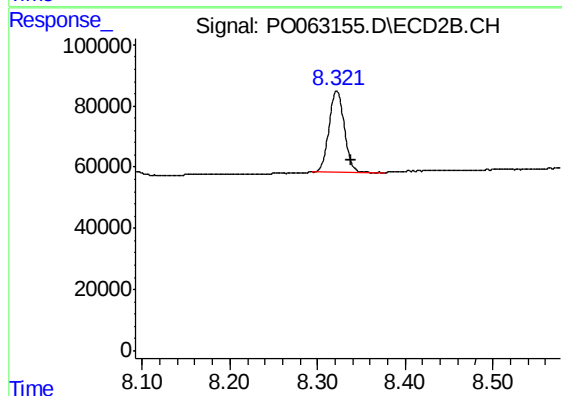

#2 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.016 min
Response: 321707
Conc: 10.96 ng/ml