

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102519\
 Data File : P0063165.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2019 14:52
 Operator : HP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 10/28/2019 10:49:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:15:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.478	1342758	1070393	21.711	24.962
2)	SA Decachlor...	9.936	8.323	1163035	613292	20.786m	20.902

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102519\
Data File : PO063165.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2019 14:52
Operator : HP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
10/28/2019 10:49:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:15:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

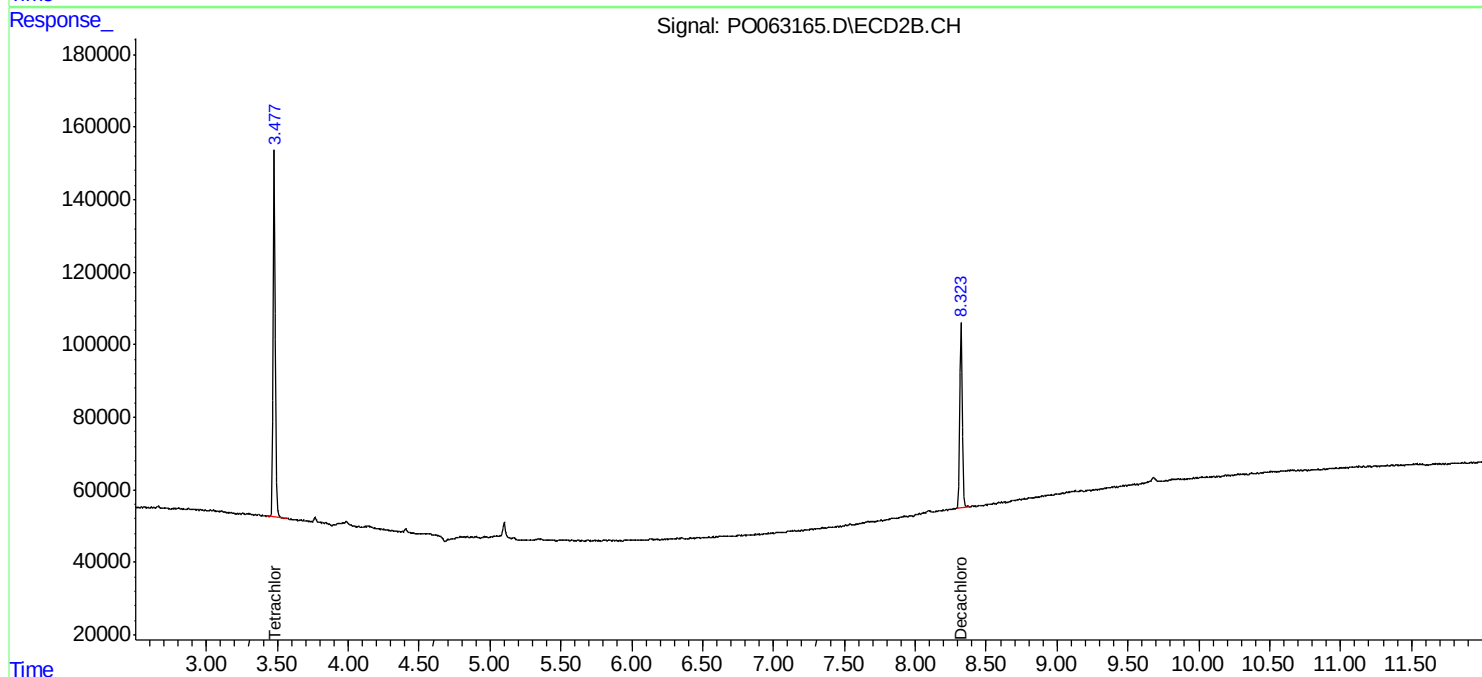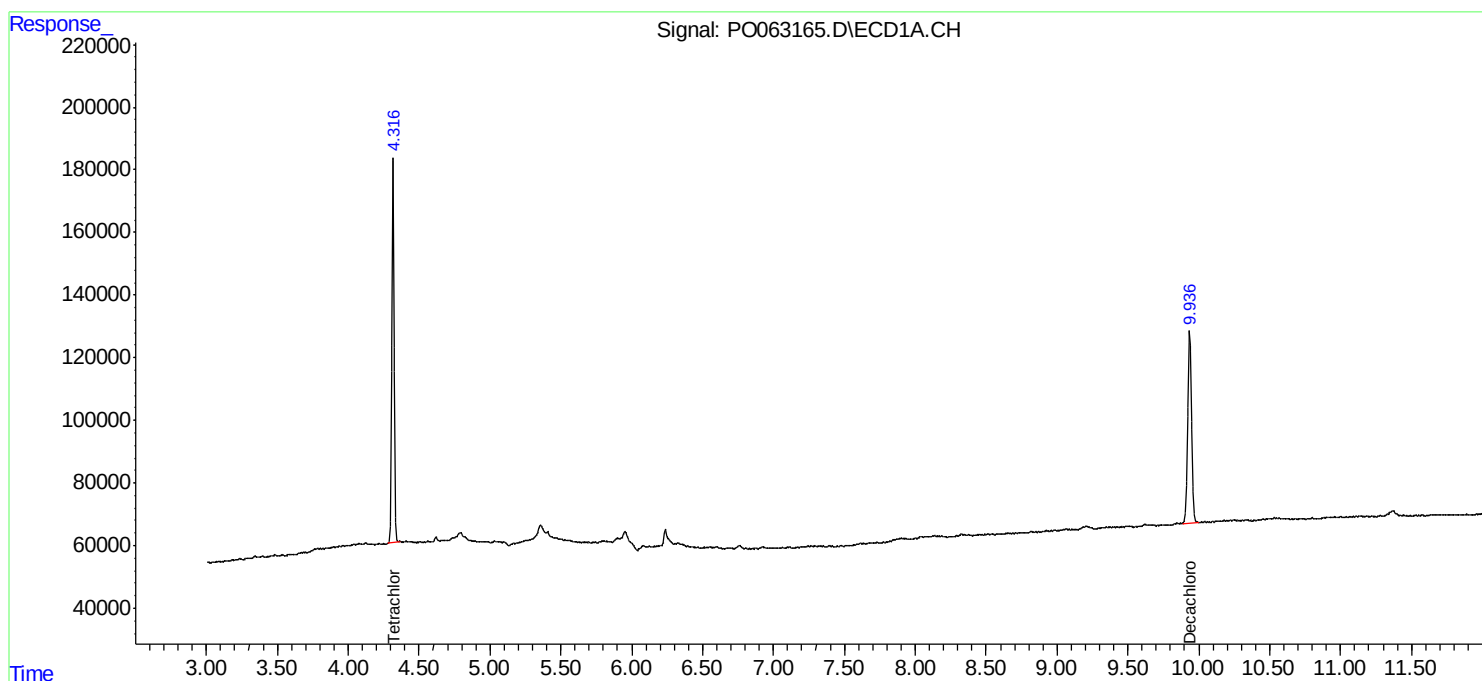

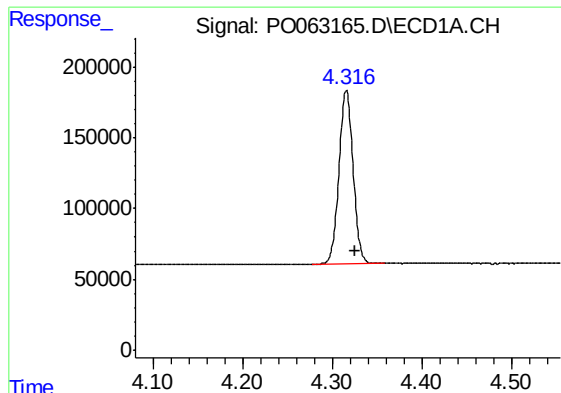


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.009 min
Response: 1342758
Conc: 21.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
10/28/2019 10:49:23 AM

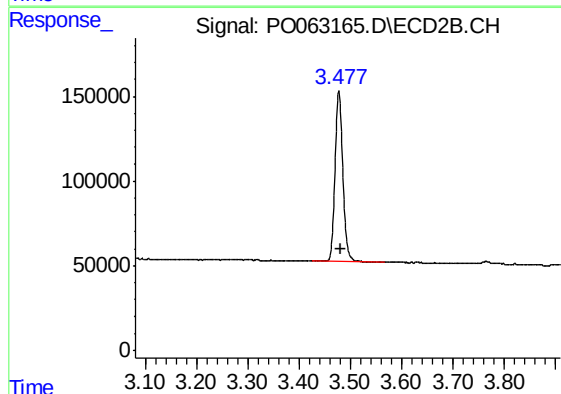


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: -0.004 min
Response: 1070393
Conc: 24.96 ng/ml

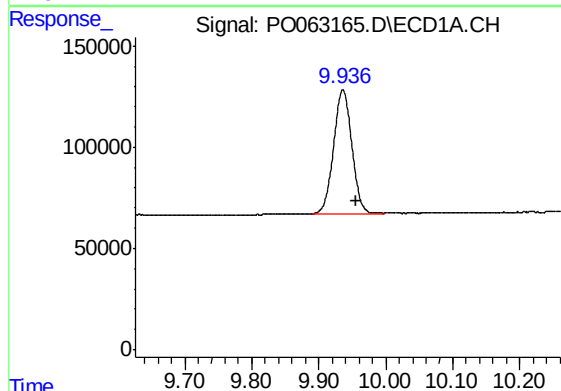

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: -0.021 min
Response: 1163035
Conc: 20.79 ng/ml m

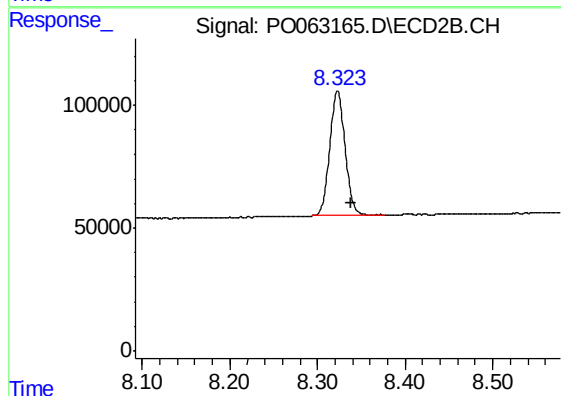

#2 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.015 min
Response: 613292
Conc: 20.90 ng/ml