

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102519\
 Data File : P0063177.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2019 18:26
 Operator : HP/AJ
 Sample : K5512-01RE
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT-26706RE

Manual Integrations
 APPROVED

Ankita
 10/28/2019 10:49:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:19:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.316	3.478	1105582	955979	17.876	22.293
2) SA Decachlor...	9.937	8.324	958457	502992	17.130m	17.143

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102519\
Data File : PO063177.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2019 18:26
Operator : HP/AJ
Sample : K5512-01RE
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHRT-26706RE


Manual Integrations
APPROVED

Ankita
10/28/2019 10:49:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:19:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

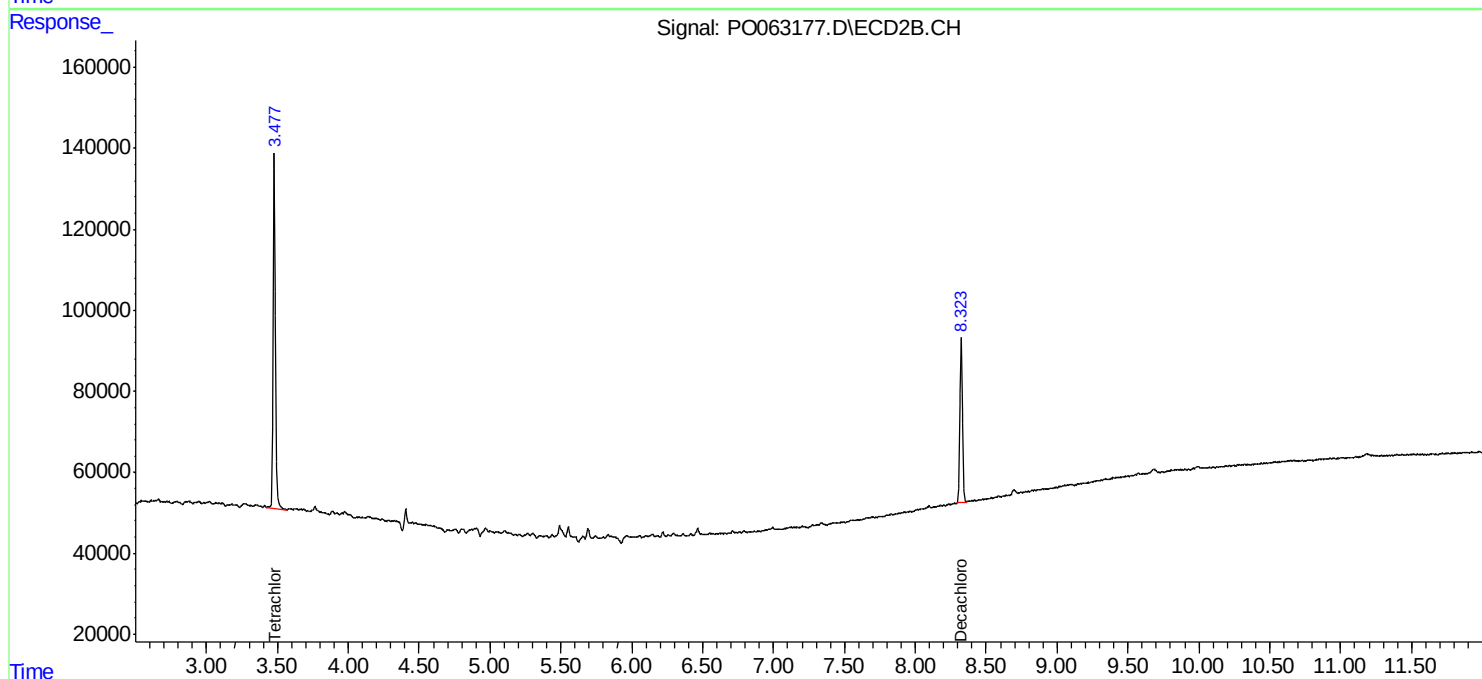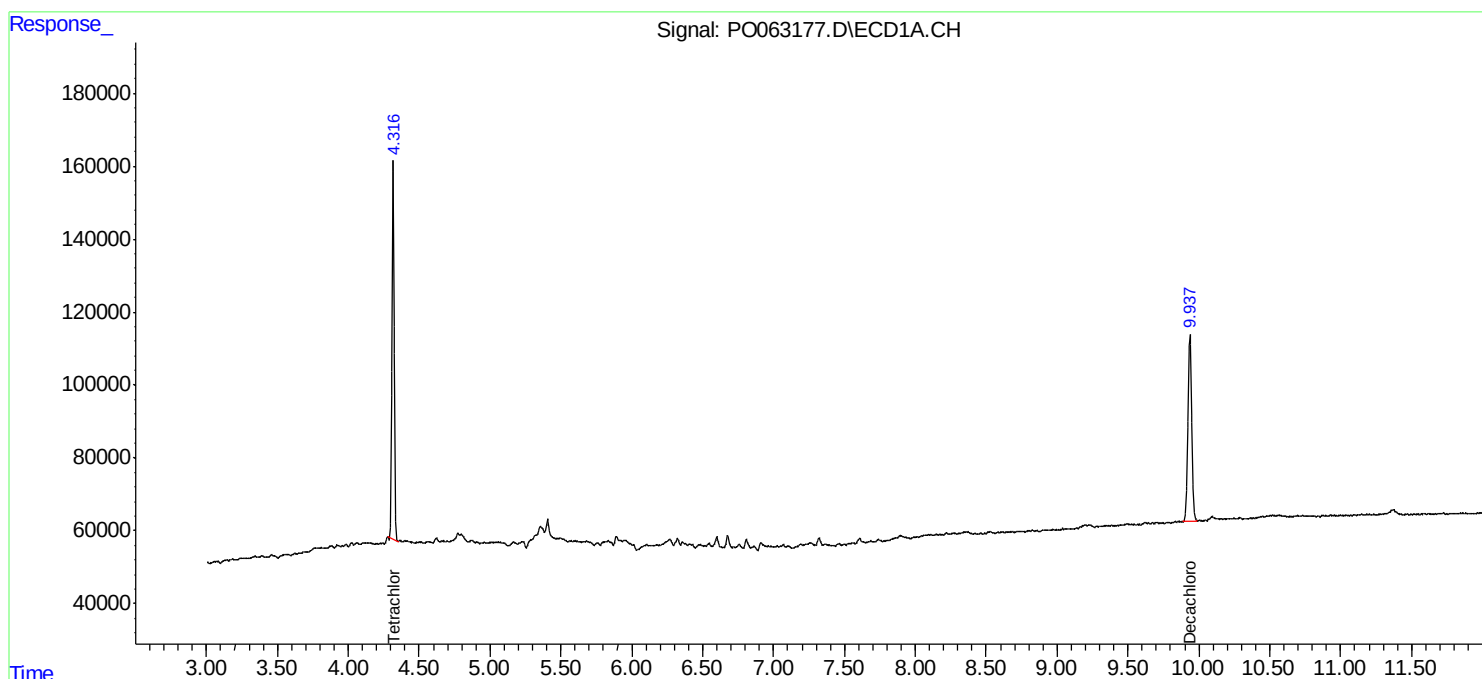

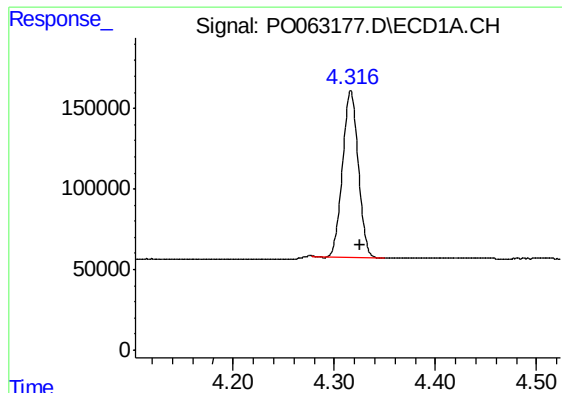


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.009 min
Response: 1105582
Conc: 17.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26706RE


Manual Integrations
APPROVED

Ankita
10/28/2019 10:49:55 AM

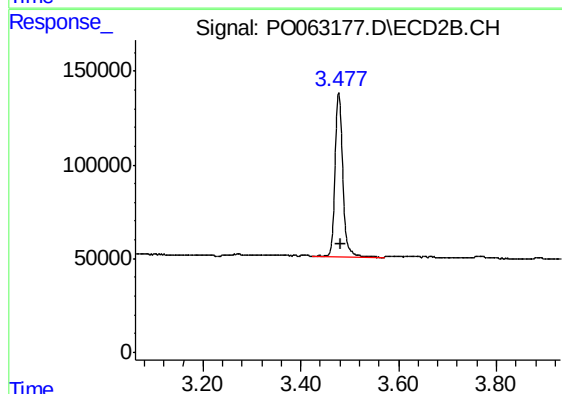


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: -0.004 min
Response: 955979
Conc: 22.29 ng/ml

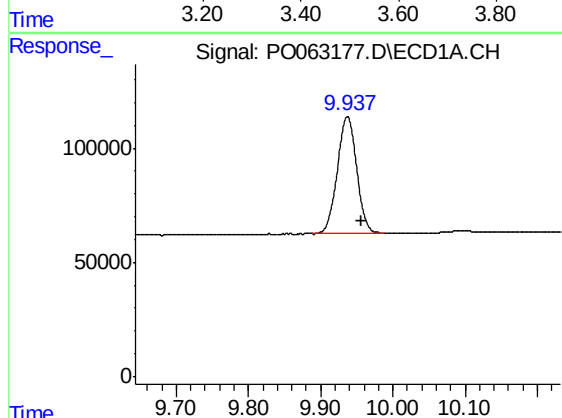

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.020 min
Response: 958457
Conc: 17.13 ng/ml m

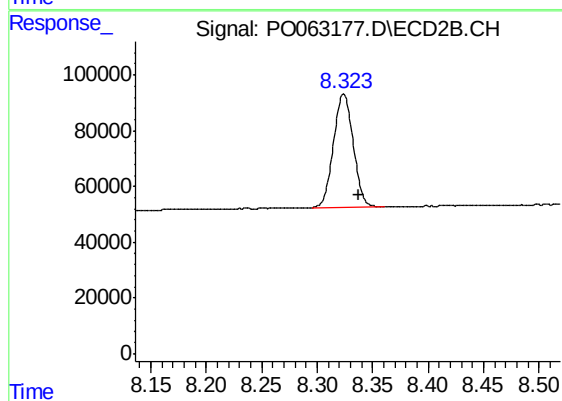

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.014 min
Response: 502992
Conc: 17.14 ng/ml