

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102519\
 Data File : P0063179.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2019 18:59
 Operator : HP/AJ
 Sample : K5500-07RE
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 804-00-(0-1.8)RE

Manual Integrations
 APPROVED

Ankita
 10/28/2019 10:52:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:20:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.478	1391077	1105876	22.492	25.789
2)	SA Decachlor...	9.937	8.324	1262843	597208	22.570m	20.354

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102519\
Data File : PO063179.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2019 18:59
Operator : HP/AJ
Sample : K5500-07RE
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
804-00-(0-1.8)RE


Manual Integrations
APPROVED

Ankita
10/28/2019 10:52:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:20:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

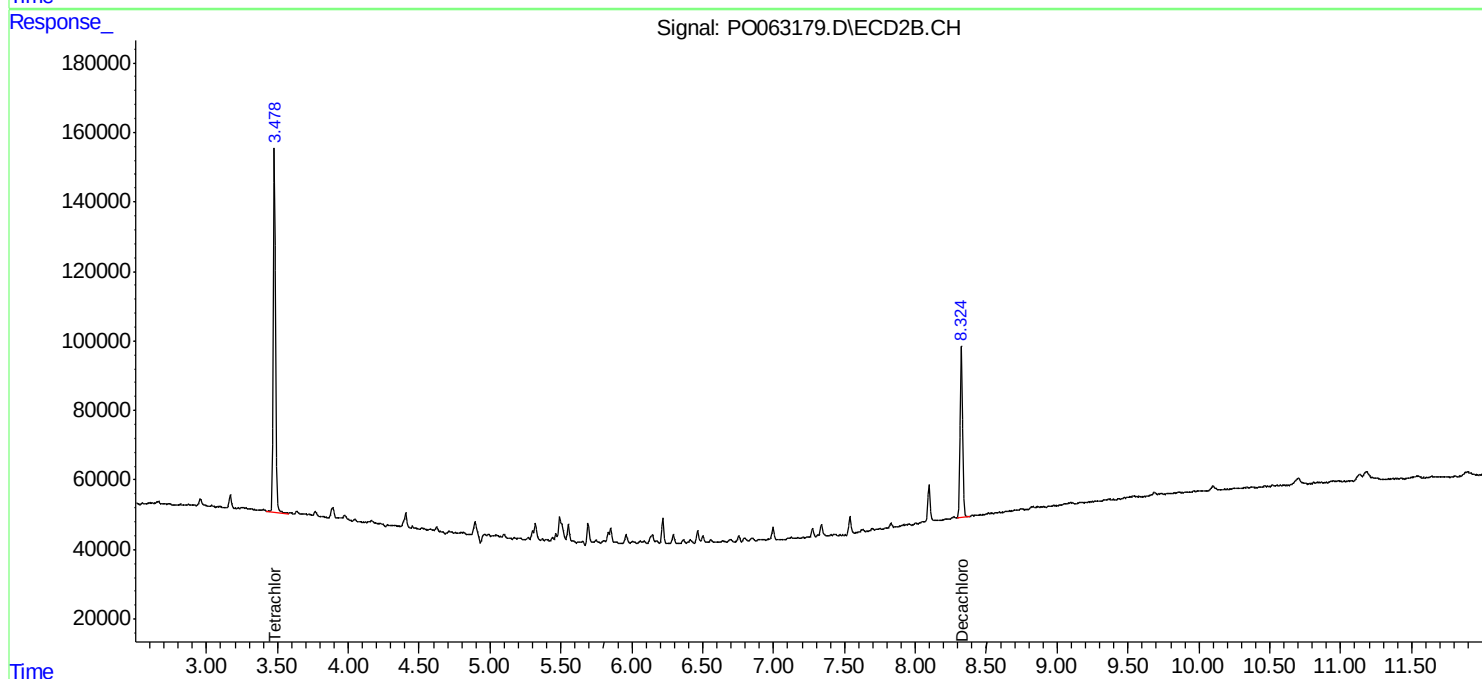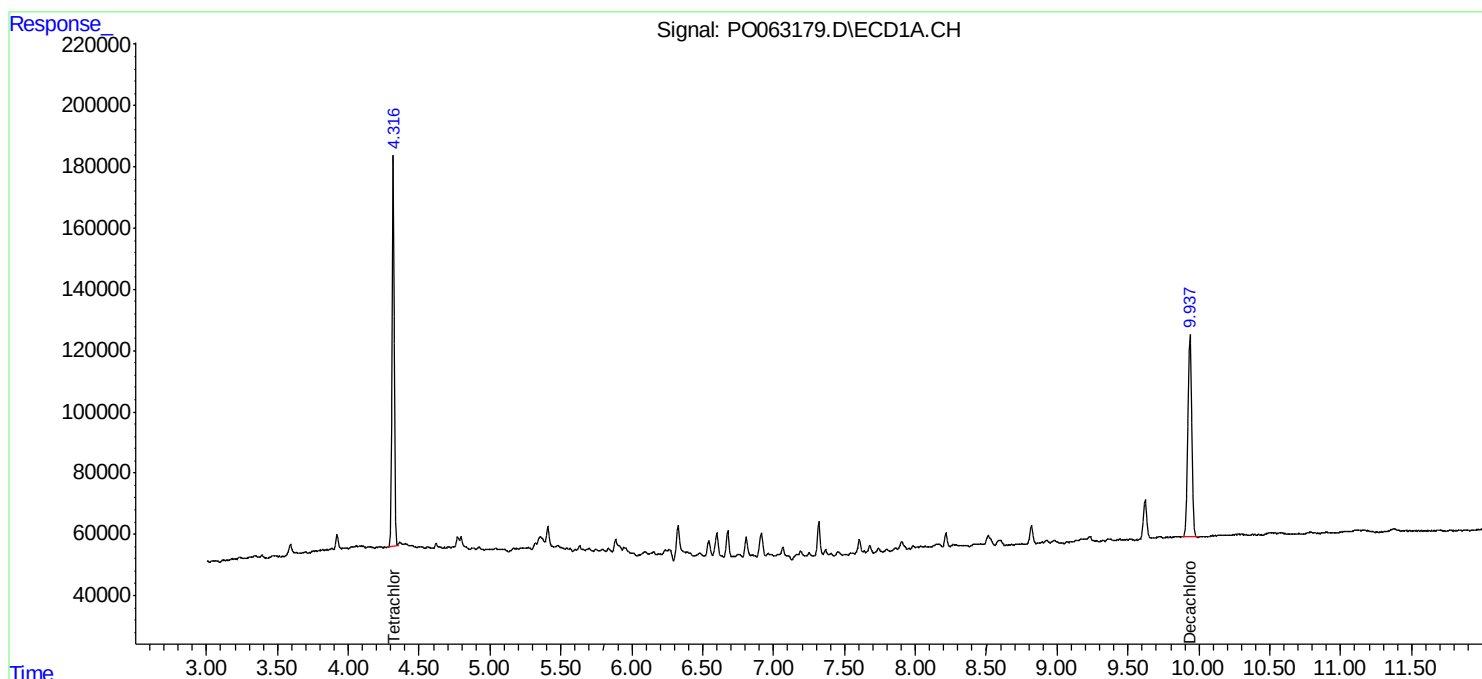

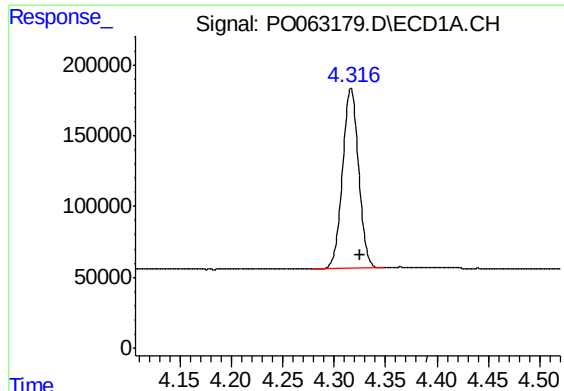


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.009 min
Response: 1391077
Conc: 22.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
804-00-(0-1.8)RE


Manual Integrations
APPROVED

Ankita
10/28/2019 10:52:05 AM

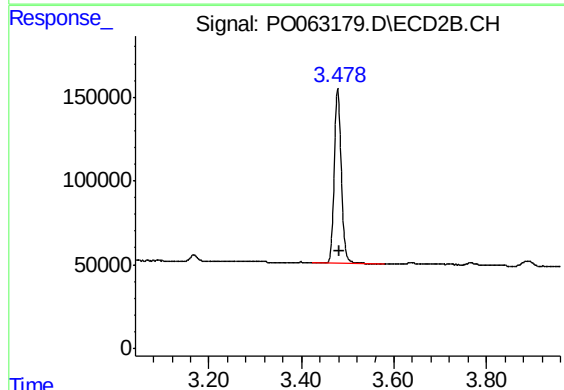


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: -0.003 min
Response: 1105876
Conc: 25.79 ng/ml

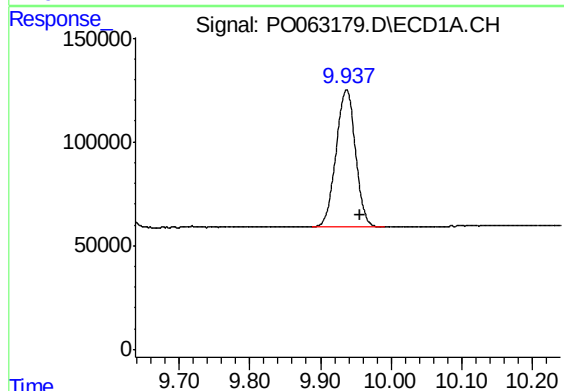

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.020 min
Response: 1262843
Conc: 22.57 ng/ml m

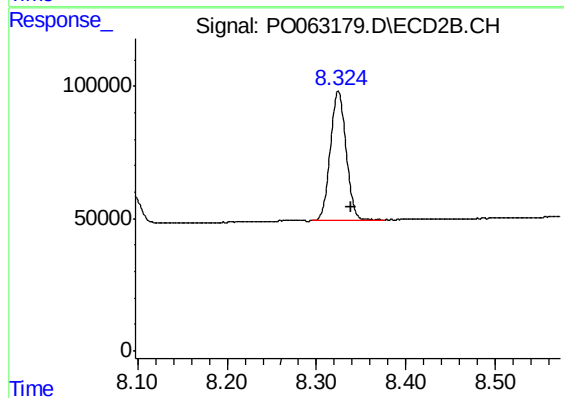

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.014 min
Response: 597208
Conc: 20.35 ng/ml