

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102519\
 Data File : P0063183.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2019 20:05
 Operator : HP/AJ
 Sample : K5500-01RE
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 802-50-(0-1.1)RE

Manual Integrations
 APPROVED

Ankita
 10/28/2019 10:52:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:21:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.318	3.480	1285379	1101284	20.783	25.682
2)	SA Decachlor...	9.939	8.326	826134	423251	14.765m	14.425

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102519\
Data File : PO063183.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2019 20:05
Operator : HP/AJ
Sample : K5500-01RE
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
802-50-(0-1.1)RE


Manual Integrations
APPROVED

Ankita
10/28/2019 10:52:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:21:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

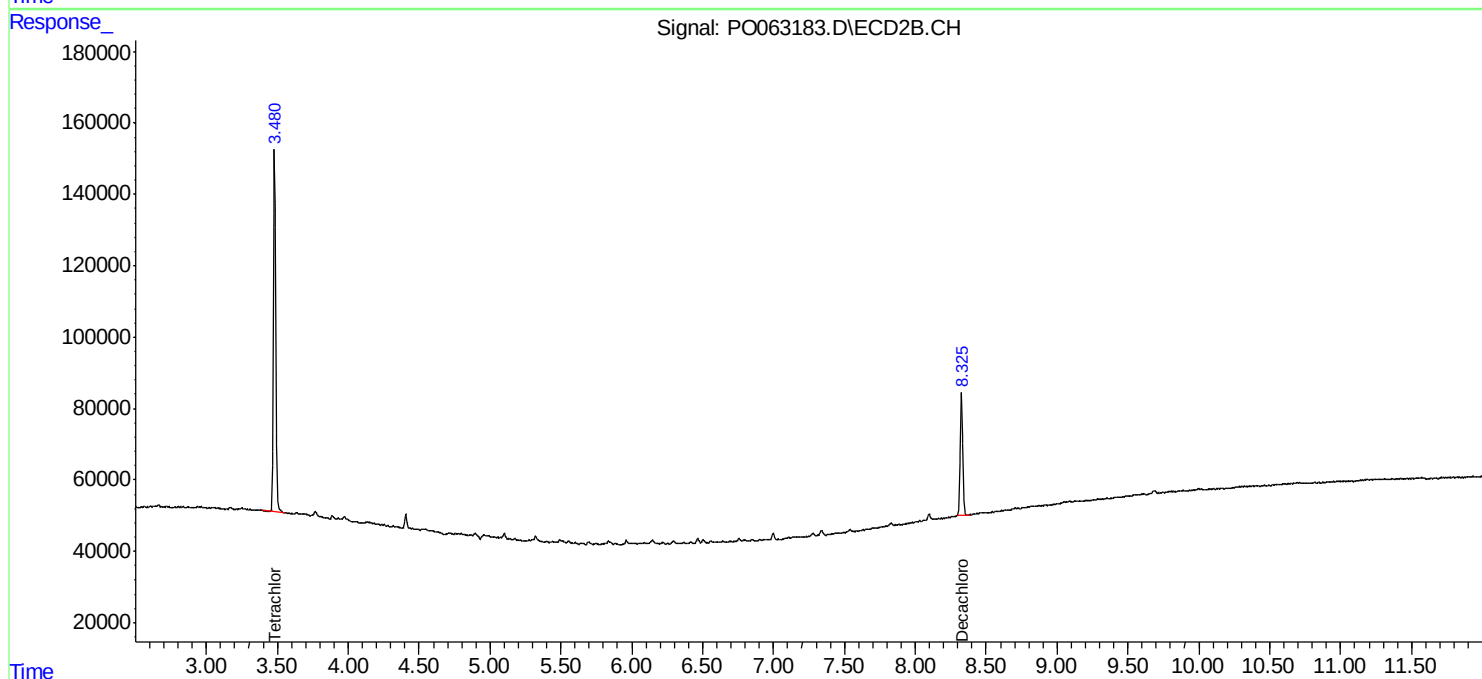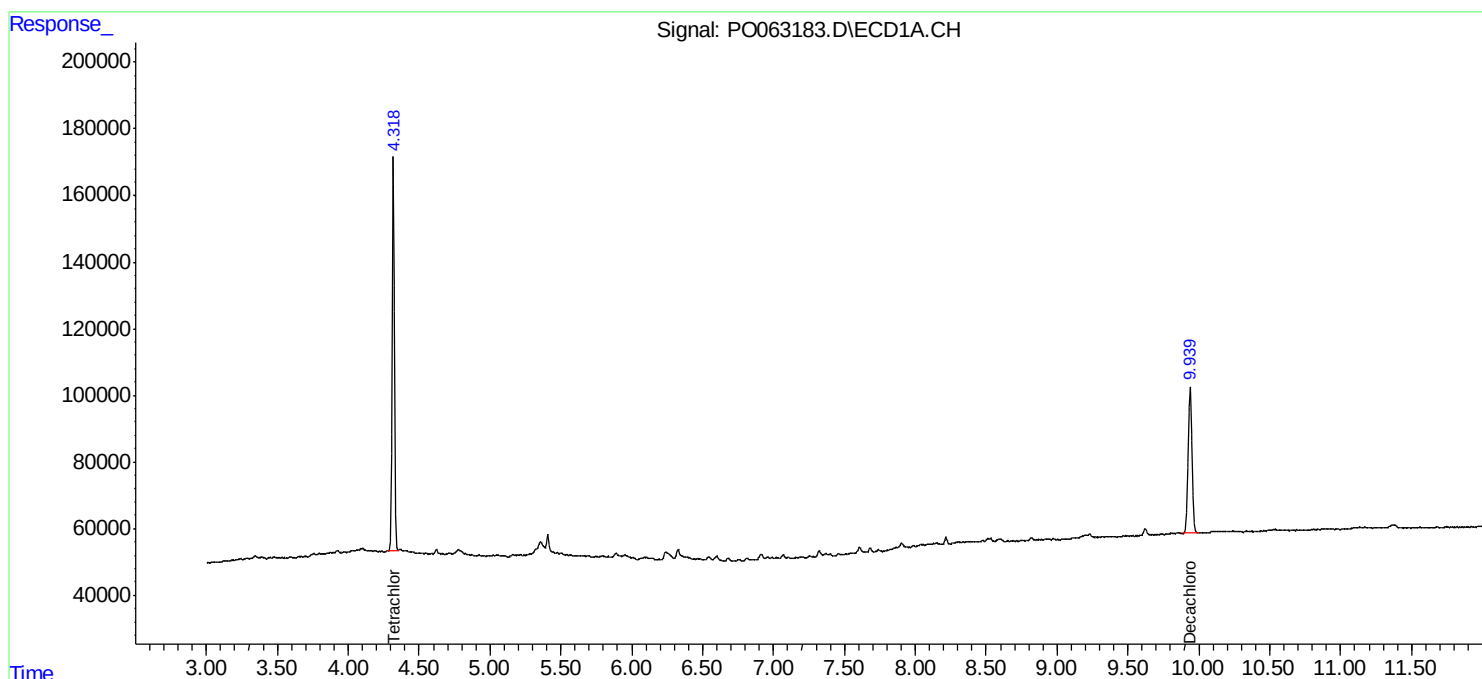

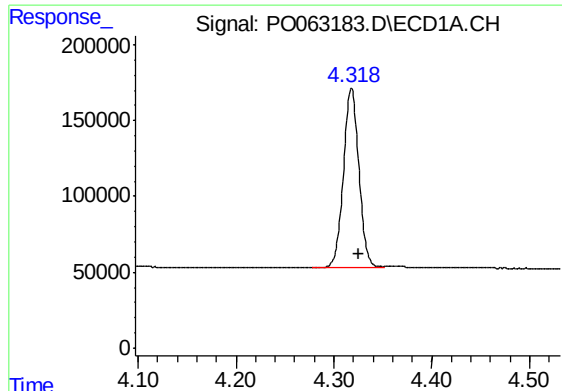


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: -0.007 min
Response: 1285379
Conc: 20.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
802-50-(0-1.1)RE


Manual Integrations
APPROVED

Ankita
10/28/2019 10:52:12 AM

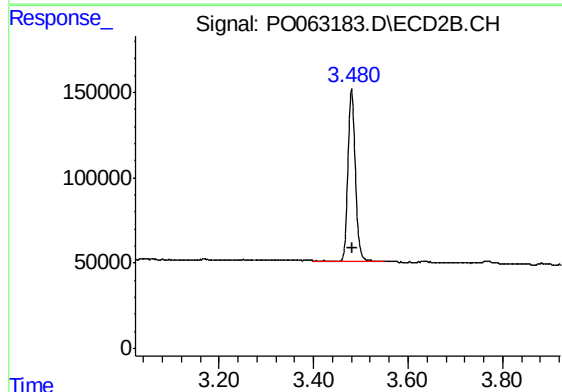


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: -0.001 min
Response: 1101284
Conc: 25.68 ng/ml

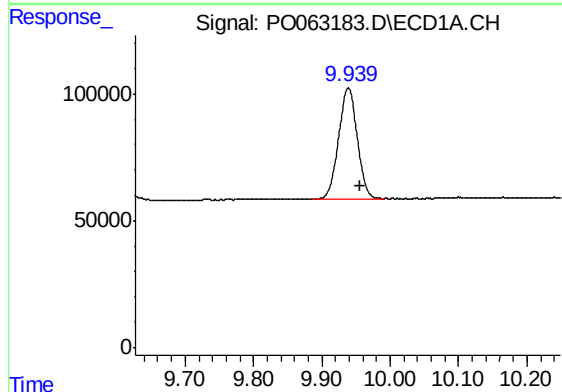

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: -0.017 min
Response: 826134
Conc: 14.76 ng/ml m

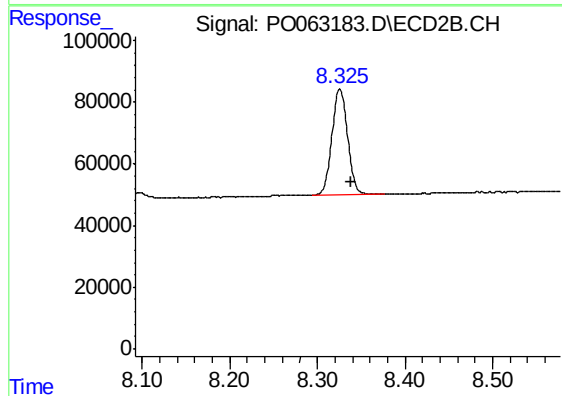

#2 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.012 min
Response: 423251
Conc: 14.43 ng/ml