

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063216.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2019 10:12
 Operator : HP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 02:27:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.479	1068614	1036414	18.335	18.977
2) SA Decachlor...	9.936	8.322	1084436	761076	18.638	17.802
Target Compounds						
3) L1 AR-1016-1	0.000	4.544	0	11176	N.D.	5.965 #
4) L1 AR-1016-2	0.000	4.544	0	11176	N.D.	4.097 #
12) L3 AR-1232-2	0.000	4.544	0	11176	N.D.	5.682 #
16) L4 AR-1242-1	0.000	4.544	0	11176	N.D.	8.088 #
17) L4 AR-1242-2	0.000	4.544	0	11176	N.D.	5.447 #
20) L4 AR-1242-5	0.000	5.328	0	3631	N.D.	2.599 #
21) L5 AR-1248-1	0.000	4.544	0	11176	N.D.	10.225 #
25) L5 AR-1248-5	0.000	5.328	0	3631	N.D.	1.964 #
26) L6 AR-1254-1	0.000	5.328	0	3631	N.D.	1.205 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063216.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2019 10:12
Operator : HP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 02:27:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

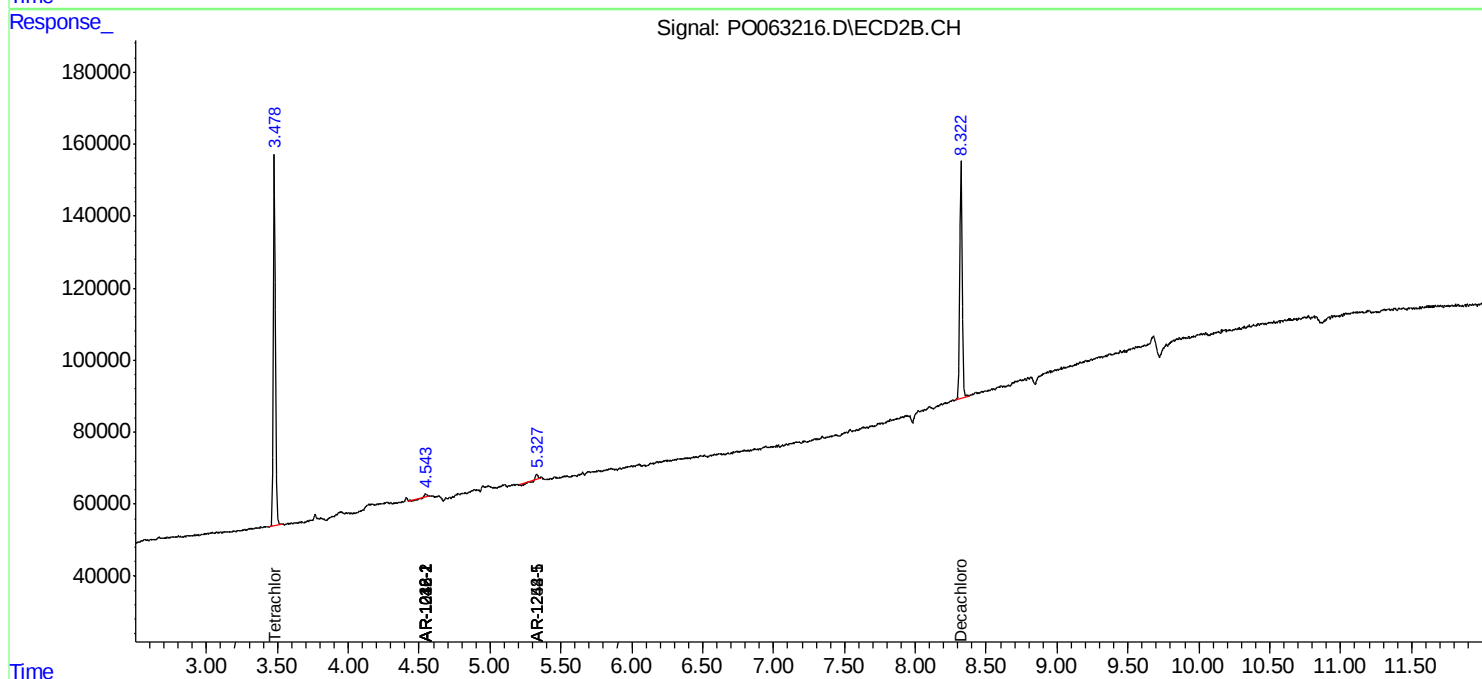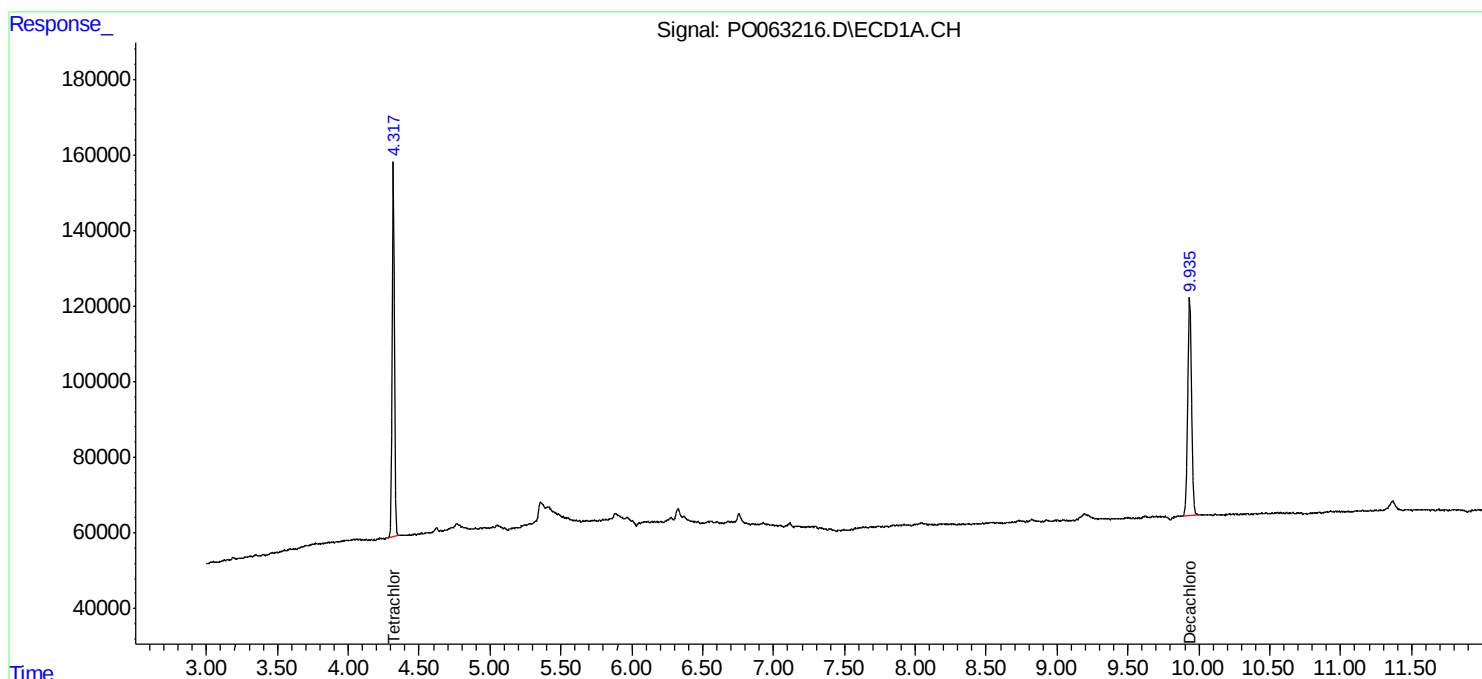


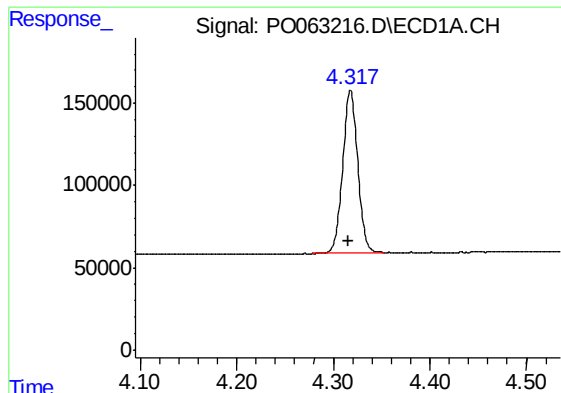

#1 Tetrachloro-m-xylene


R.T.: 4.318 min
Delta R.T.: 0.002 min
Response: 1068614
Conc: 18.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

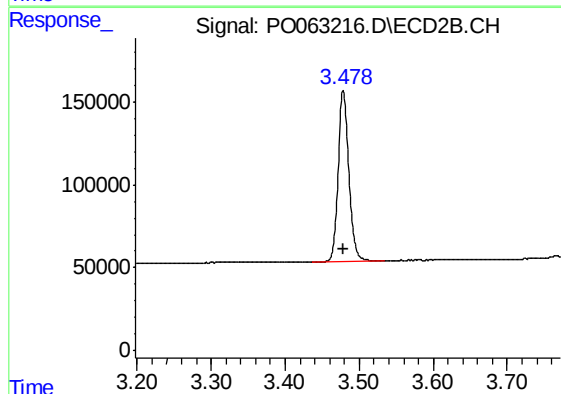


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 1036414
Conc: 18.98 ng/ml

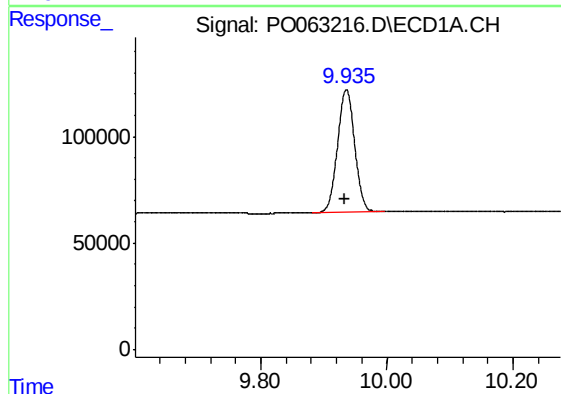


#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.002 min
Response: 1084436
Conc: 18.64 ng/ml

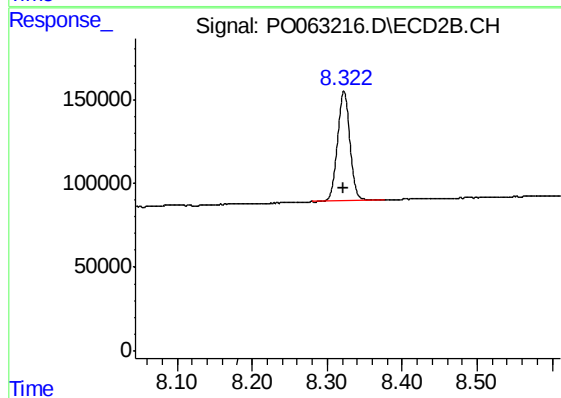

#2 Decachlorobiphenyl


R.T.: 8.322 min
Delta R.T.: 0.001 min
Response: 761076
Conc: 17.80 ng/ml

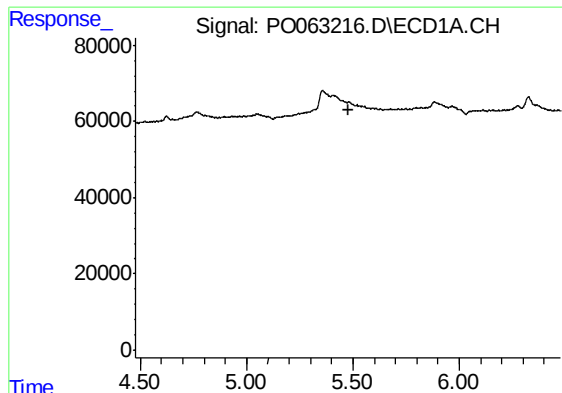

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

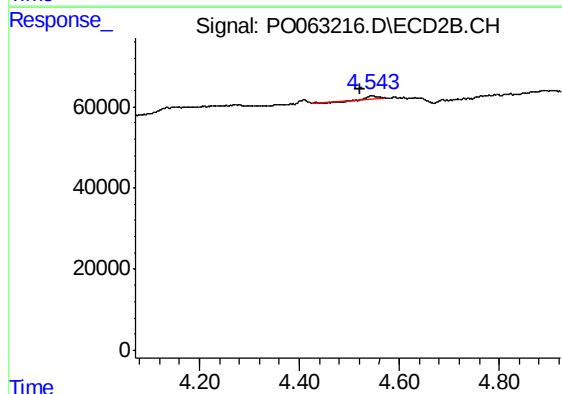


#3 AR-1016-1

R.T.: 4.544 min
Delta R.T.: 0.022 min
Response: 11176
Conc: 5.97 ng/ml

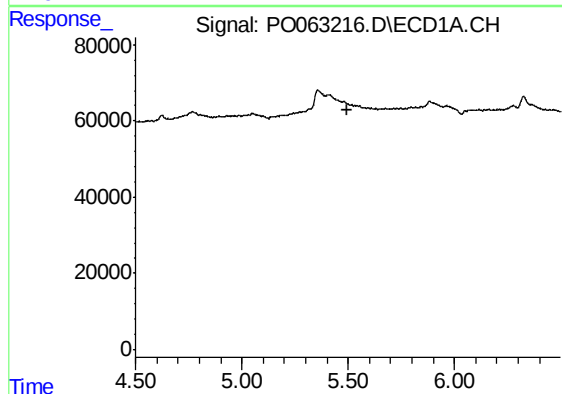


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

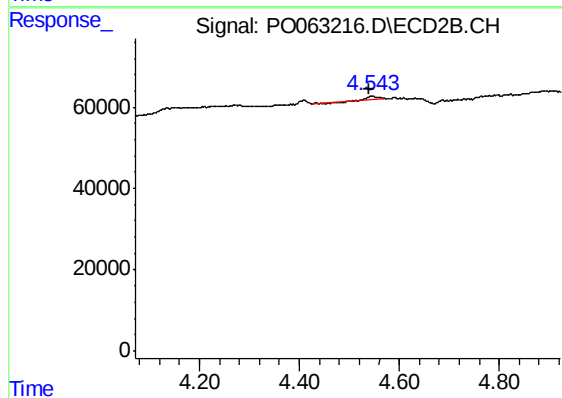

#4 AR-1016-2


R.T.: 4.544 min
Delta R.T.: 0.005 min
Response: 11176
Conc: 4.10 ng/ml

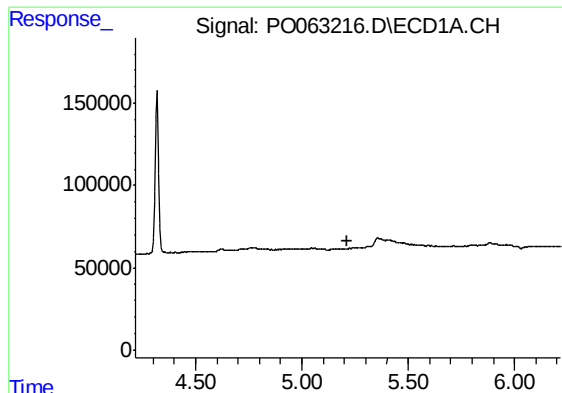

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 5.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

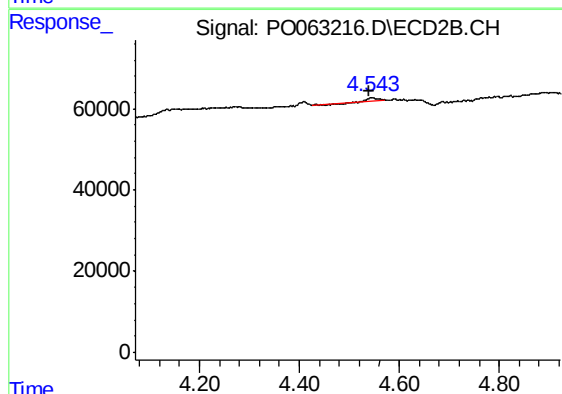


#12 AR-1232-2

R.T.: 4.544 min
Delta R.T.: 0.004 min
Response: 11176
Conc: 5.68 ng/ml

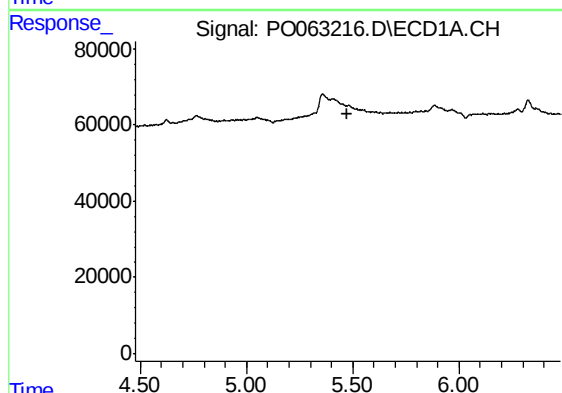


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

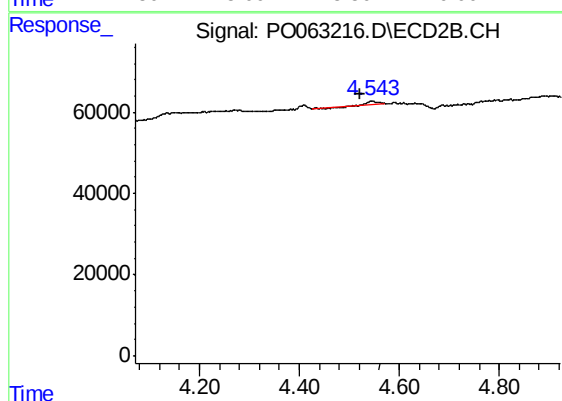

#16 AR-1242-1


R.T.: 4.544 min
Delta R.T.: 0.022 min
Response: 11176
Conc: 8.09 ng/ml

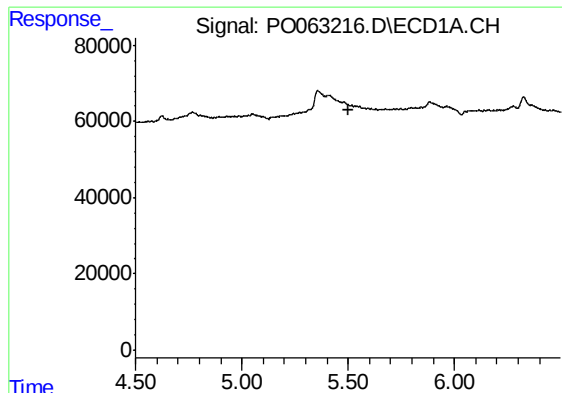

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

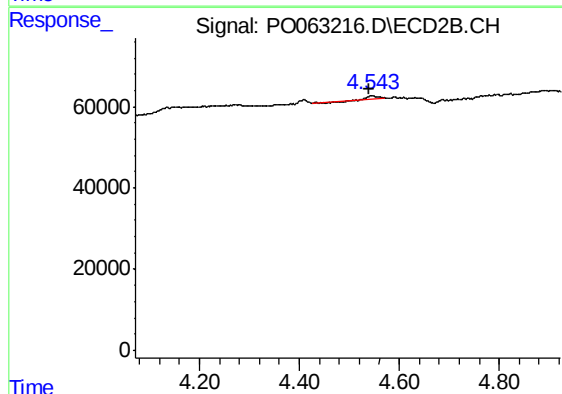


#17 AR-1242-2

R.T.: 4.544 min
Delta R.T.: 0.005 min
Response: 11176
Conc: 5.45 ng/ml

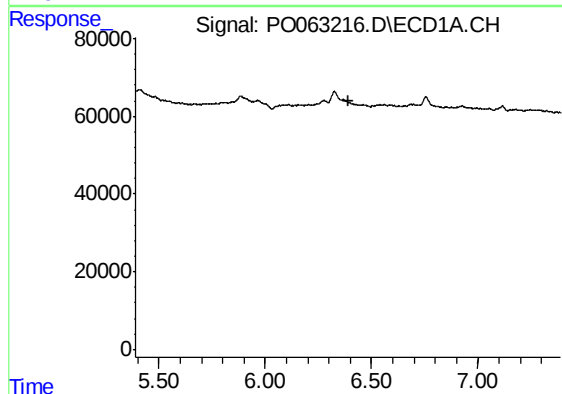


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

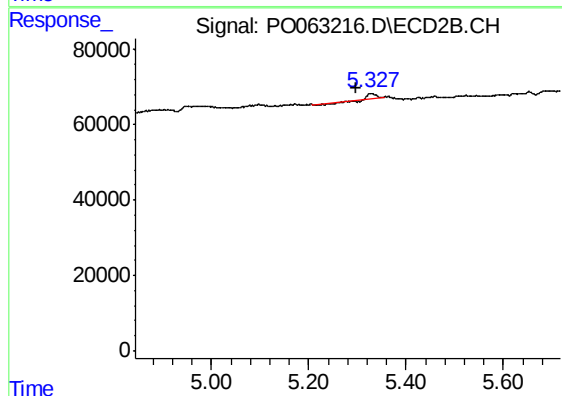

#20 AR-1242-5


R.T.: 5.328 min
Delta R.T.: 0.032 min
Response: 3631
Conc: 2.60 ng/ml

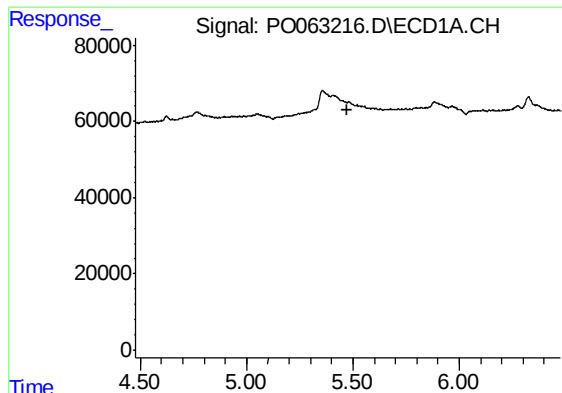

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

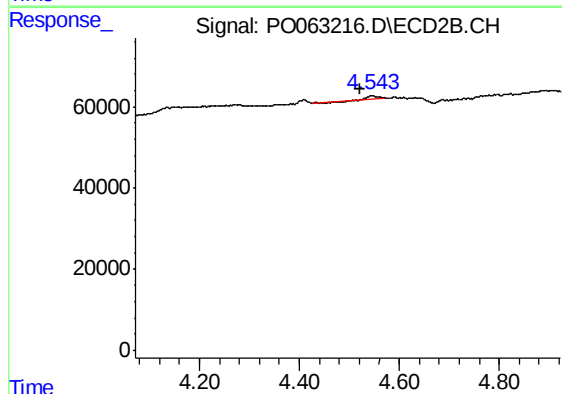


#21 AR-1248-1

R.T.: 4.544 min
Delta R.T.: 0.022 min
Response: 11176
Conc: 10.23 ng/ml

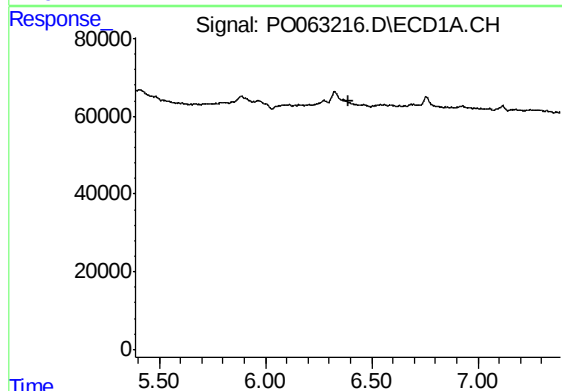


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.388 min
Response: 0
Conc: N.D.

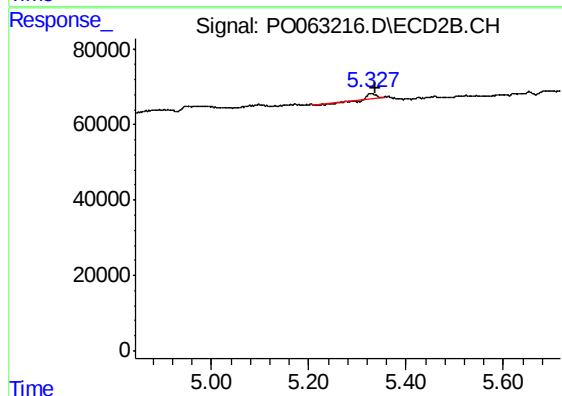

#25 AR-1248-5


R.T.: 5.328 min
Delta R.T.: -0.008 min
Response: 3631
Conc: 1.96 ng/ml

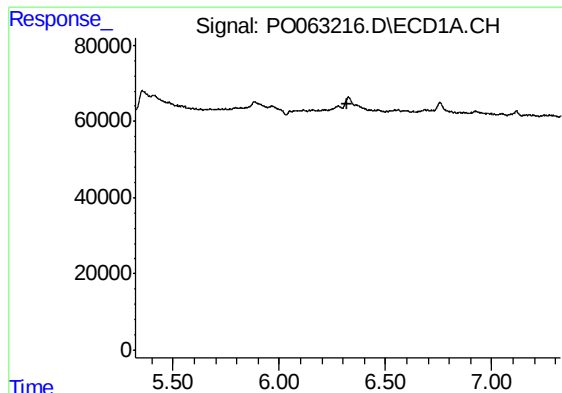

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

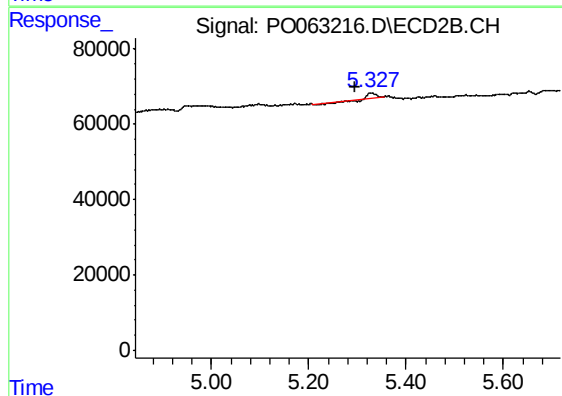

#26 AR-1254-1

R.T.: 5.328 min
Delta R.T.: 0.032 min
Response: 3631
Conc: 1.21 ng/ml