

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
 Data File : PO063243.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2019 18:50
 Operator : HP/AJ
 Sample : K5569-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-DECON-WATER-102519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:07:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.317	3.481	198583	191231	3.407	3.502
Target Compounds							
12)	L3 AR-1232-2	5.246	0.000	77404	0	78.193	N.D. #
20)	L4 AR-1242-5	0.000	5.263	0	29358	N.D.	21.015 #
26)	L6 AR-1254-1	0.000	5.263	0	29358	N.D.	9.746 #
29)	L6 AR-1254-4	0.000	6.098	0	69115	N.D.	24.254 #
32)	L7 AR-1260-2	0.000	6.174	0	40109	N.D.	10.454 #
33)	L7 AR-1260-3	0.000	6.228	0	17677	N.D.	5.634 #
34)	L7 AR-1260-4	0.000	6.753	0	105167	N.D.	41.537 #
36)	L8 AR-1262-1	0.000	6.580	0	228016	N.D.	125.313 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : P0063243.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2019 18:50
Operator : HP/AJ
Sample : K5569-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:07:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

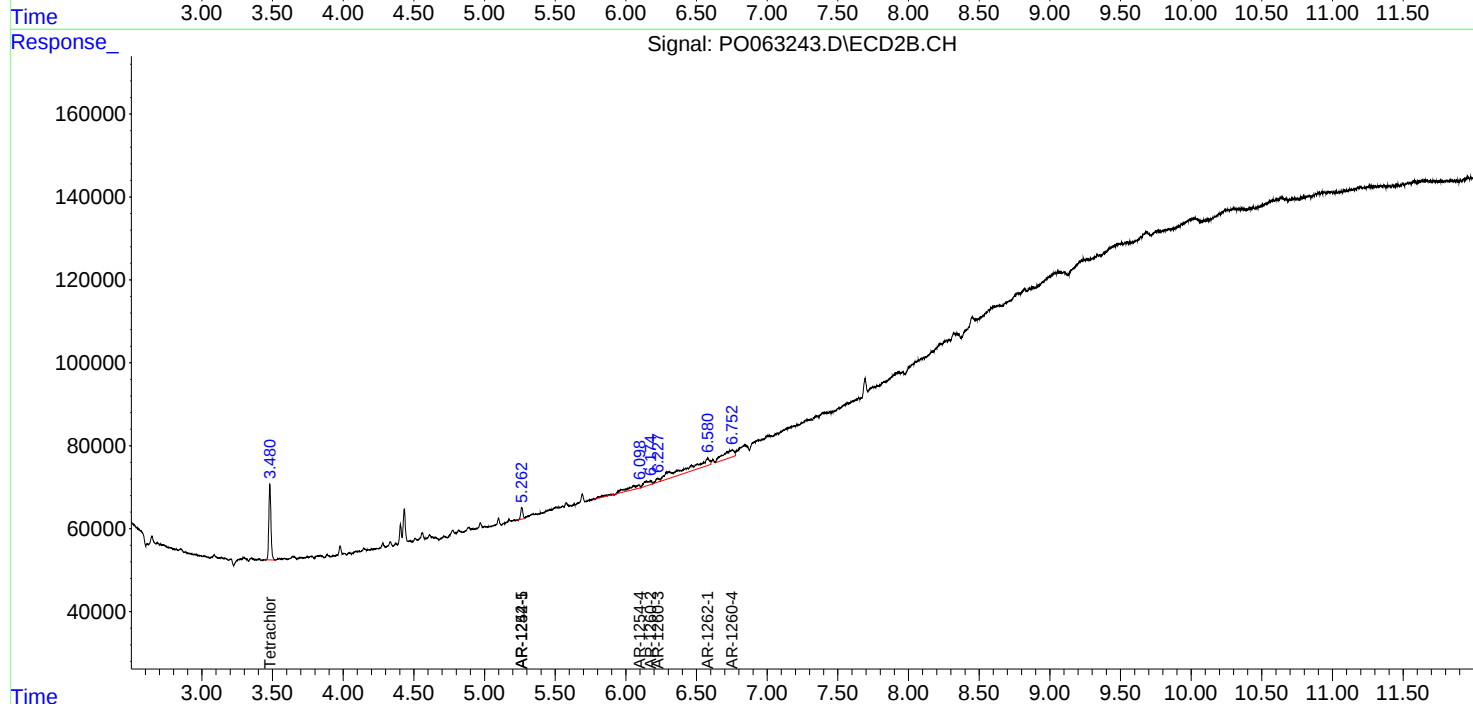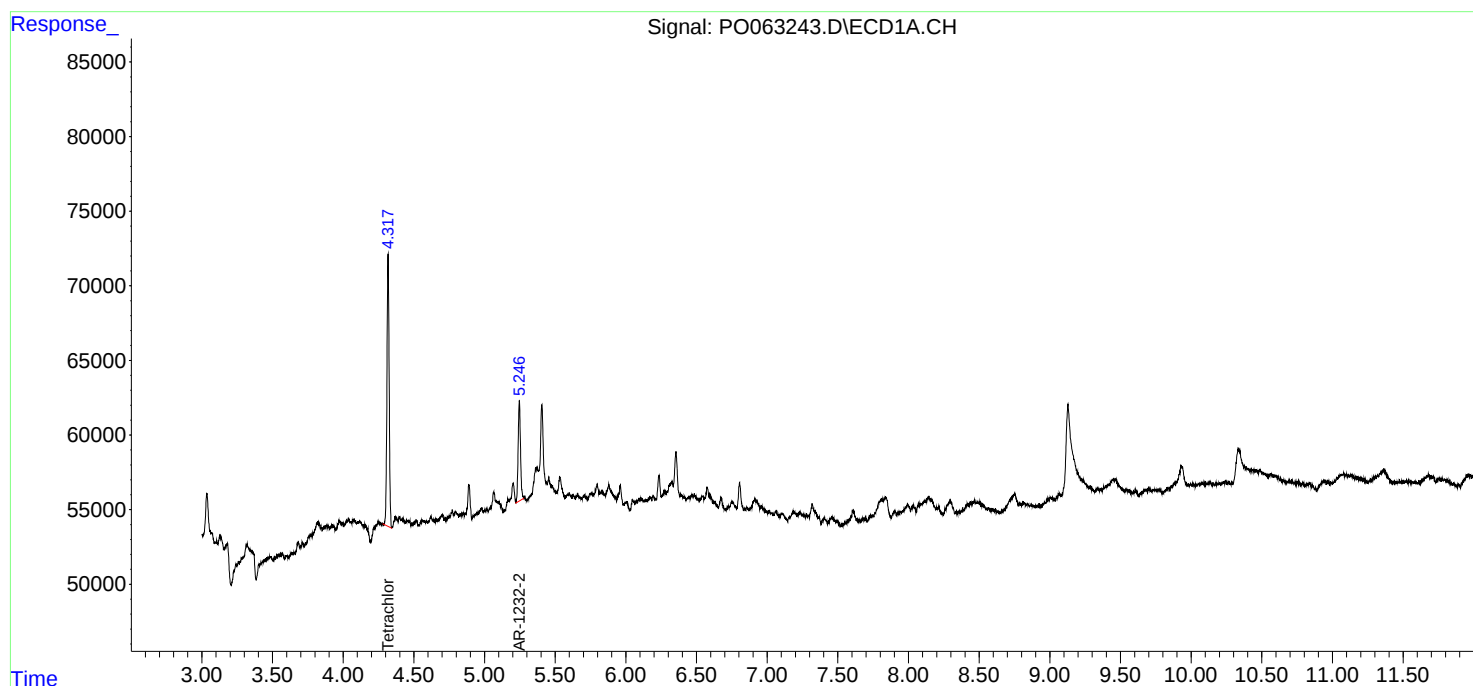


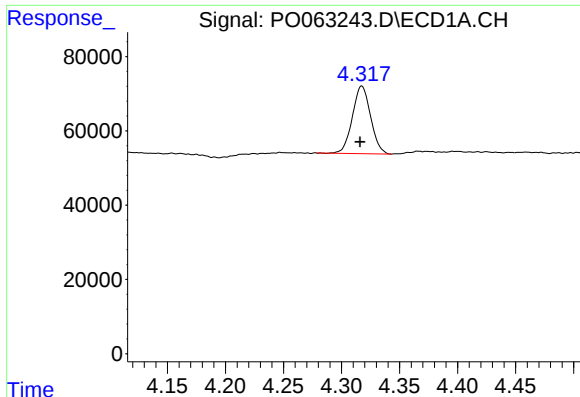

#1 Tetrachloro-m-xylene


R.T.: 4.317 min
Delta R.T.: 0.001 min
Response: 198583
Conc: 3.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

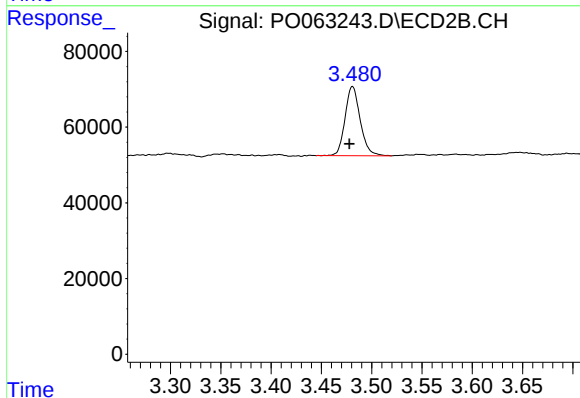


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.003 min
Response: 191231
Conc: 3.50 ng/ml

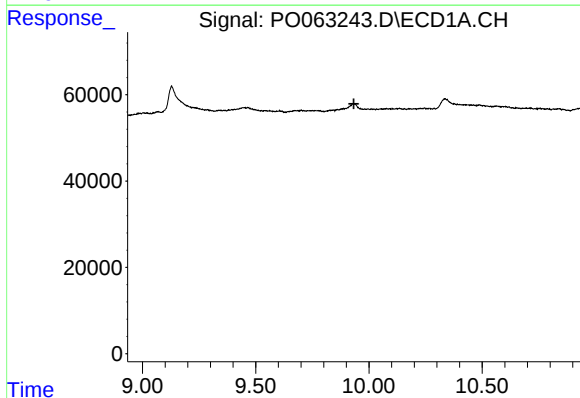


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.934 min
Response: 0
Conc: N.D.

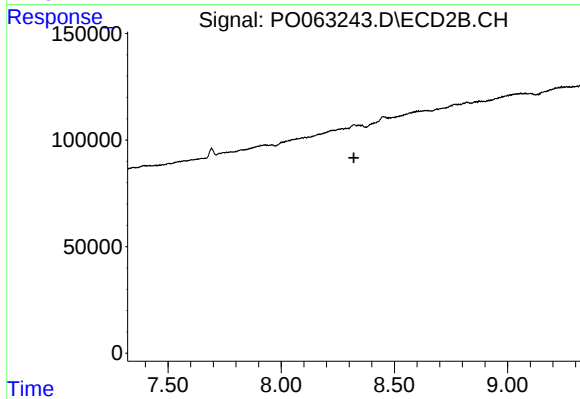

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.321 min
Response: 0
Conc: N.D.

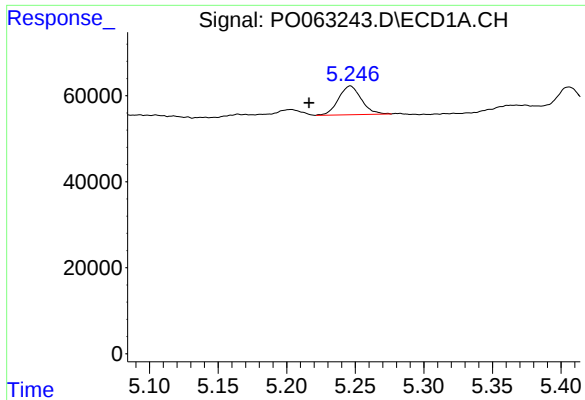

#12 AR-1232-2


R.T.: 5.246 min
Delta R.T.: 0.030 min
Response: 77404
Conc: 78.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

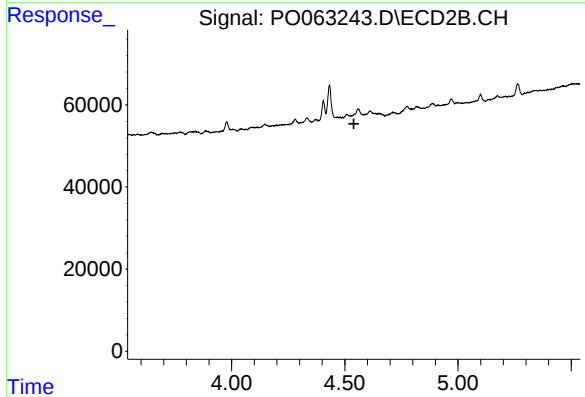


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.540 min
Response: 0
Conc: N.D.

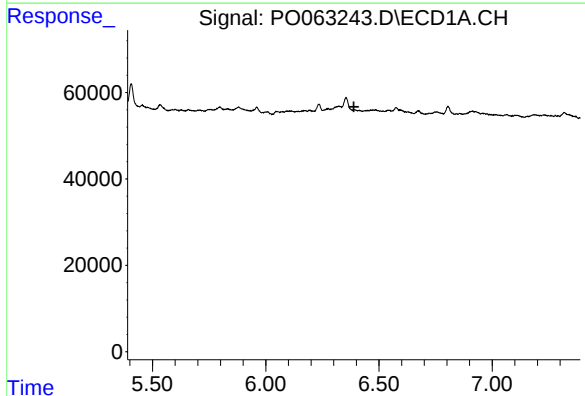


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

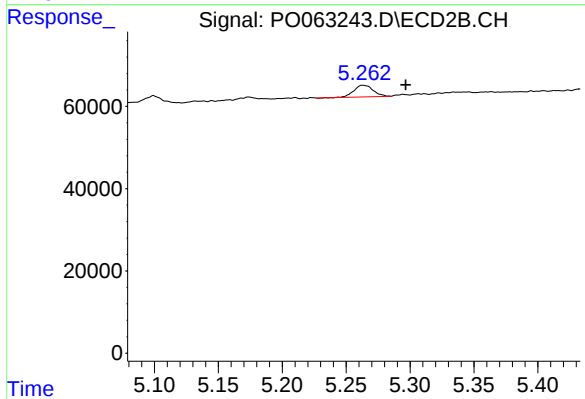

#20 AR-1242-5


R.T.: 5.263 min
Delta R.T.: -0.033 min
Response: 29358
Conc: 21.01 ng/ml

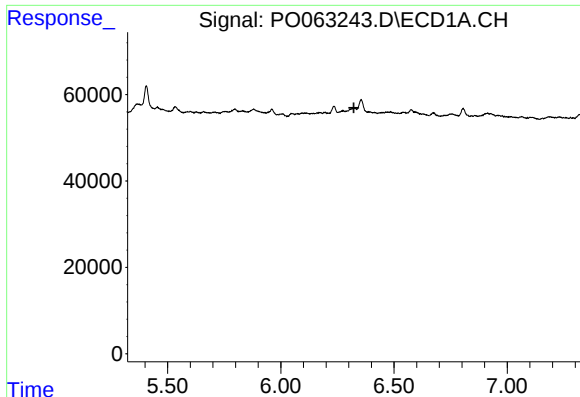

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

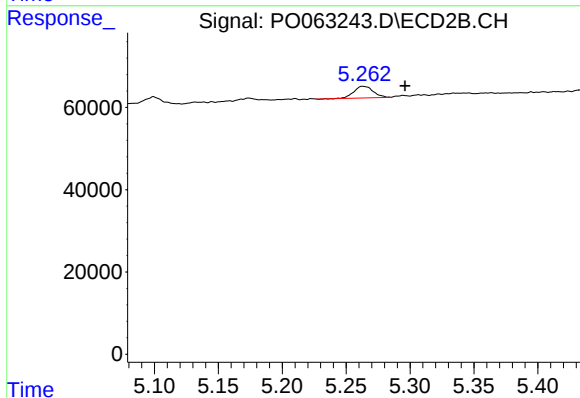


#26 AR-1254-1

R.T.: 5.263 min
Delta R.T.: -0.033 min
Response: 29358
Conc: 9.75 ng/ml

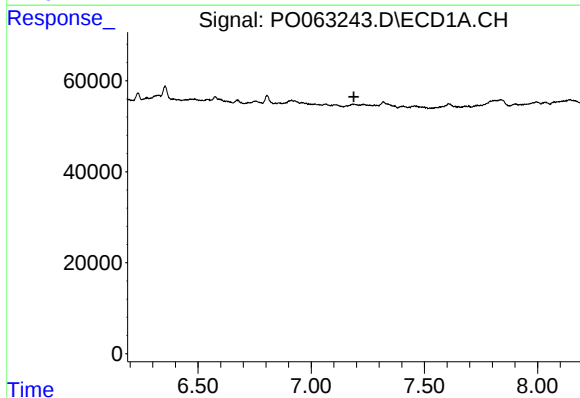


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.189 min
Response: 0
Conc: N.D.

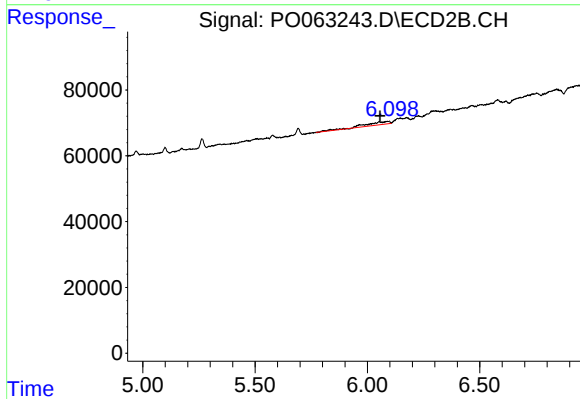

#29 AR-1254-4


R.T.: 6.098 min
Delta R.T.: 0.042 min
Response: 69115
Conc: 24.25 ng/ml

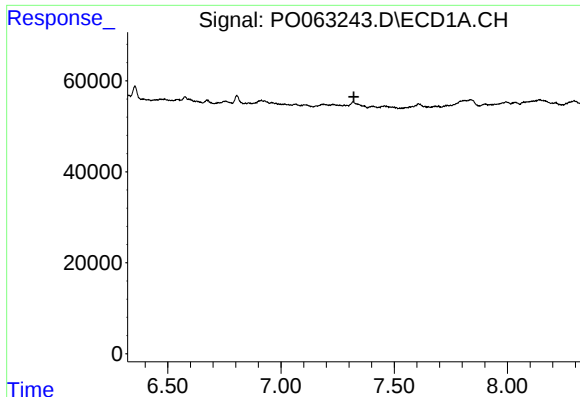

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.322 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

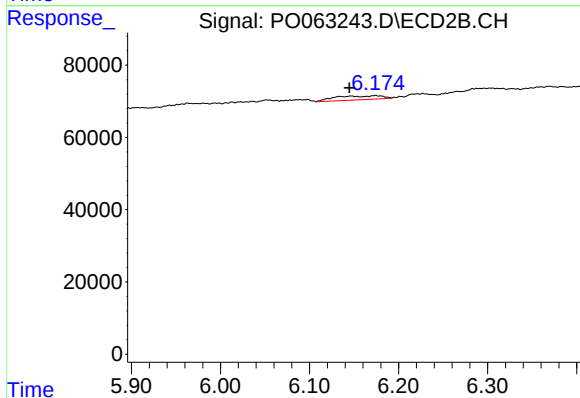


#32 AR-1260-2

R.T.: 6.174 min
Delta R.T.: 0.030 min
Response: 40109
Conc: 10.45 ng/ml

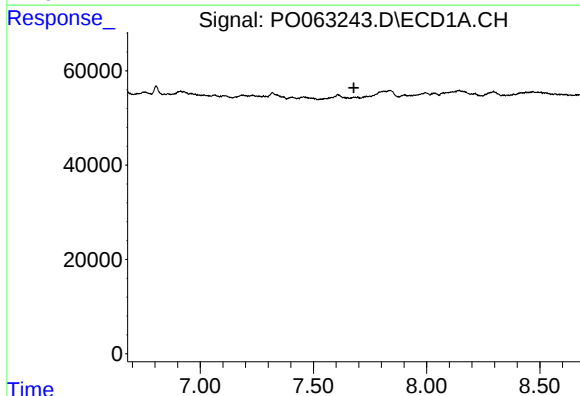


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.678 min
Response: 0
Conc: N.D.

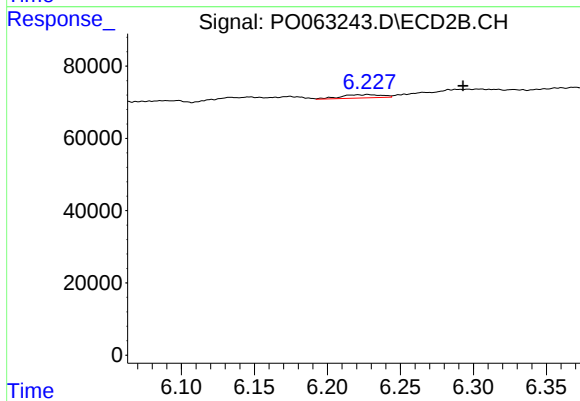

#33 AR-1260-3


R.T.: 6.228 min
Delta R.T.: -0.065 min
Response: 17677
Conc: 5.63 ng/ml

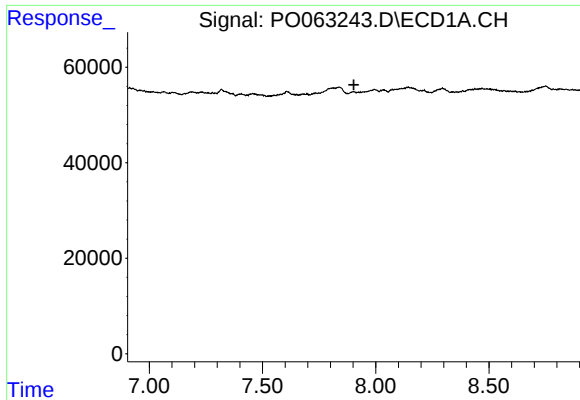

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

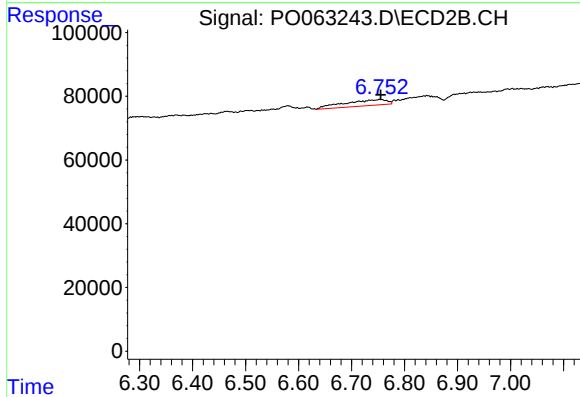


#34 AR-1260-4

R.T.: 6.753 min
Delta R.T.: -0.002 min
Response: 105167
Conc: 41.54 ng/ml

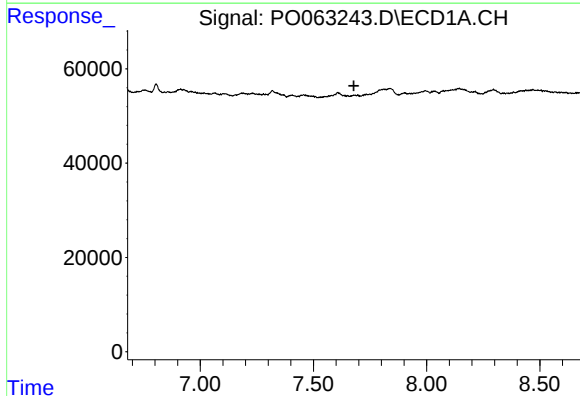

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.678 min
Response: 0
Conc: N.D.

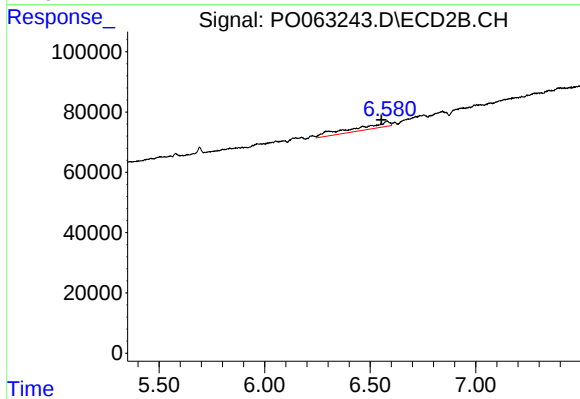

#36 AR-1262-1

R.T.: 6.580 min
Delta R.T.: 0.026 min
Response: 228016
Conc: 125.31 ng/ml