

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063243.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2019 18:50
 Operator : HP/AJ
 Sample : K5569-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-DECON-WATER-102519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:07:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.481	198583	191231	3.407	3.502
2) SA Decachlor...	9.927	8.319	27787	24328	0.478m	0.569m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063243.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2019 18:50
Operator : HP/AJ
Sample : K5569-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:07:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

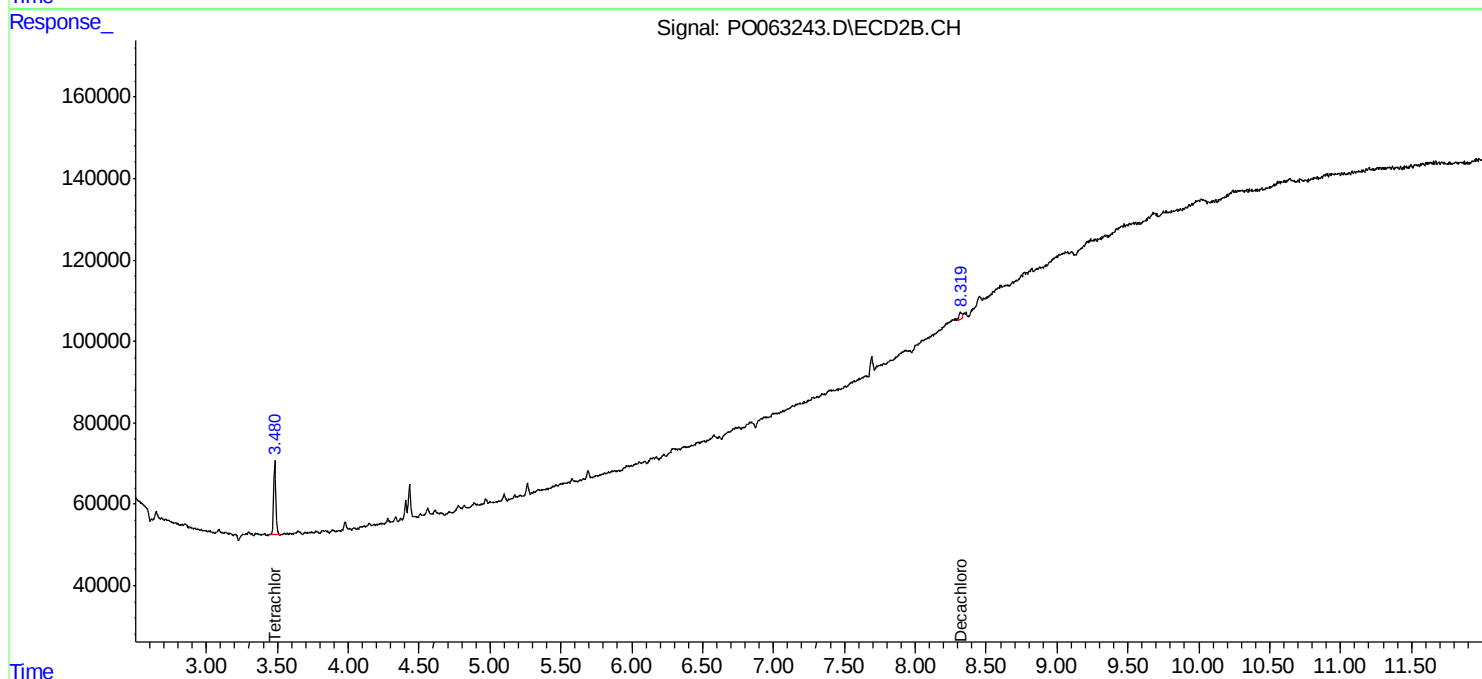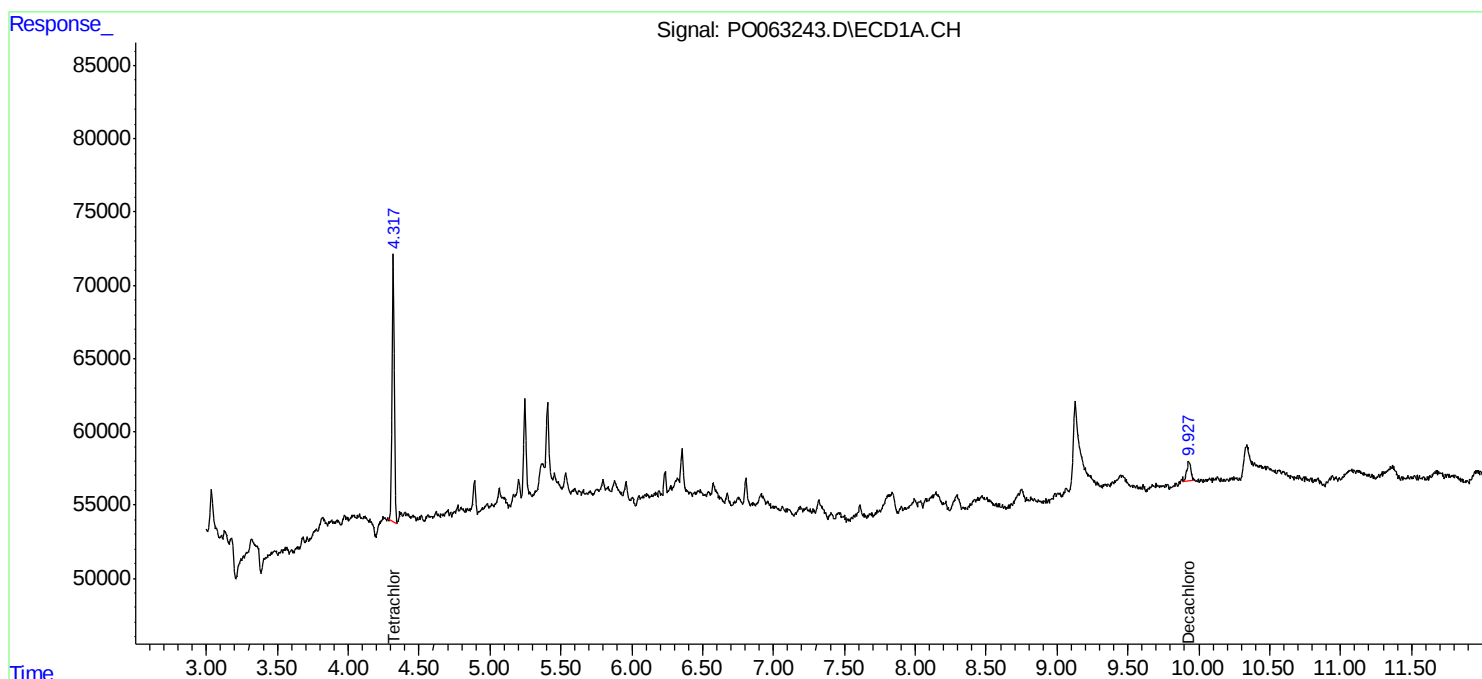


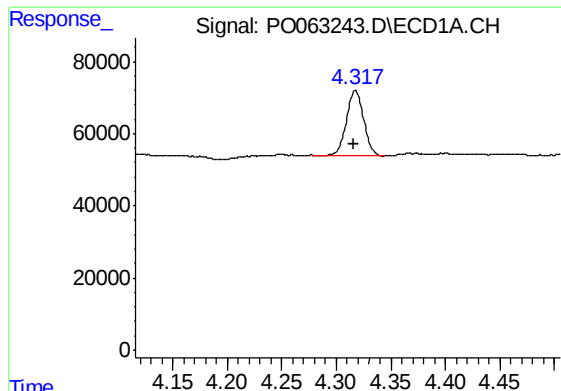

#1 Tetrachloro-m-xylene


R.T.: 4.317 min
Delta R.T.: 0.001 min
Response: 198583
Conc: 3.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519

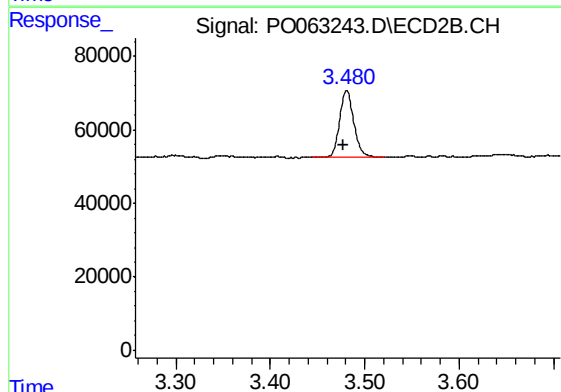


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.003 min
Response: 191231
Conc: 3.50 ng/ml

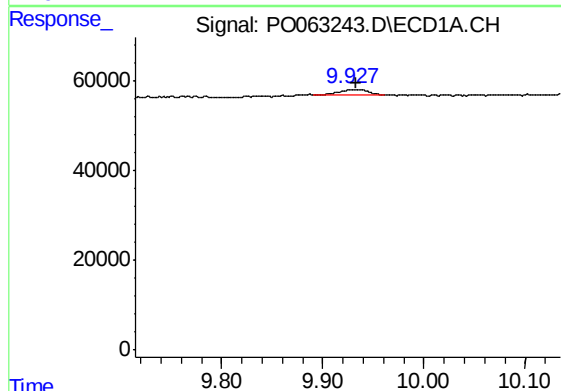

#2 Decachlorobiphenyl

R.T.: 9.927 min
Delta R.T.: -0.007 min
Response: 27787
Conc: 0.48 ng/ml m

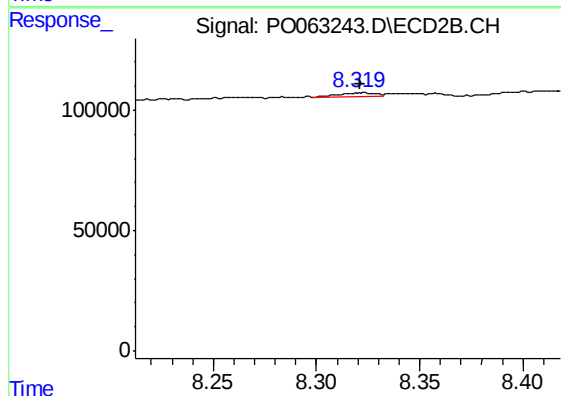

#2 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: -0.002 min
Response: 24328
Conc: 0.57 ng/ml m