

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063250.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2019 20:46
 Operator : HP/AJ
 Sample : K5563-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 10/30/2019 3:31:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 11:34:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.479	942706	932392	16.175m	17.073
2)	SA Decachlor...	9.934	8.320	647948	439945	11.136	10.291
Target Compounds							
26)	L6 AR-1254-1	6.322	5.297	48613	33008	19.121m	10.958m#
27)	L6 AR-1254-2	6.542	5.440	101466	33782	25.084	12.526 #
28)	L6 AR-1254-3	6.904	5.832	100615	97297	23.639m	22.663m
29)	L6 AR-1254-4	7.188	6.055	64804	38731	19.146m	13.592m#
30)	L6 AR-1254-5	7.605	6.463	103078	93779	31.076m	25.158m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2019 20:46
Operator : HP/AJ
Sample : K5563-10
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
10/30/2019 3:31:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 11:34:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

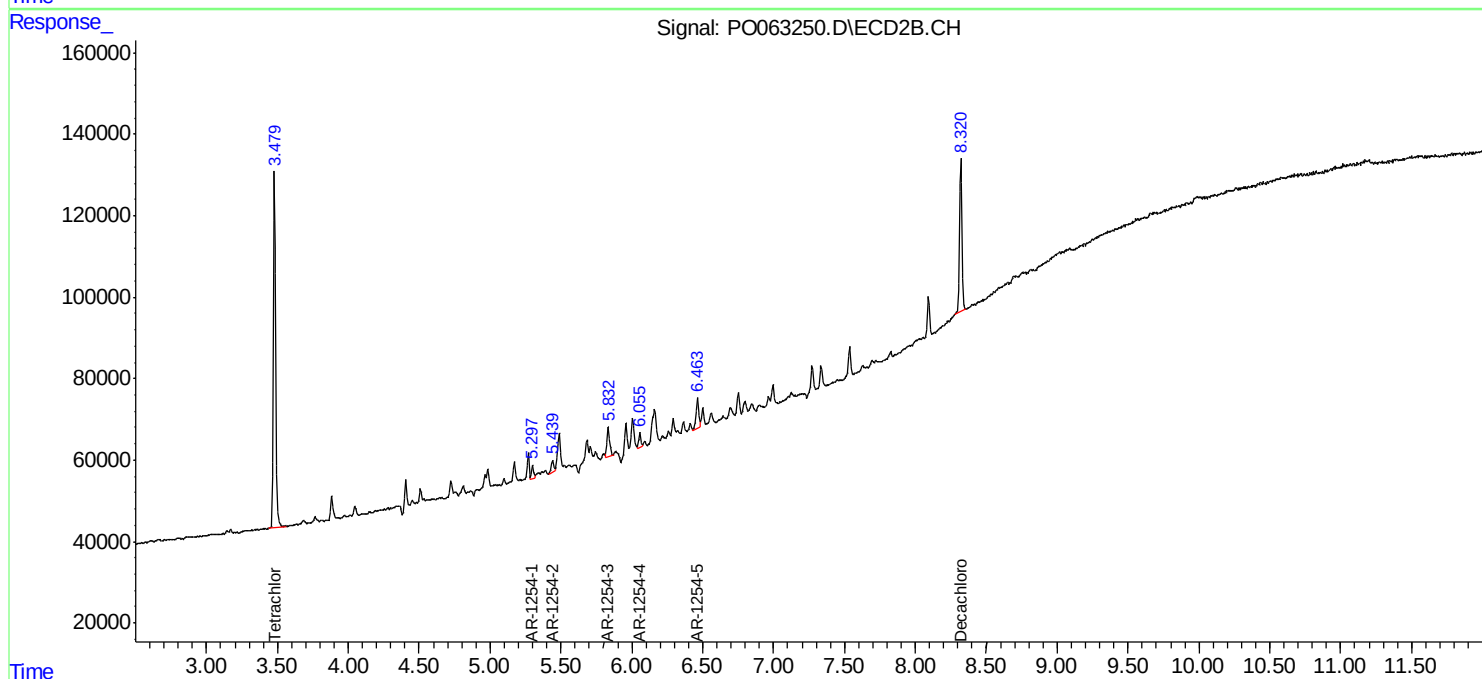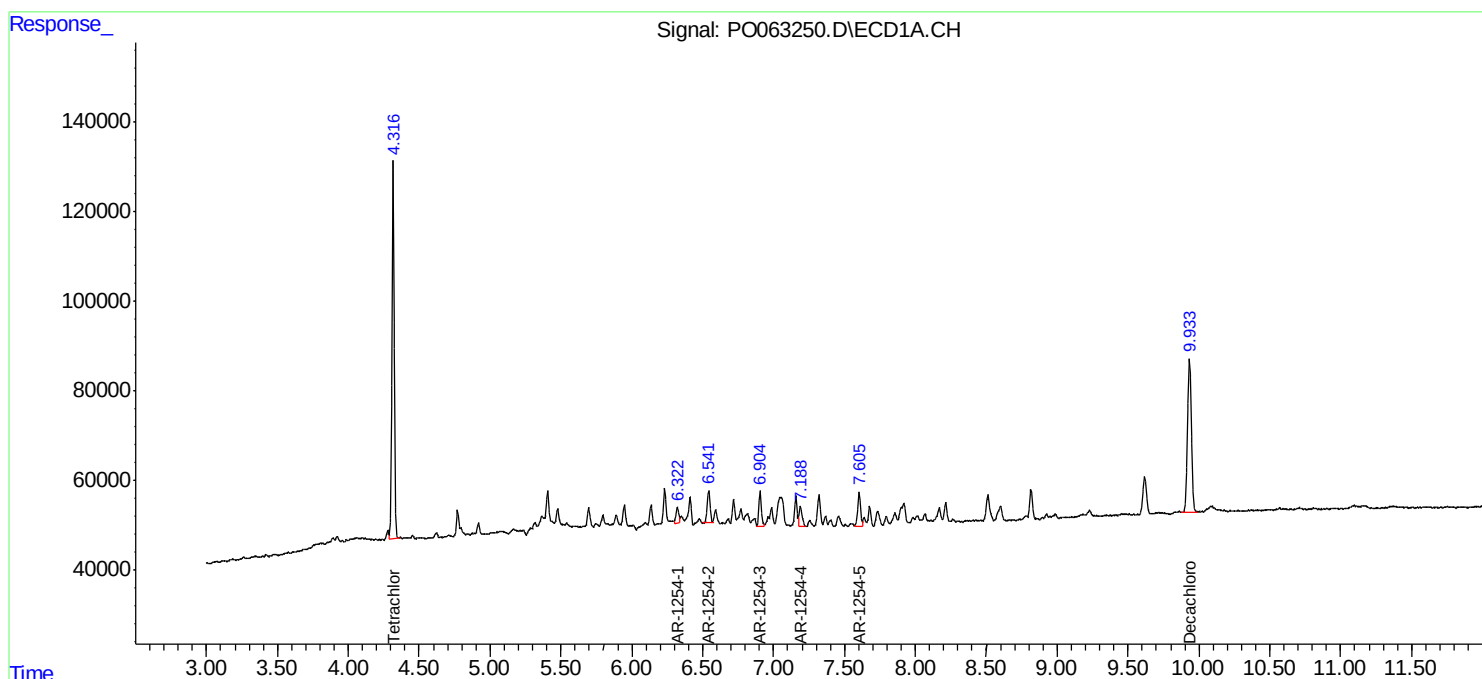

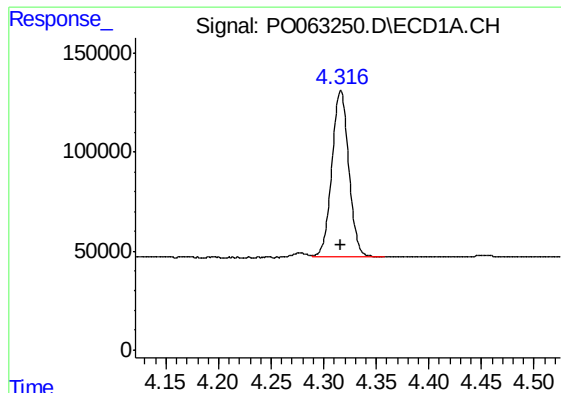


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 942706
Conc: 16.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
10/30/2019 3:31:34 PM

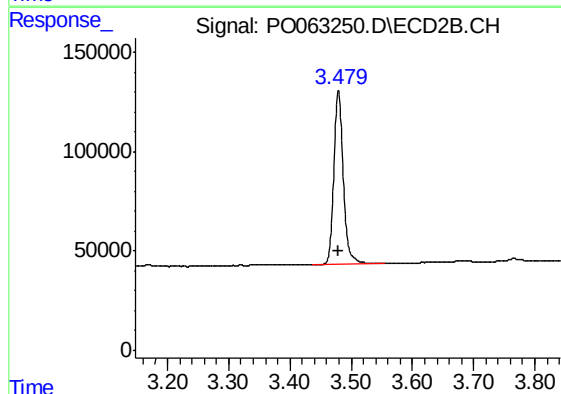


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.001 min
Response: 932392
Conc: 17.07 ng/ml

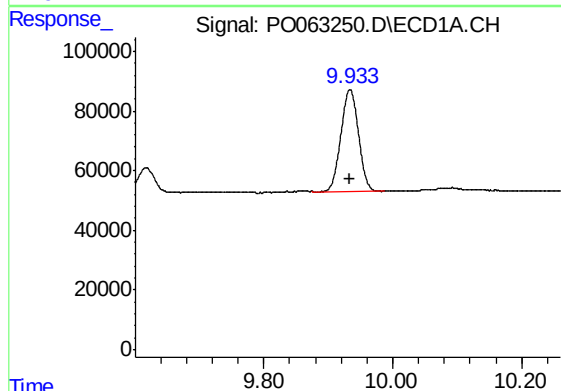


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: 0.000 min
Response: 647948
Conc: 11.14 ng/ml

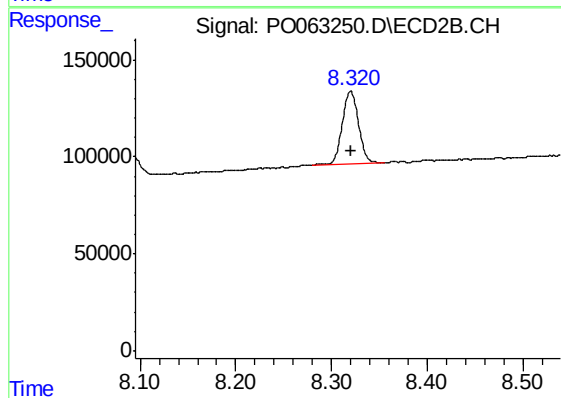

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 439945
Conc: 10.29 ng/ml

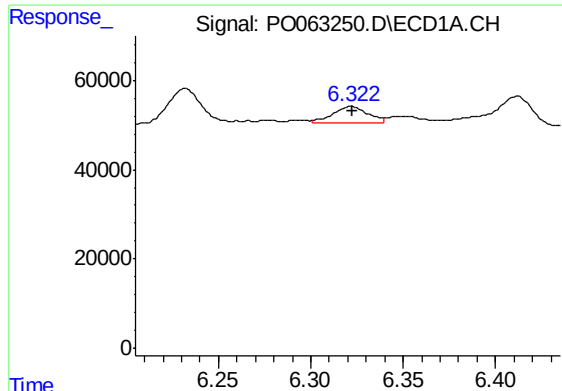


#26 AR-1254-1

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 48613
Conc: 19.12 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
10/30/2019 3:31:34 PM

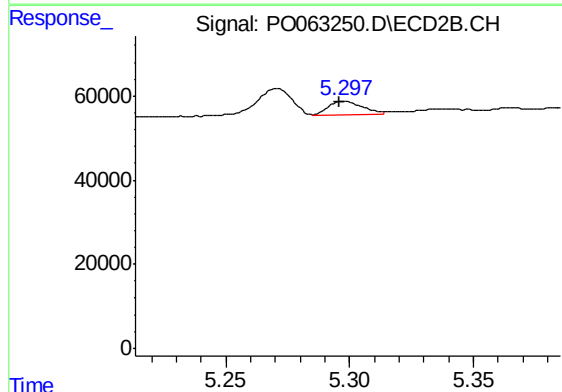


#26 AR-1254-1

R.T.: 5.297 min
Delta R.T.: 0.001 min
Response: 33008
Conc: 10.96 ng/ml m

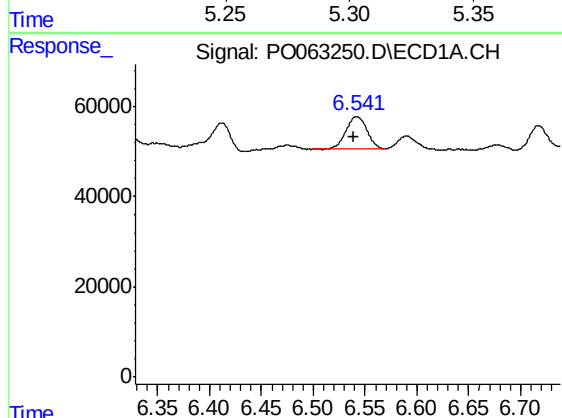


#27 AR-1254-2

R.T.: 6.542 min
Delta R.T.: 0.003 min
Response: 101466
Conc: 25.08 ng/ml

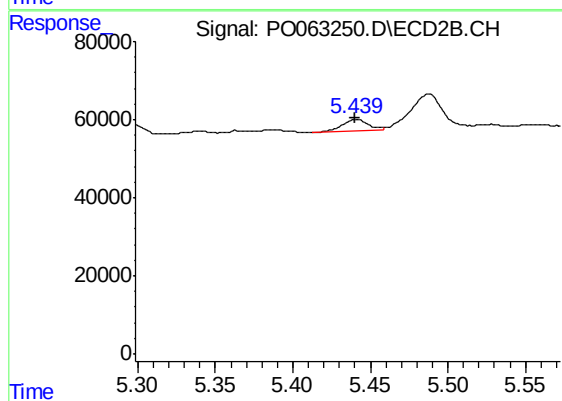

#27 AR-1254-2

R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 33782
Conc: 12.53 ng/ml

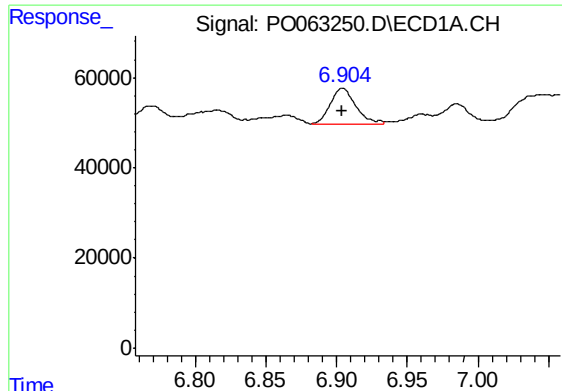


#28 AR-1254-3

R.T.: 6.904 min
Delta R.T.: 0.000 min
Response: 100615
Conc: 23.64 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
10/30/2019 3:31:34 PM

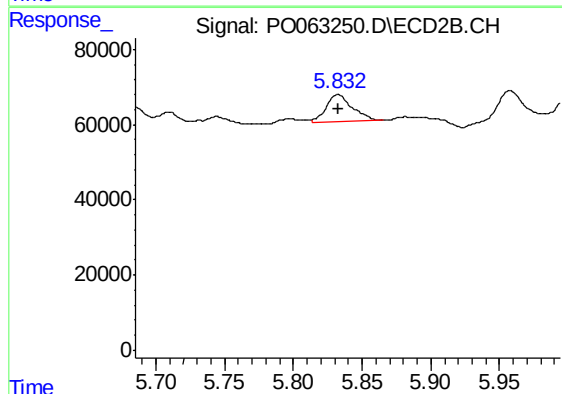


#28 AR-1254-3

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 97297
Conc: 22.66 ng/ml m

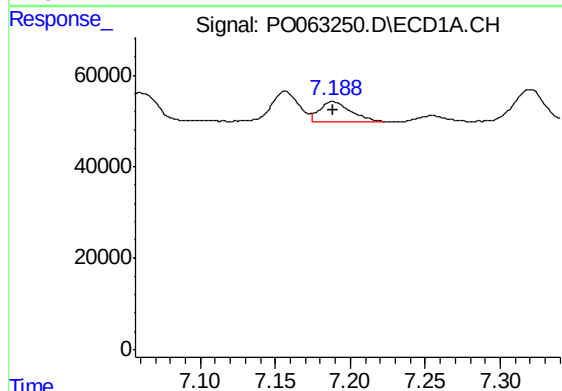


#29 AR-1254-4

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 64804
Conc: 19.15 ng/ml m

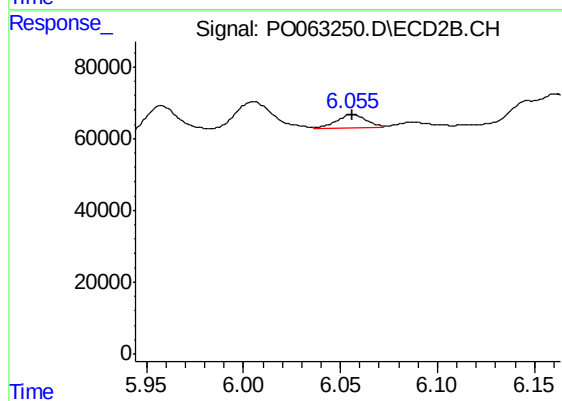

#29 AR-1254-4

R.T.: 6.055 min
Delta R.T.: -0.001 min
Response: 38731
Conc: 13.59 ng/ml m

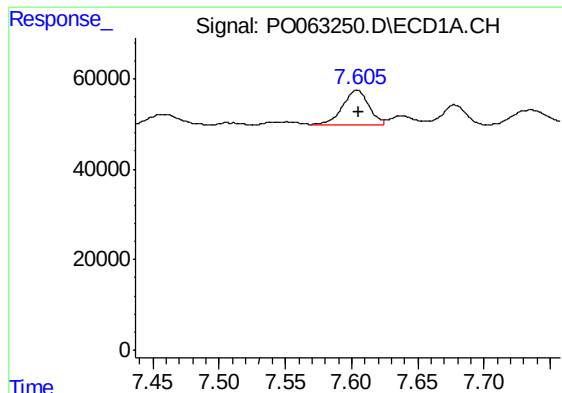


#30 AR-1254-5

R.T.: 7.605 min
Delta R.T.: -0.001 min
Response: 103078
Conc: 31.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
10/30/2019 3:31:34 PM

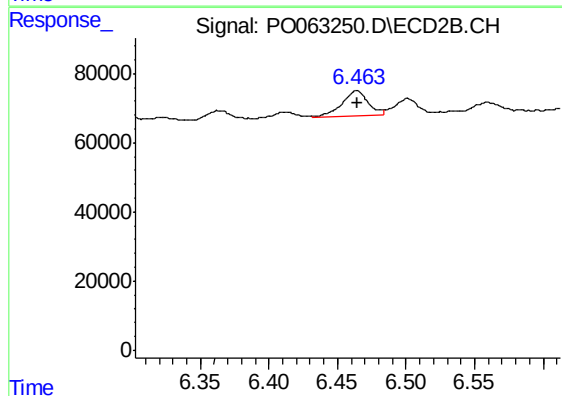

#30 AR-1254-5

R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 93779
Conc: 25.16 ng/ml m