

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063251.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2019 21:02
 Operator : HP/AJ
 Sample : K5563-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 10/30/2019 1:59:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:10:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.316	3.479	830253	842630	14.246m	15.429
2) SA Decachlor...	9.932	8.320	630265	427345	10.832	9.996
Target Compounds						
26) L6 AR-1254-1	6.322	5.296	225079	218230	88.530	72.447
27) L6 AR-1254-2	6.539	5.440	484055	229318	119.667	85.027 #
28) L6 AR-1254-3	6.905	5.831	447847	494011	105.217	115.068
29) L6 AR-1254-4	7.188	6.056	319539	269403	94.404	94.539
30) L6 AR-1254-5	7.604	6.463	269609	327979	81.281	87.986

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063251.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2019 21:02
Operator : HP/AJ
Sample : K5563-07
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-1


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:10:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

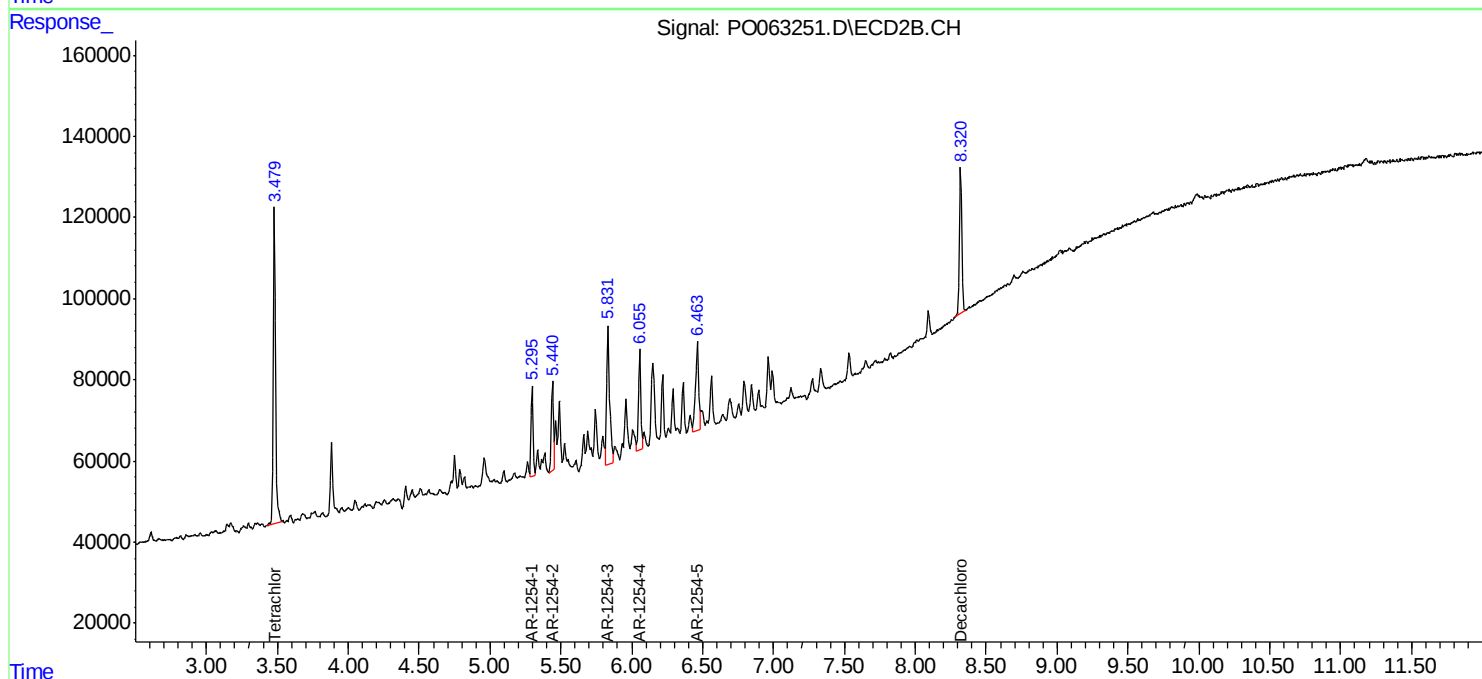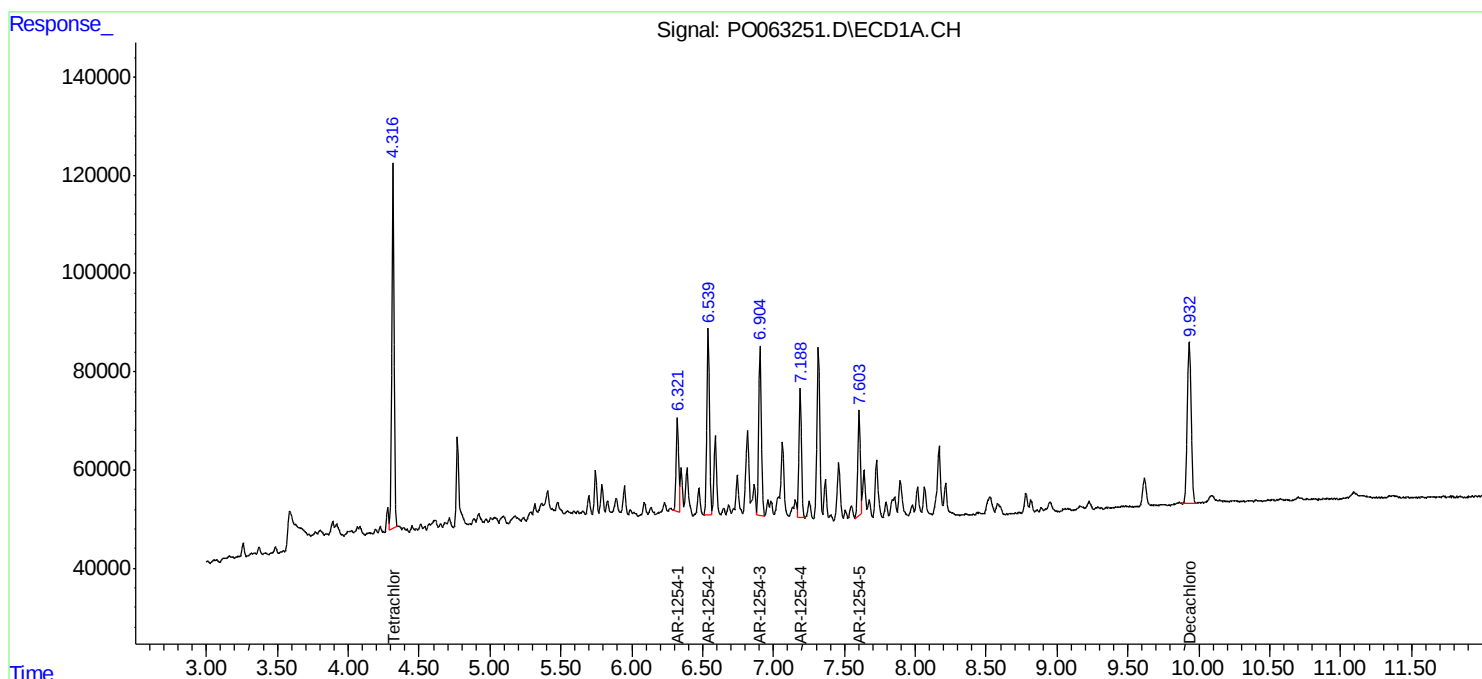

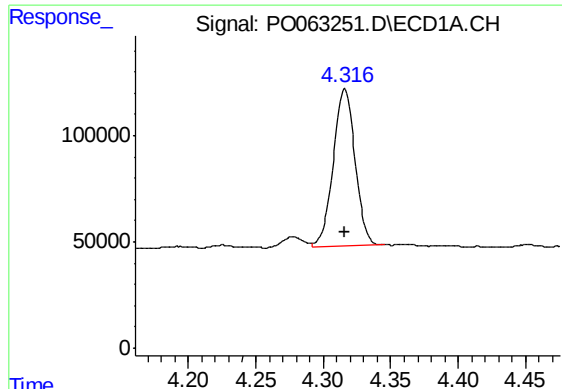


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 830253
Conc: 14.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:01 PM

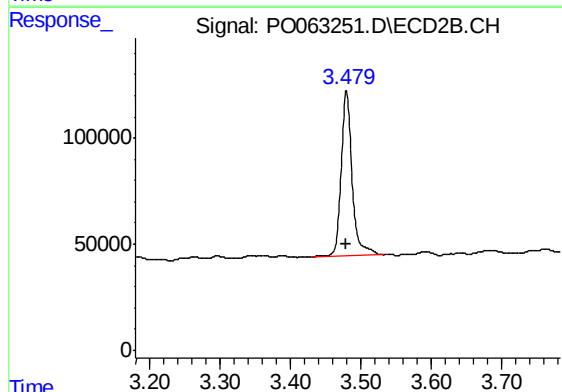


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.001 min
Response: 842630
Conc: 15.43 ng/ml

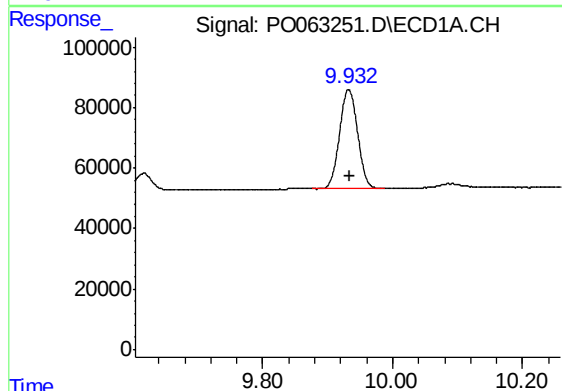


#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.001 min
Response: 630265
Conc: 10.83 ng/ml

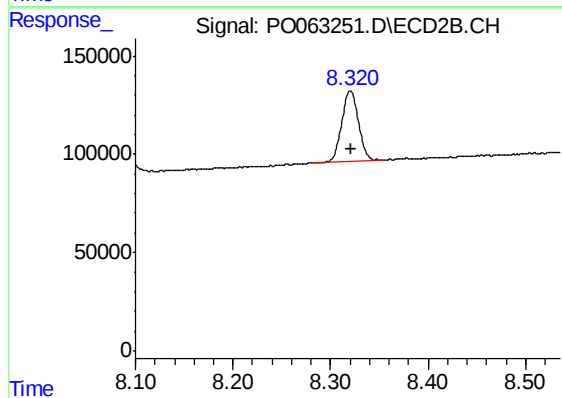

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 427345
Conc: 10.00 ng/ml

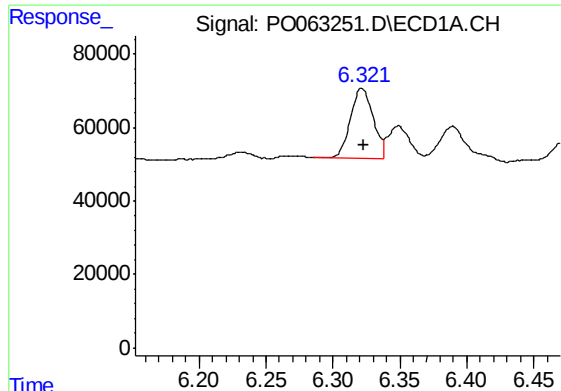


#26 AR-1254-1

R.T.: 6.322 min
Delta R.T.: -0.001 min
Response: 225079
Conc: 88.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:01 PM

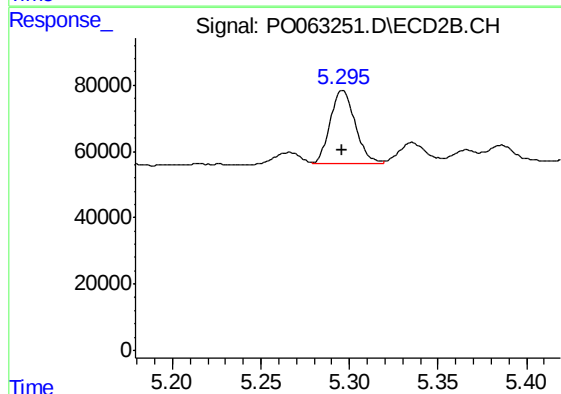


#26 AR-1254-1

R.T.: 5.296 min
Delta R.T.: 0.000 min
Response: 218230
Conc: 72.45 ng/ml

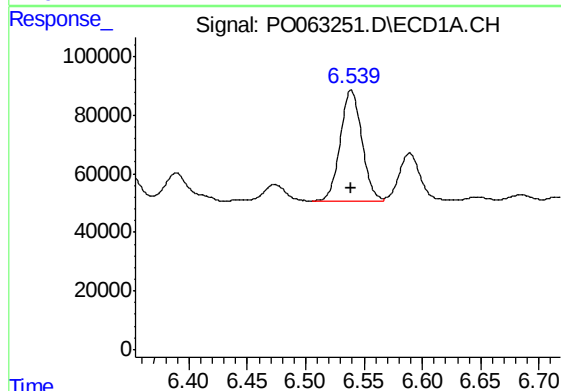


#27 AR-1254-2

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 484055
Conc: 119.67 ng/ml

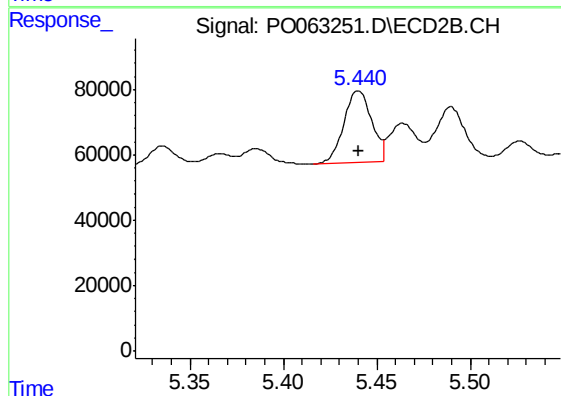

#27 AR-1254-2

R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 229318
Conc: 85.03 ng/ml

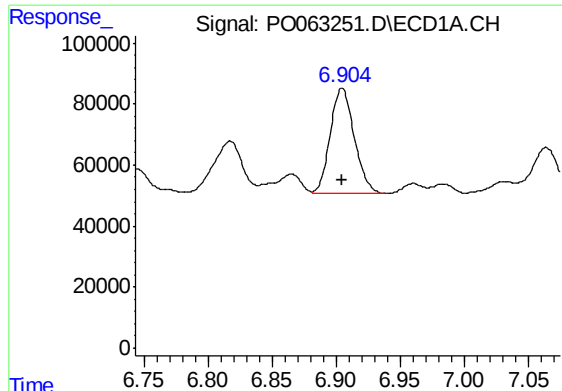


#28 AR-1254-3

R.T.: 6.905 min
Delta R.T.: 0.000 min
Response: 447847
Conc: 105.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:01 PM

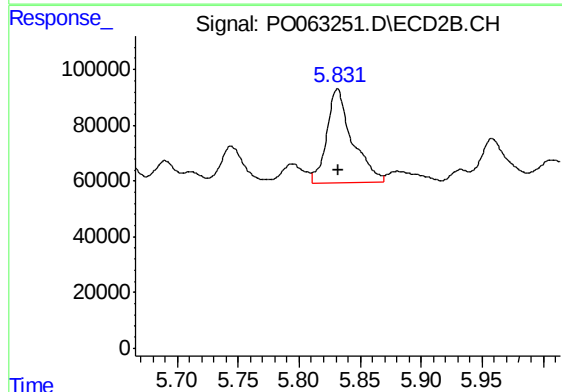


#28 AR-1254-3

R.T.: 5.831 min
Delta R.T.: 0.000 min
Response: 494011
Conc: 115.07 ng/ml

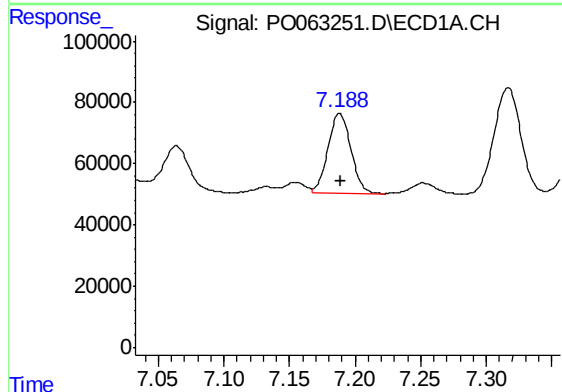


#29 AR-1254-4

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 319539
Conc: 94.40 ng/ml

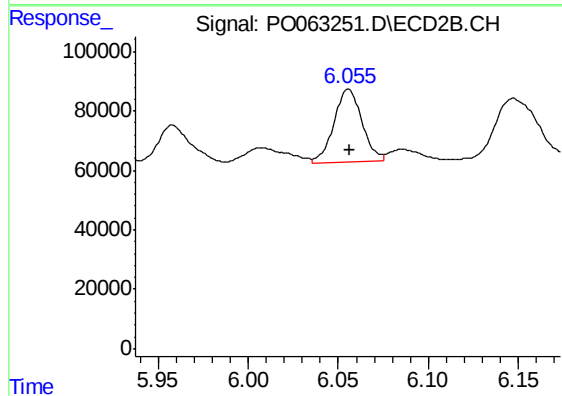

#29 AR-1254-4

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 269403
Conc: 94.54 ng/ml

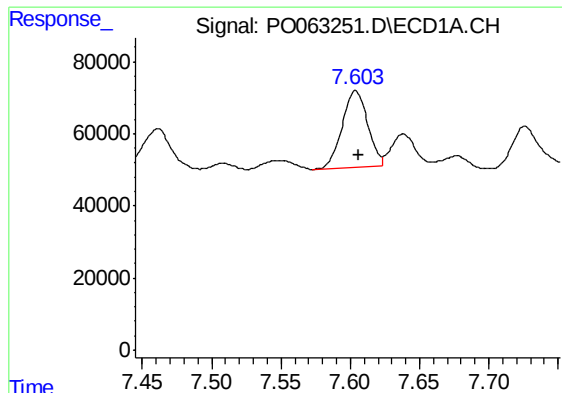


#30 AR-1254-5

R.T.: 7.604 min
Delta R.T.: -0.002 min
Response: 269609
Conc: 81.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:01 PM

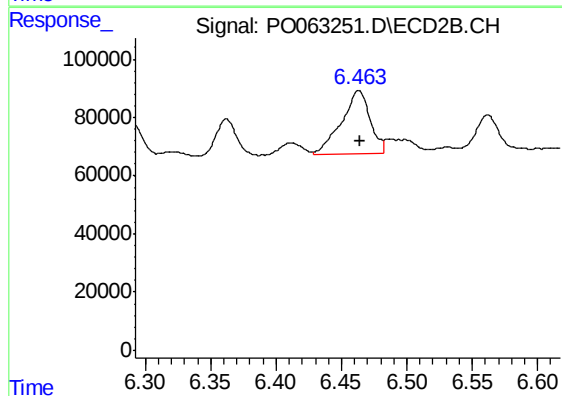

#30 AR-1254-5

R.T.: 6.463 min
Delta R.T.: -0.001 min
Response: 327979
Conc: 87.99 ng/ml