

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063252.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2019 21:19
 Operator : HP/AJ
 Sample : K5542-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 608-60-(0-1.5)

Manual Integrations
 APPROVED

Ankita
 10/30/2019 1:59:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:10:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.479	937335	931555	16.083m	17.057
2)	SA Decachlor...	9.932	8.320	637930	445168	10.964	10.413
Target Compounds							
26)	L6 AR-1254-1	6.323	5.298	186810	213917	73.477m	71.015
27)	L6 AR-1254-2	6.540	5.441	280030	132158	69.228	49.002 #
28)	L6 AR-1254-3	6.906	5.832	340560	280265	80.011	65.281
29)	L6 AR-1254-4	7.188	6.056	148711	163097	43.935	57.234 #
30)	L6 AR-1254-5	7.604	6.463	260145	237626	78.428	63.747

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063252.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2019 21:19
Operator : HP/AJ
Sample : K5542-17
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
608-60-(0-1.5)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:10:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

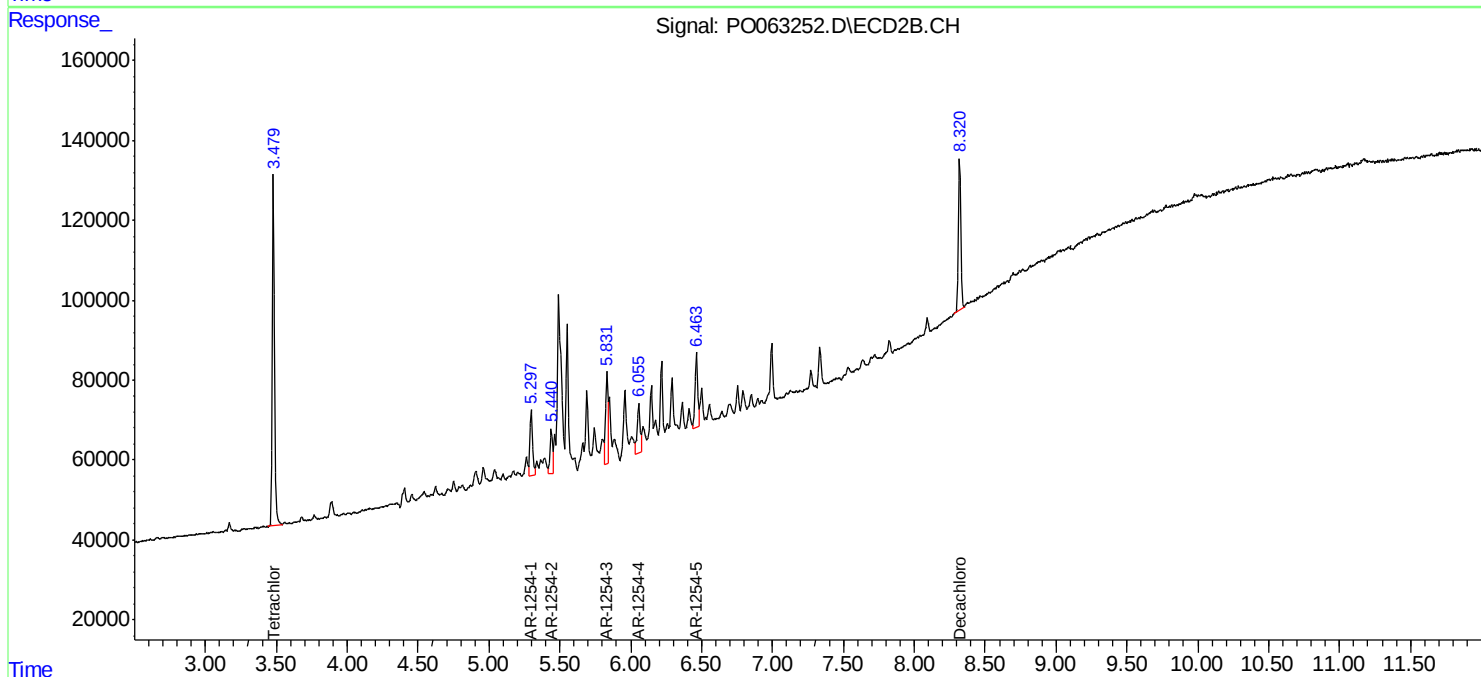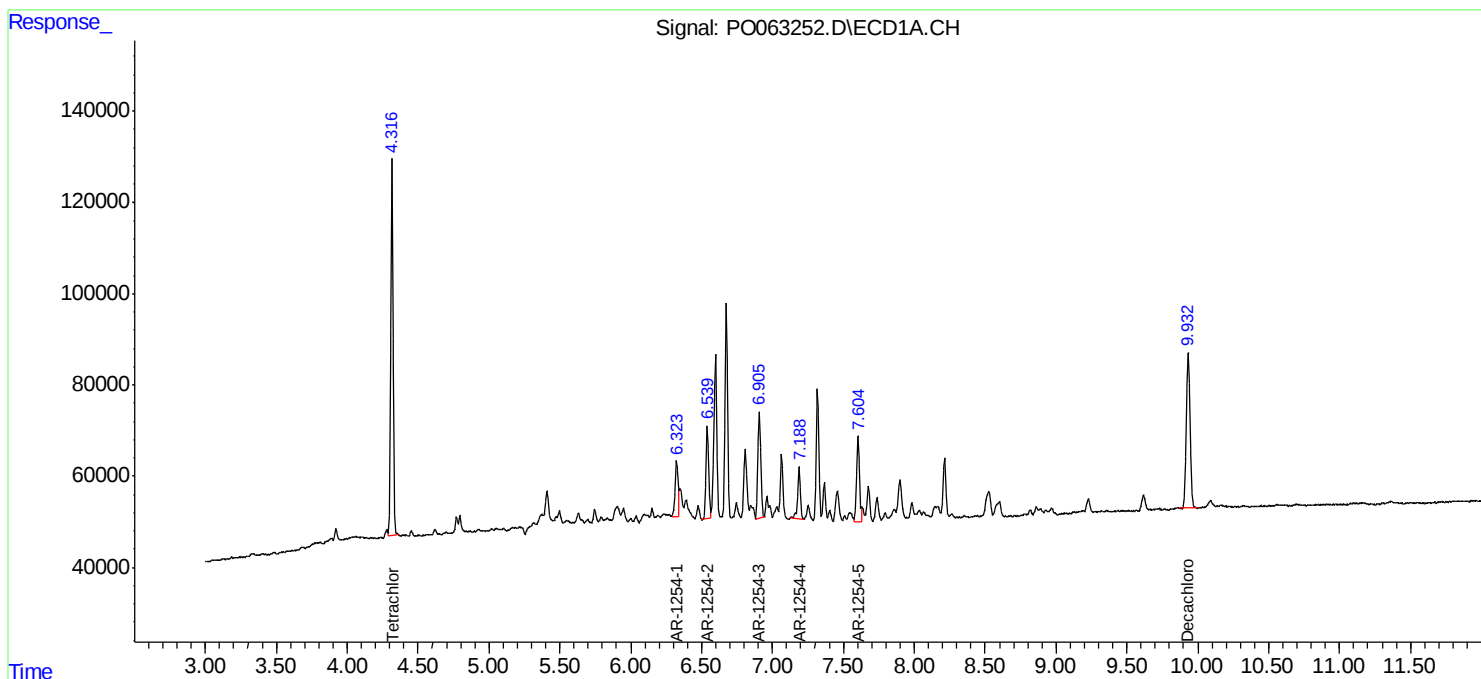

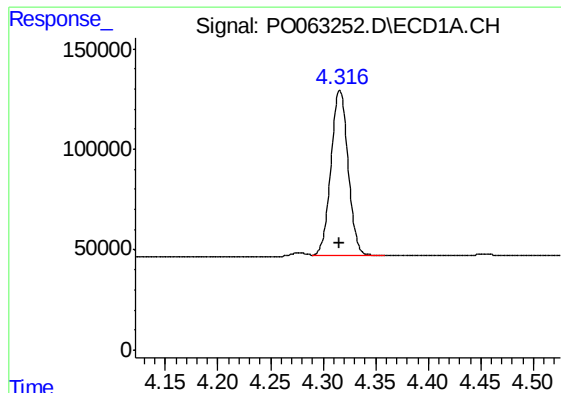


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 937335
Conc: 16.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
608-60-(0-1.5)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:03 PM

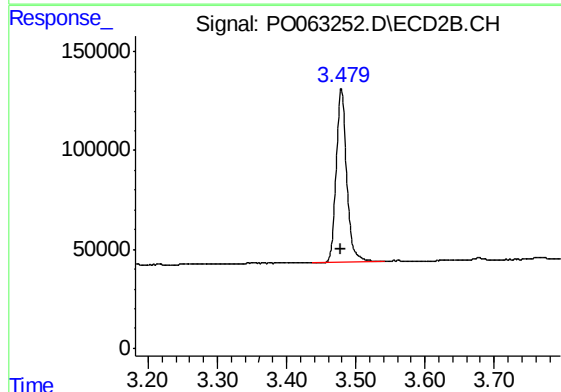


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.001 min
Response: 931555
Conc: 17.06 ng/ml

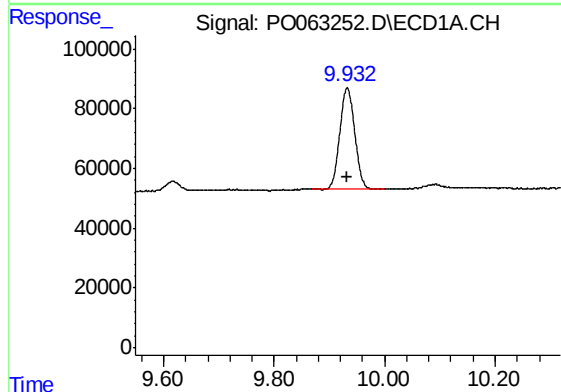


#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.001 min
Response: 637930
Conc: 10.96 ng/ml

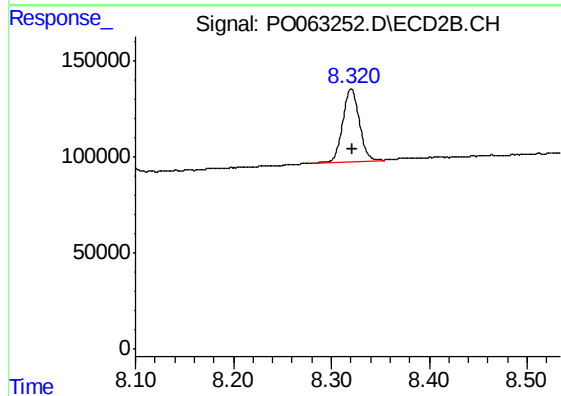

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 445168
Conc: 10.41 ng/ml

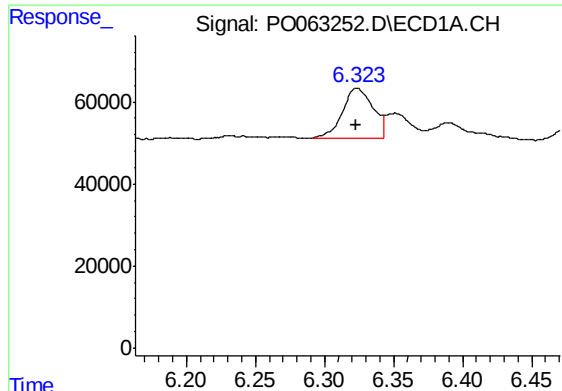


#26 AR-1254-1

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 186810
Conc: 73.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
608-60-(0-1.5)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:03 PM

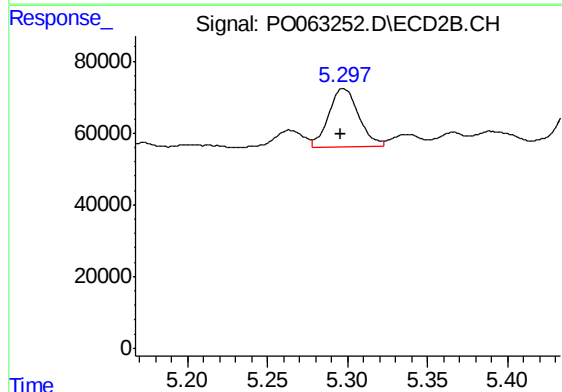


#26 AR-1254-1

R.T.: 5.298 min
Delta R.T.: 0.002 min
Response: 213917
Conc: 71.01 ng/ml

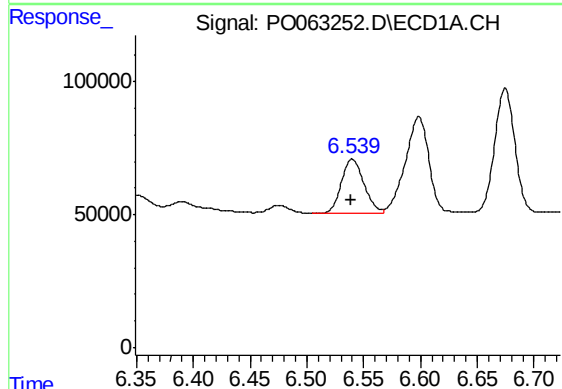


#27 AR-1254-2

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 280030
Conc: 69.23 ng/ml

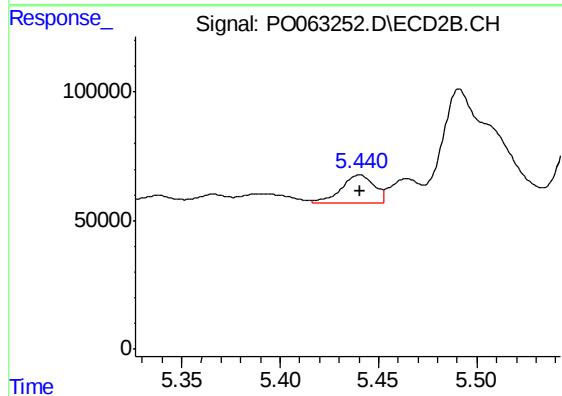

#27 AR-1254-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 132158
Conc: 49.00 ng/ml

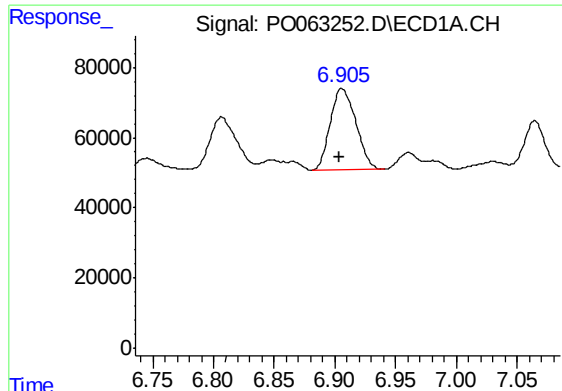


#28 AR-1254-3

R.T.: 6.906 min
Delta R.T.: 0.001 min
Response: 340560
Conc: 80.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
608-60-(0-1.5)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:03 PM

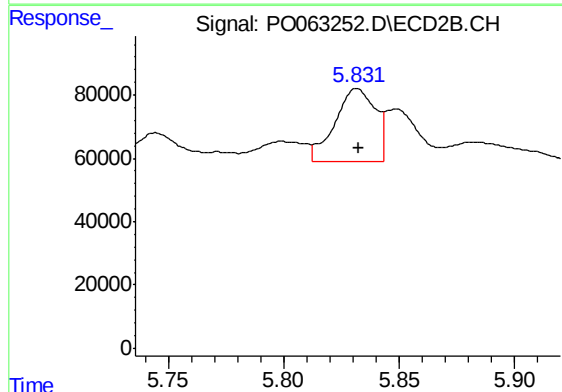


#28 AR-1254-3

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 280265
Conc: 65.28 ng/ml

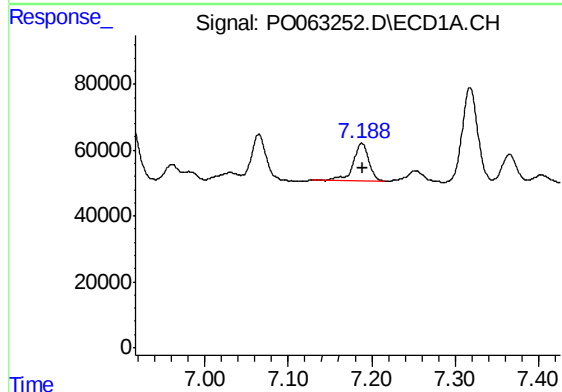


#29 AR-1254-4

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 148711
Conc: 43.93 ng/ml

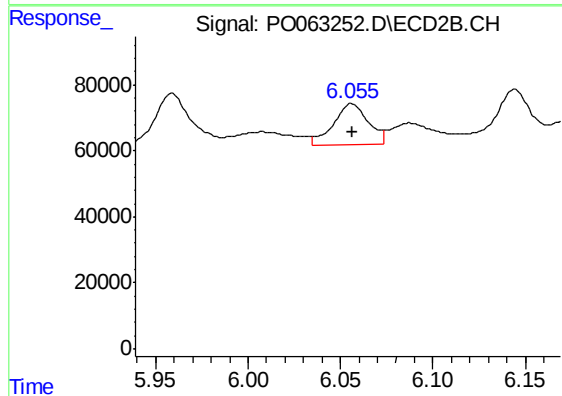

#29 AR-1254-4

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 163097
Conc: 57.23 ng/ml

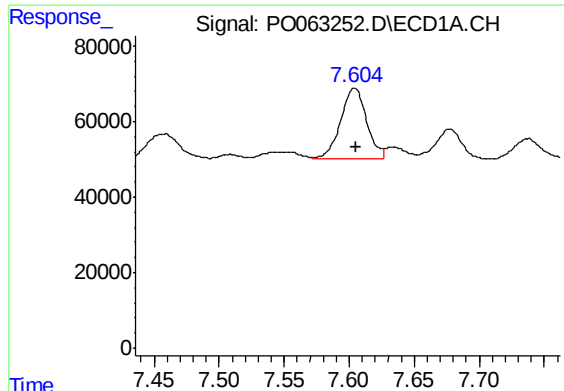


#30 AR-1254-5

R.T.: 7.604 min
Delta R.T.: -0.002 min
Response: 260145
Conc: 78.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
608-60-(0-1.5)

Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:03 PM

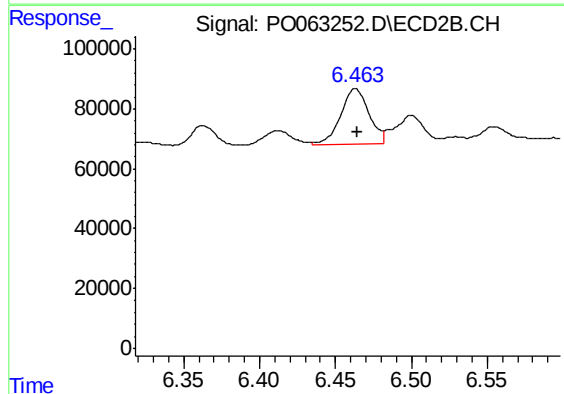

#30 AR-1254-5

R.T.: 6.463 min
Delta R.T.: -0.001 min
Response: 237626
Conc: 63.75 ng/ml