

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063258.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2019 23:48
 Operator : HP/AJ
 Sample : K5149-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-01-102819

Manual Integrations
 APPROVED

Ankita
 10/30/2019 1:59:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:12:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.316	3.480	1194601	1132578	20.497m	20.738
2) SA Decachlor...	9.933	8.321	979557	618470	16.835	14.466

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063258.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2019 23:48
Operator : HP/AJ
Sample : K5149-07
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-01-102819


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:12:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

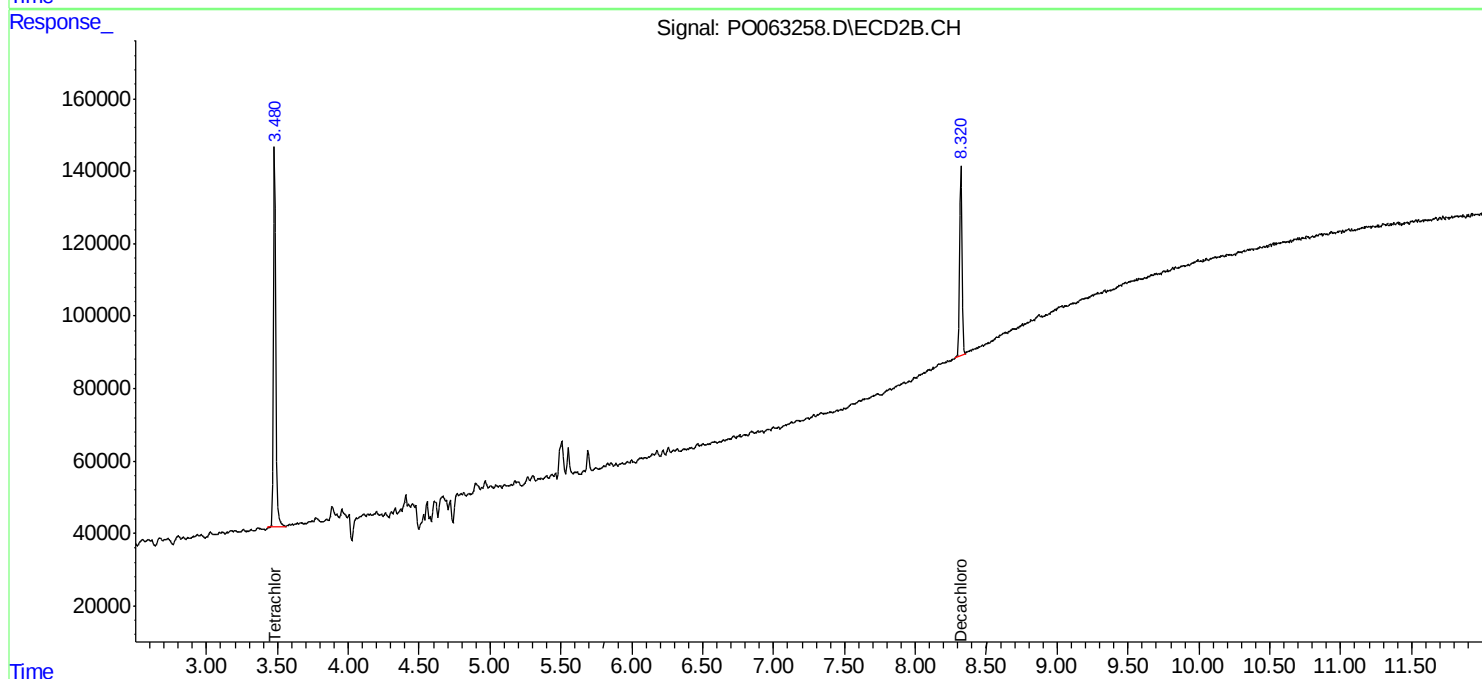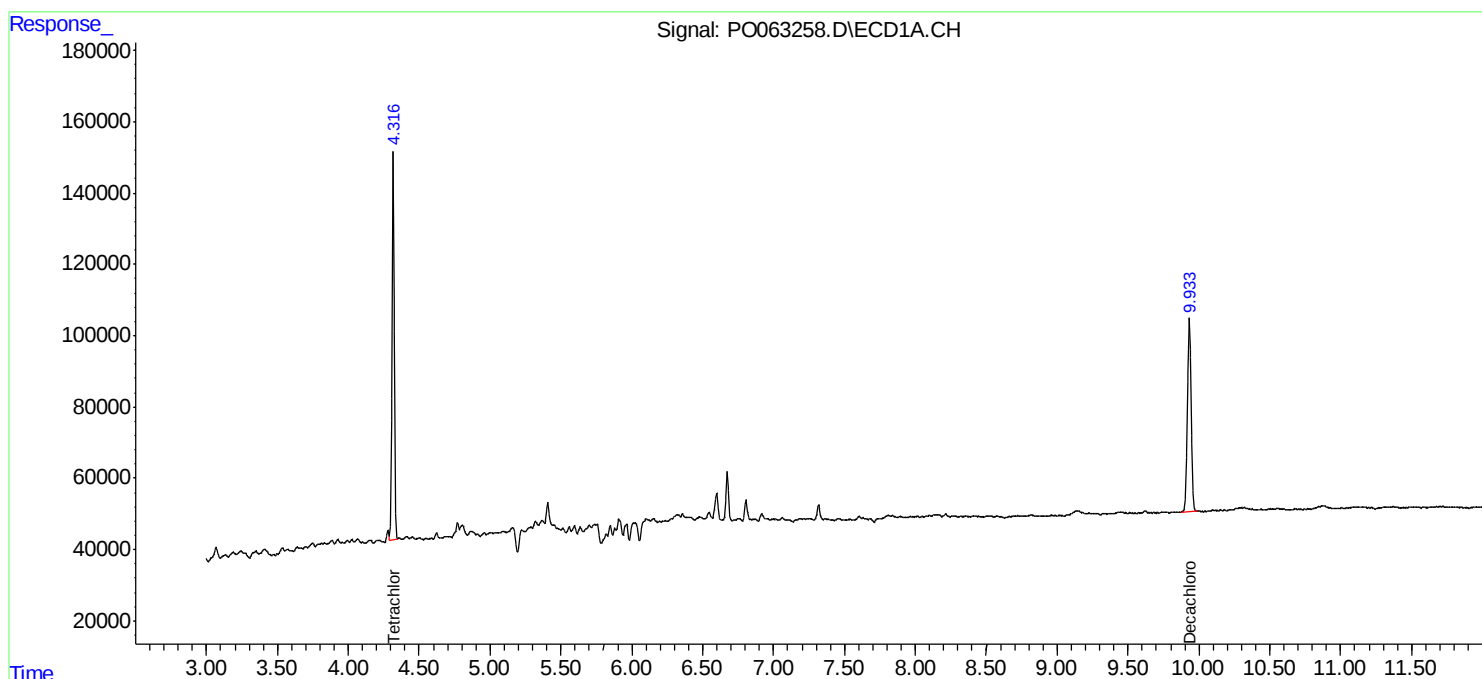

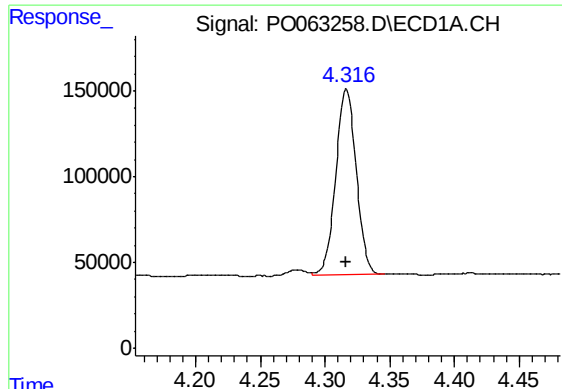


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 1194601
Conc: 20.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
EO-01-102819


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:28 PM

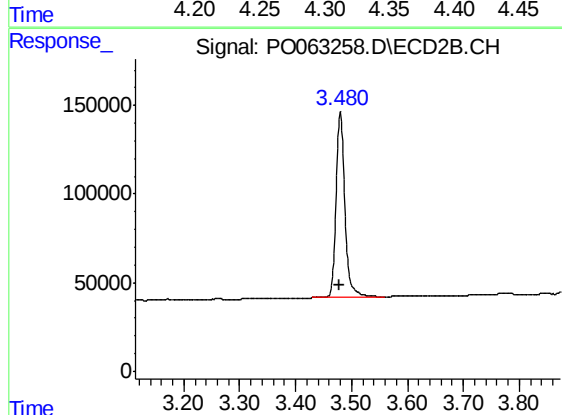


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 1132578
Conc: 20.74 ng/ml

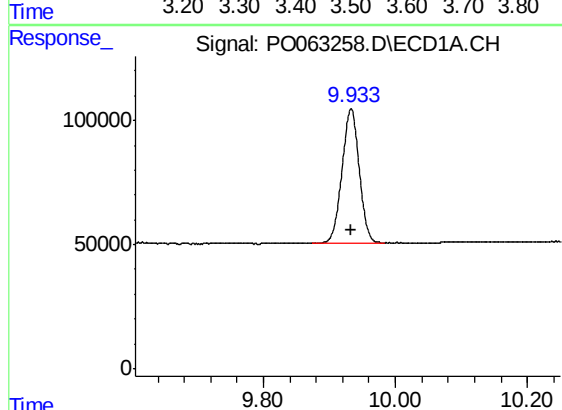

#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: 0.000 min
Response: 979557
Conc: 16.84 ng/ml

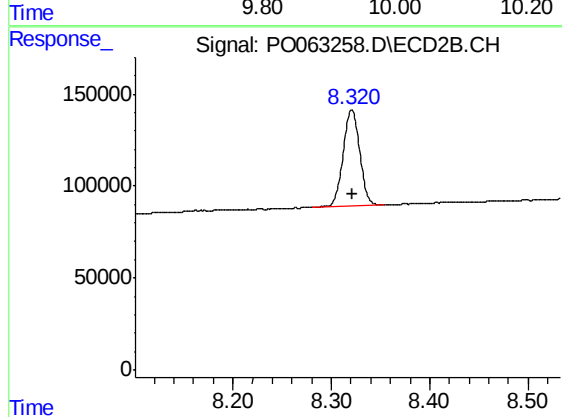

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 618470
Conc: 14.47 ng/ml