

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063264.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 1:27
 Operator : HP/AJ
 Sample : K5428-03
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-8B

Manual Integrations
 APPROVED

Ankita
 10/30/2019 1:59:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:13:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.317	3.480	1314567	1308418	22.556	23.958
2)	SA Decachlor...	9.933	8.321	870702	650251	14.964	15.210
Target Compounds							
26)	L6 AR-1254-1	6.321	5.296	281085	236047	110.558m	78.361 #
27)	L6 AR-1254-2	6.539	5.440	579510	326091	143.265	120.909
28)	L6 AR-1254-3	6.905	5.831	811172	823302	190.577	191.768
29)	L6 AR-1254-4	7.189	6.055	483129	457330	142.735	160.486
30)	L6 AR-1254-5	7.605	6.464	1102573	1395290	332.400m	374.309

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063264.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 1:27
Operator : HP/AJ
Sample : K5428-03
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
445X-8B


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:13:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

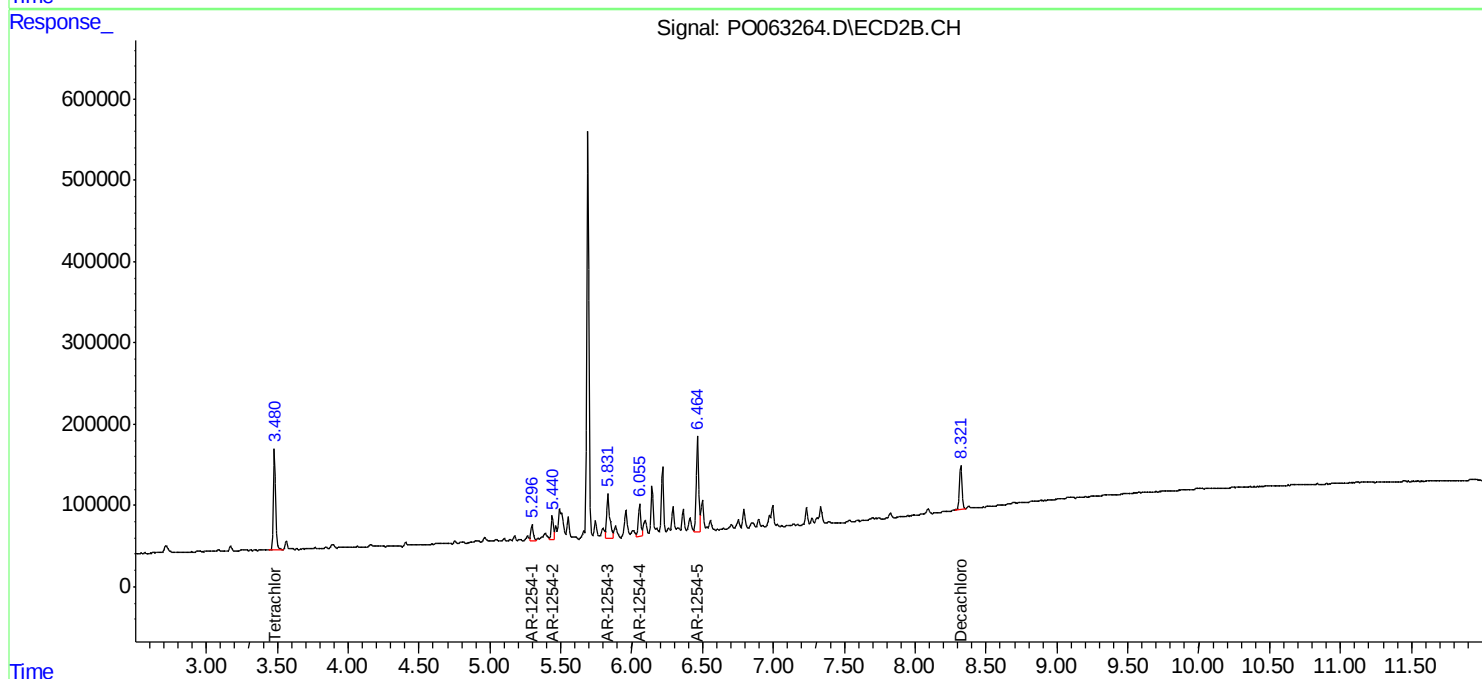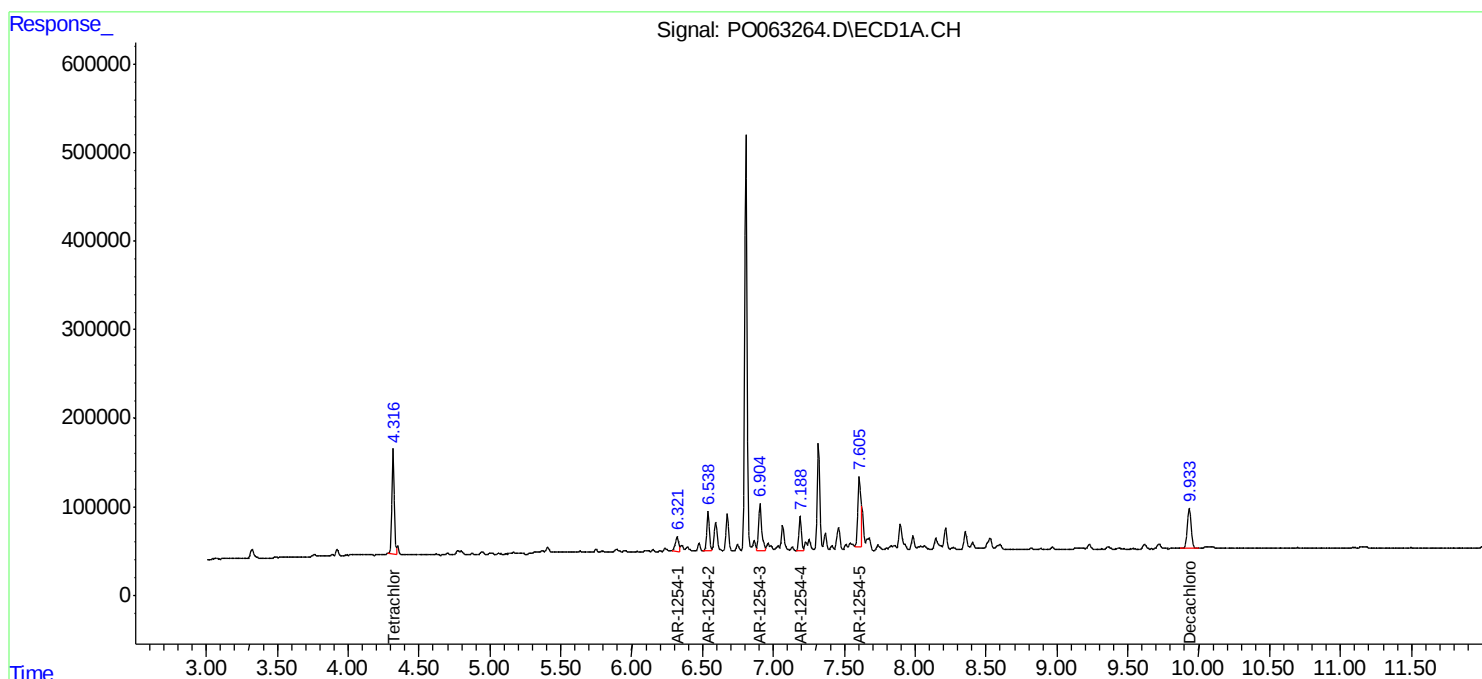

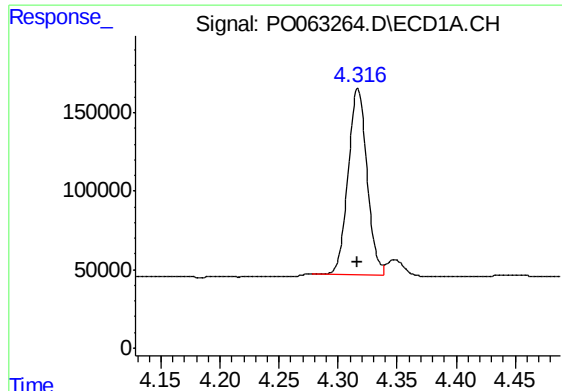


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: 0.000 min
Response: 1314567
Conc: 22.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-8B


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:38 PM

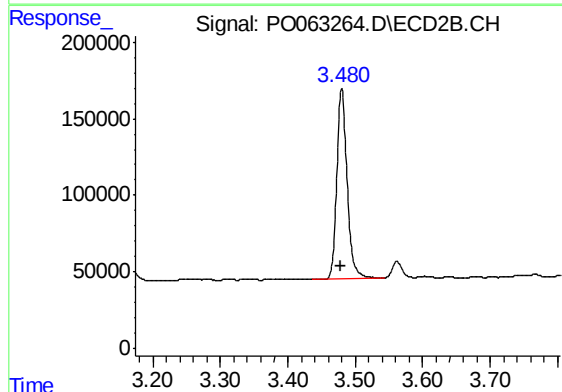


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 1308418
Conc: 23.96 ng/ml

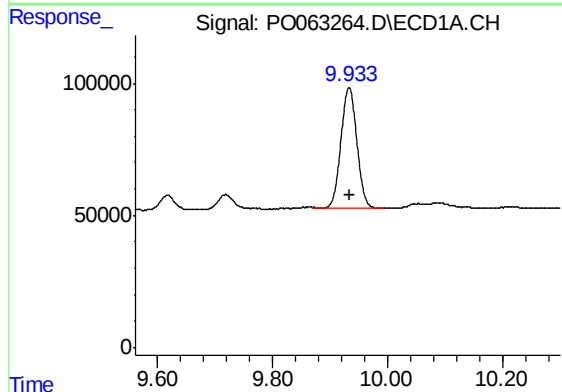


#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: 0.000 min
Response: 870702
Conc: 14.96 ng/ml

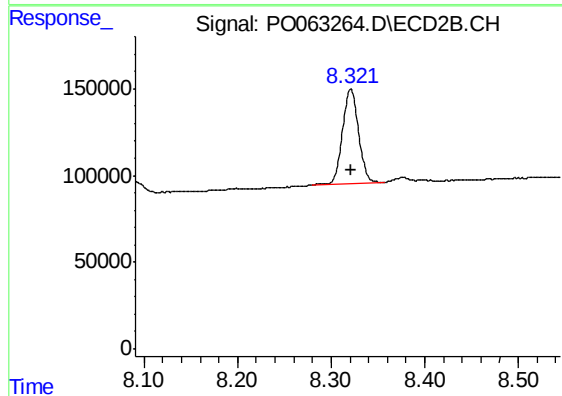

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 650251
Conc: 15.21 ng/ml

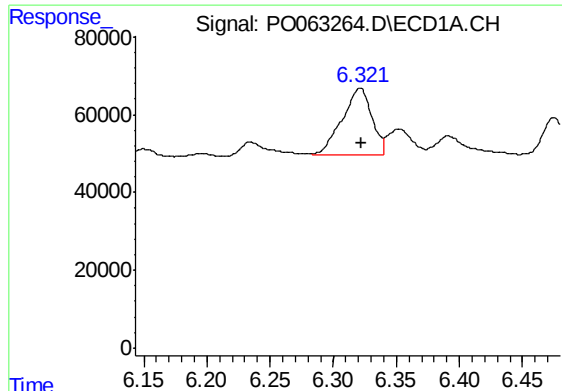


#26 AR-1254-1

R.T.: 6.321 min
Delta R.T.: -0.002 min
Response: 281085
Conc: 110.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-8B


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:38 PM

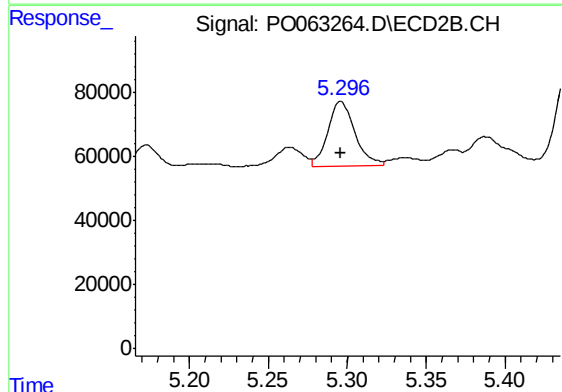


#26 AR-1254-1

R.T.: 5.296 min
Delta R.T.: 0.000 min
Response: 236047
Conc: 78.36 ng/ml

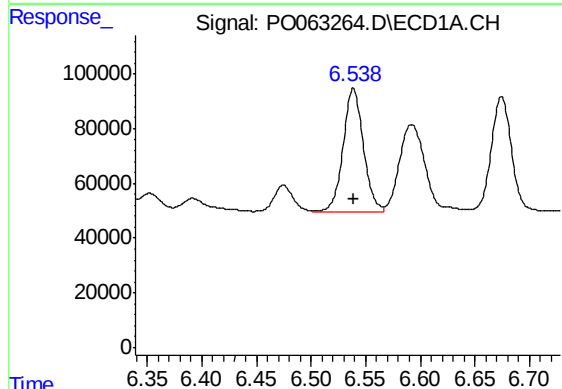


#27 AR-1254-2

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 579510
Conc: 143.27 ng/ml

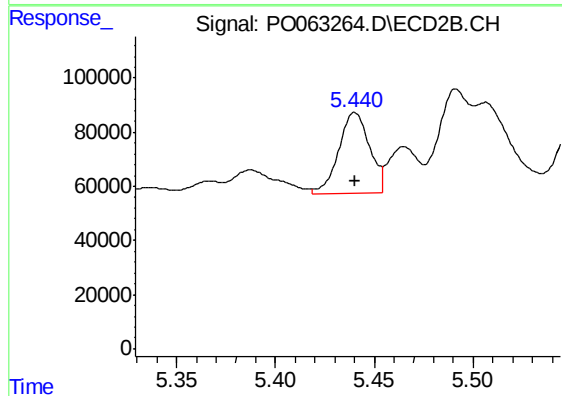

#27 AR-1254-2

R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 326091
Conc: 120.91 ng/ml

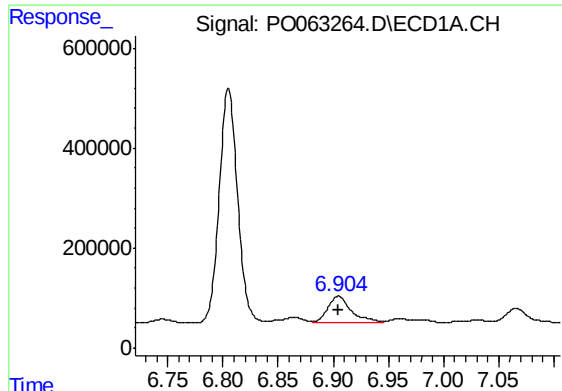


#28 AR-1254-3

R.T.: 6.905 min
Delta R.T.: 0.000 min
Response: 811172
Conc: 190.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-8B


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:38 PM

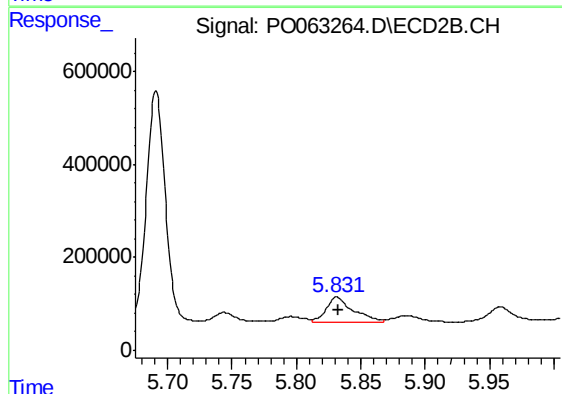


#28 AR-1254-3

R.T.: 5.831 min
Delta R.T.: 0.000 min
Response: 823302
Conc: 191.77 ng/ml

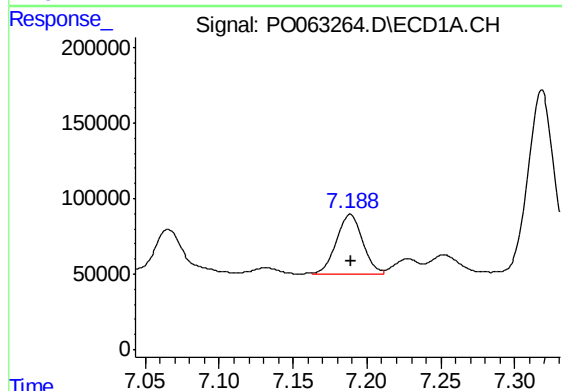


#29 AR-1254-4

R.T.: 7.189 min
Delta R.T.: 0.000 min
Response: 483129
Conc: 142.74 ng/ml

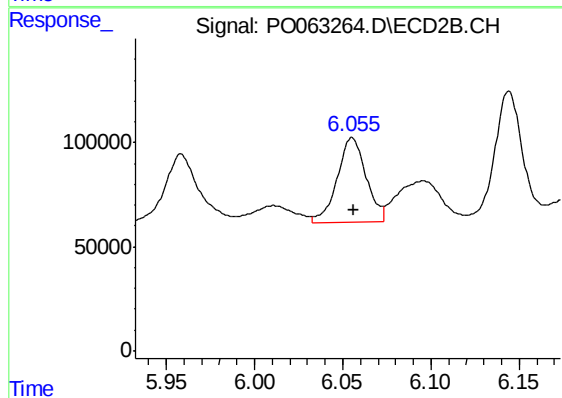

#29 AR-1254-4

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 457330
Conc: 160.49 ng/ml

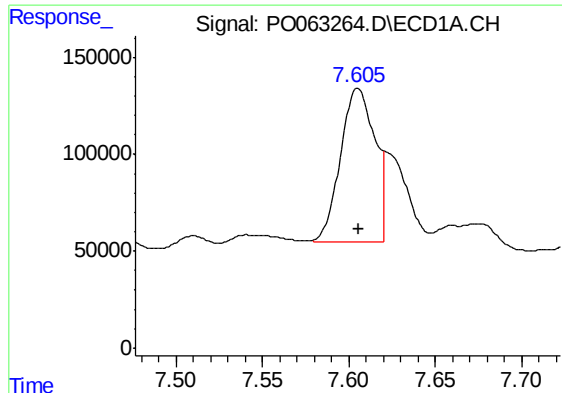


#30 AR-1254-5

R.T.: 7.605 min
Delta R.T.: -0.001 min
Response: 1102573
Conc: 332.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-8B

Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:38 PM

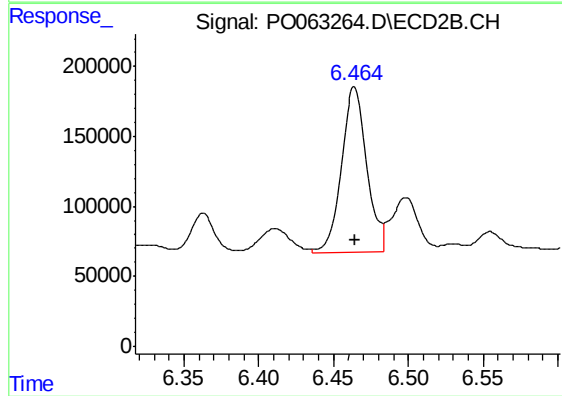

#30 AR-1254-5

R.T.: 6.464 min
Delta R.T.: 0.000 min
Response: 1395290
Conc: 374.31 ng/ml