

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102919\
 Data File : P0063266.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 2:00
 Operator : HP/AJ
 Sample : K5584-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-9A-(2-4)

Manual Integrations
 APPROVED

Ankita
 10/30/2019 1:59:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:14:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.317	3.481	1374305	1337861	23.581	24.497
2)	SA Decachlor...	9.933	8.321	919236	599939	15.799m	14.033
Target Compounds							
26)	L6 AR-1254-1	6.322	5.296	4937752	4744612	1942.150	1575.084
27)	L6 AR-1254-2	6.539	5.441	10081795	7346015	2492.400	2723.771
28)	L6 AR-1254-3	6.904	5.832	15271513	13981263	3587.887	3256.599
29)	L6 AR-1254-4	7.188	6.056	10438834	8693067	3084.039	3050.578
30)	L6 AR-1254-5	7.605	6.464	17889575	23133235	5393.286	6205.858

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102919\
Data File : PO063266.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 2:00
Operator : HP/AJ
Sample : K5584-02
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
445X-9A-(2-4)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:14:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

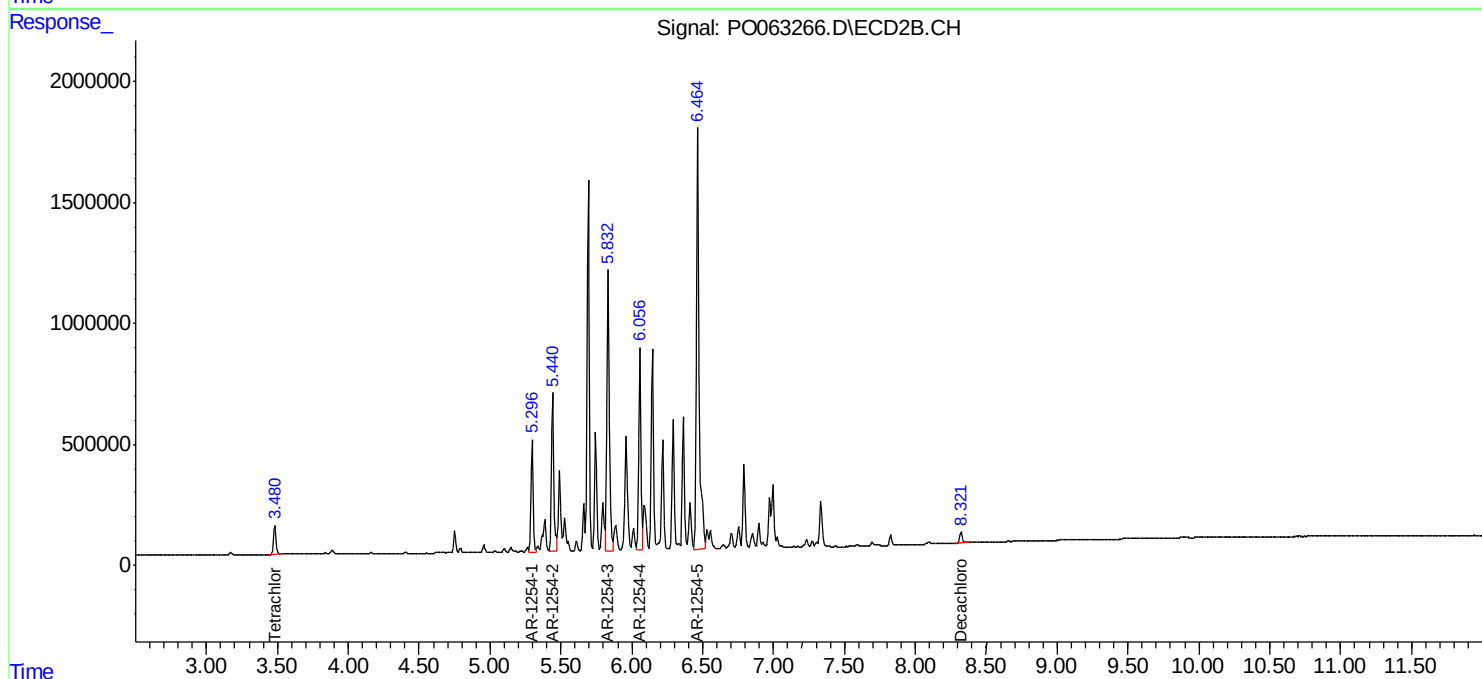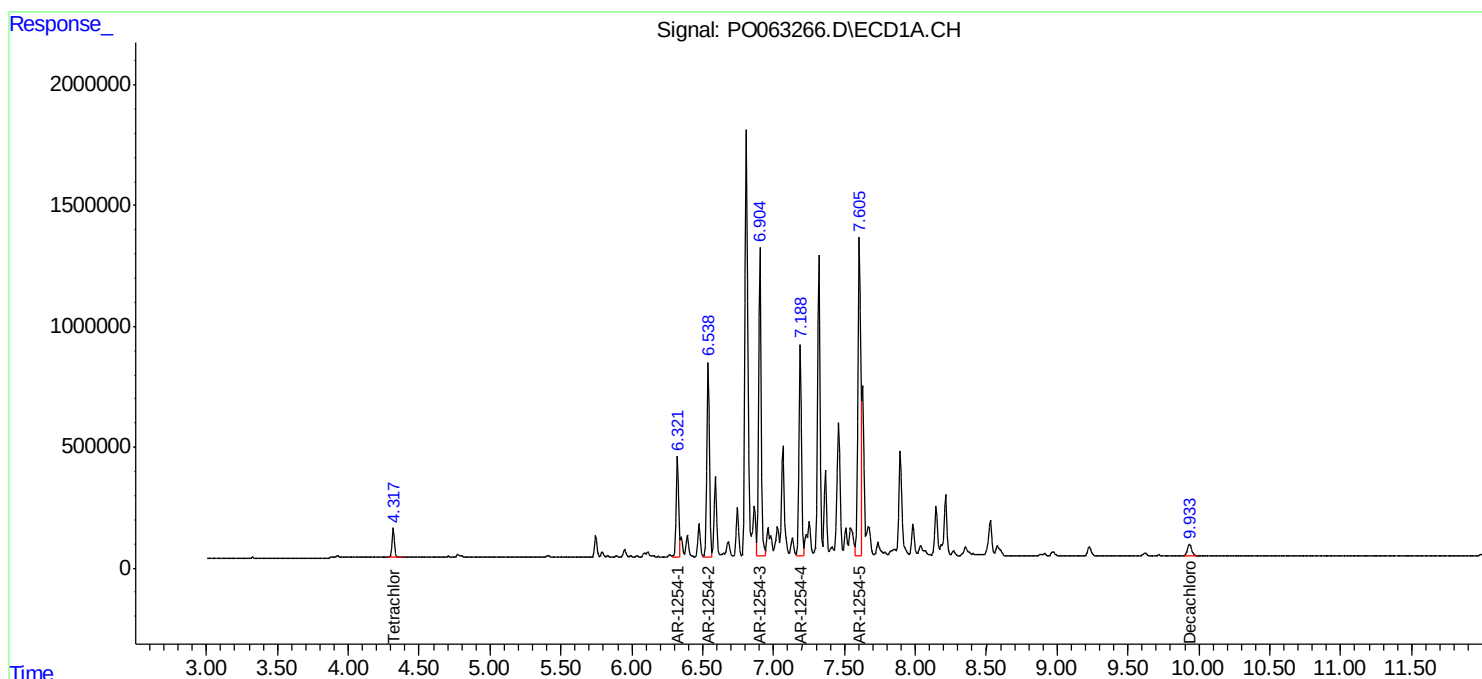

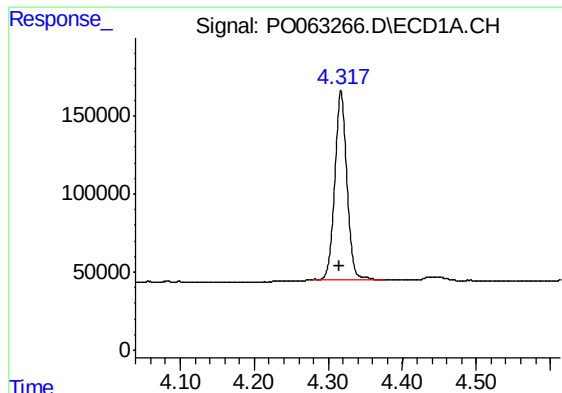


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: 0.001 min
Response: 1374305
Conc: 23.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:42 PM

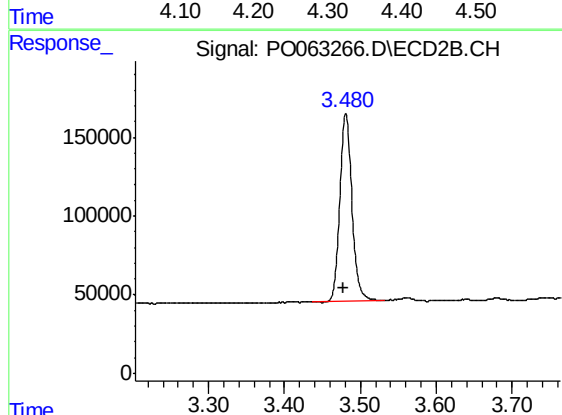


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.003 min
Response: 1337861
Conc: 24.50 ng/ml

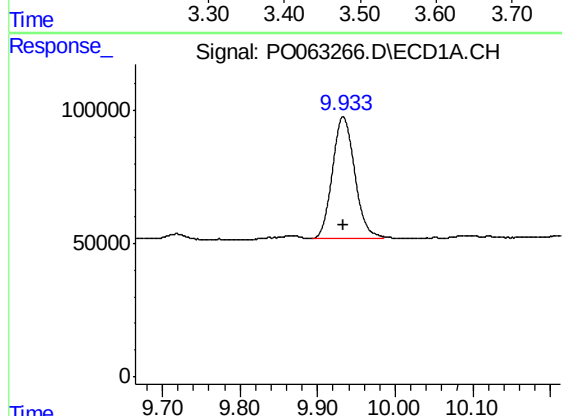


#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.001 min
Response: 919236
Conc: 15.80 ng/ml m

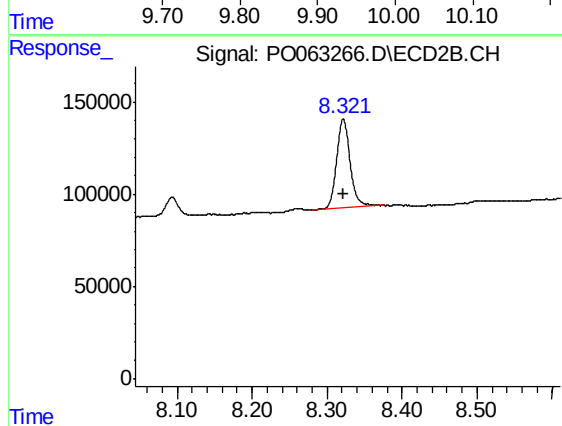

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 599939
Conc: 14.03 ng/ml

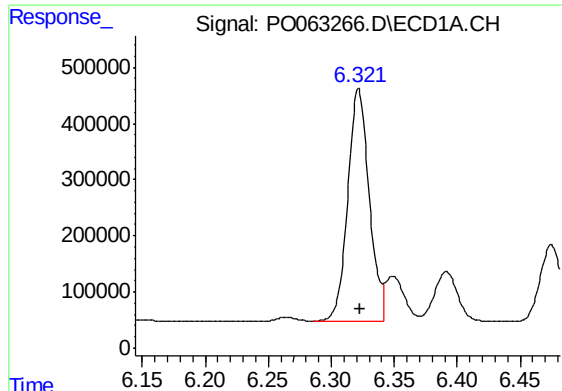


#26 AR-1254-1

R.T.: 6.322 min
Delta R.T.: -0.001 min
Response: 4937752
Conc: 1942.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:42 PM

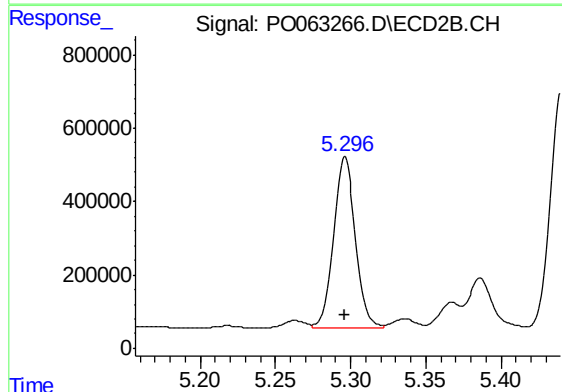


#26 AR-1254-1

R.T.: 5.296 min
Delta R.T.: 0.000 min
Response: 4744612
Conc: 1575.08 ng/ml

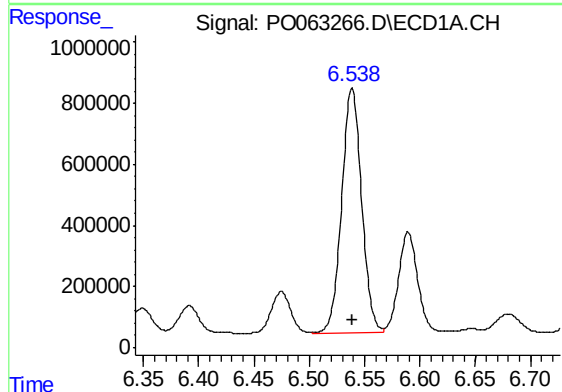


#27 AR-1254-2

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 10081795
Conc: 2492.40 ng/ml

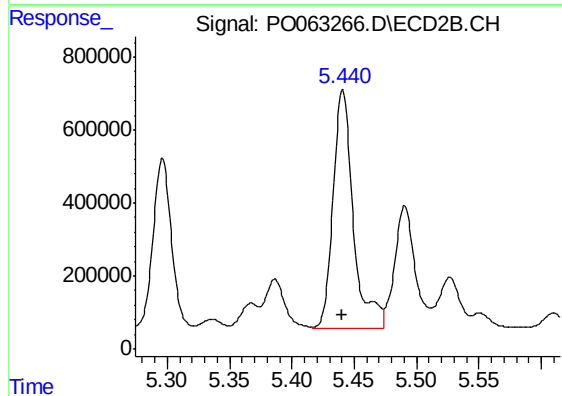

#27 AR-1254-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 7346015
Conc: 2723.77 ng/ml

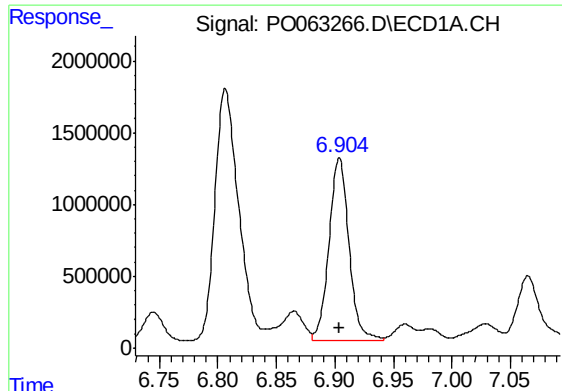


#28 AR-1254-3

R.T.: 6.904 min
Delta R.T.: 0.000 min
Response: 15271513
Conc: 3587.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)


Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:42 PM

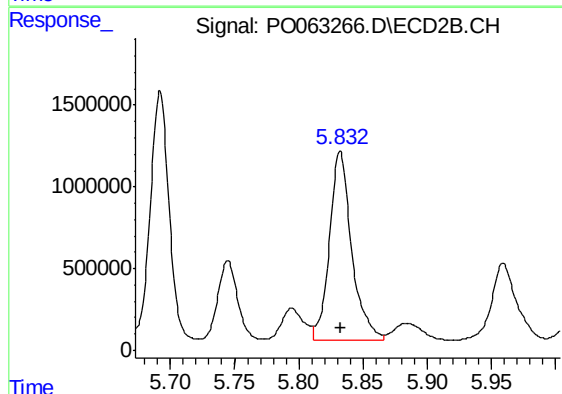


#28 AR-1254-3

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 13981263
Conc: 3256.60 ng/ml

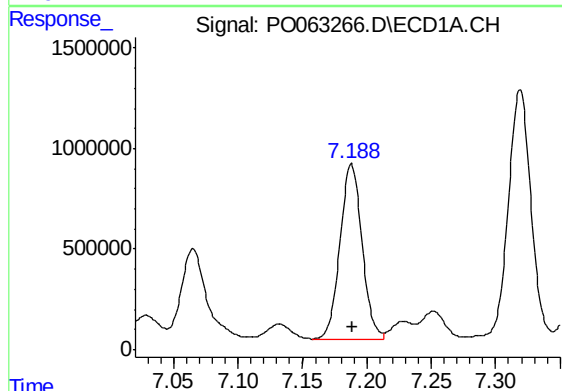


#29 AR-1254-4

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 10438834
Conc: 3084.04 ng/ml

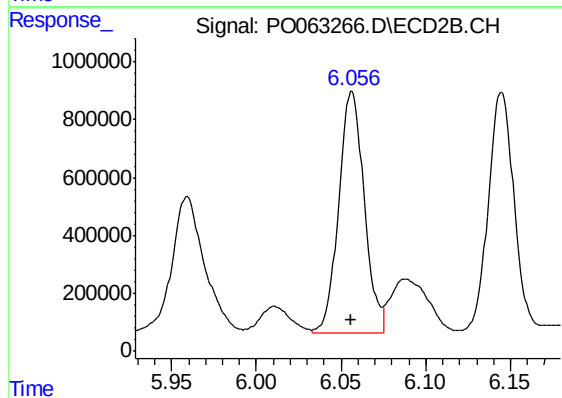

#29 AR-1254-4

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 8693067
Conc: 3050.58 ng/ml

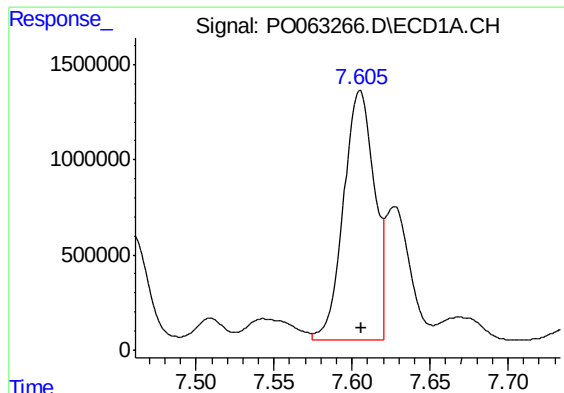


#30 AR-1254-5

R.T.: 7.605 min
Delta R.T.: 0.000 min
Response: 17889575
Conc: 5393.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)

Manual Integrations
APPROVED

Ankita
10/30/2019 1:59:42 PM

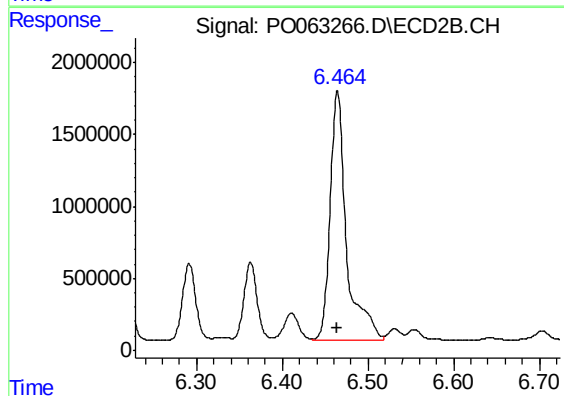

#30 AR-1254-5

R.T.: 6.464 min
Delta R.T.: 0.000 min
Response: 23133235
Conc: 6205.86 ng/ml