

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103018\
 Data File : PO050743.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2018 9:24
 Operator : SM/SJ
 Sample : J5688-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DPC-91567-OD-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 09:51:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.354	3.347	10299599	4501904	20.605	20.712
2) SA Decachlor...	10.013	8.094	6588073	5231836	21.195	20.454

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103018\
Data File : P0050743.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2018 9:24
Operator : SM/SJ
Sample : J5688-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DPC-91567-OD-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 09:51:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

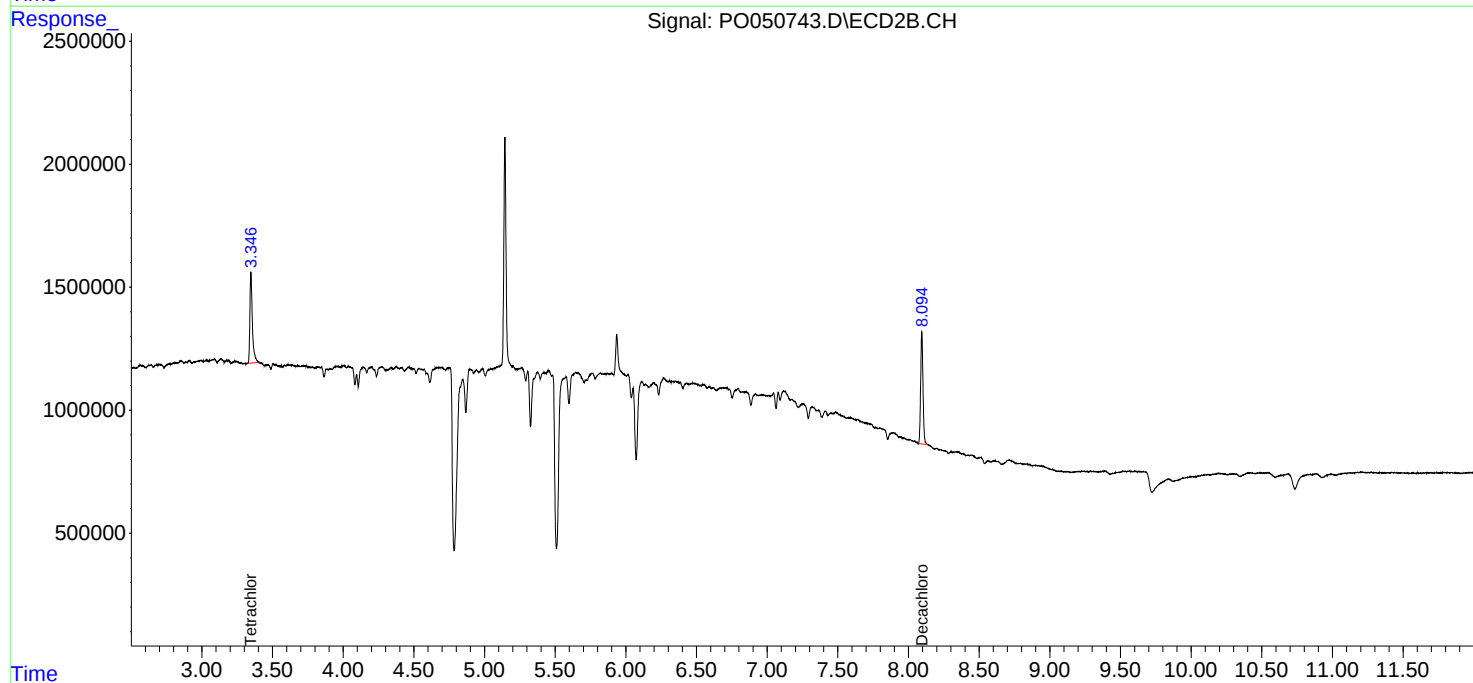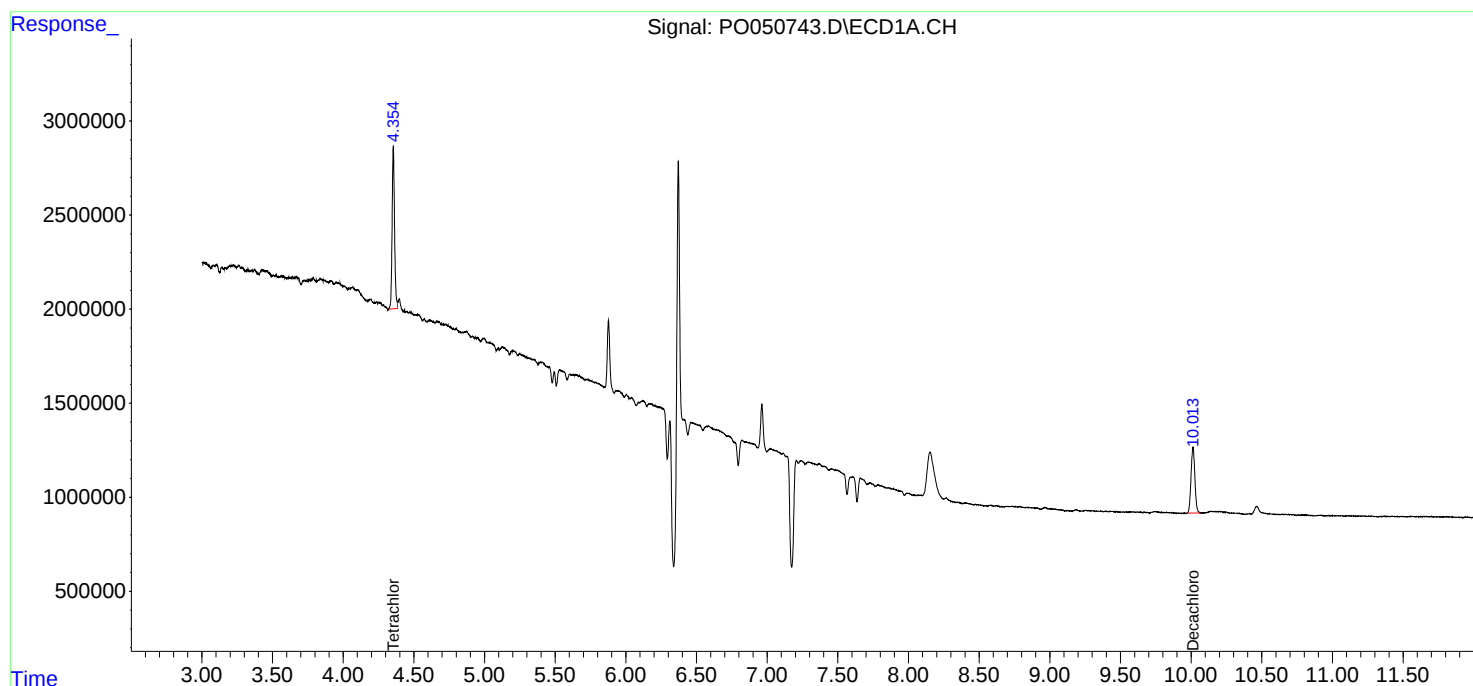


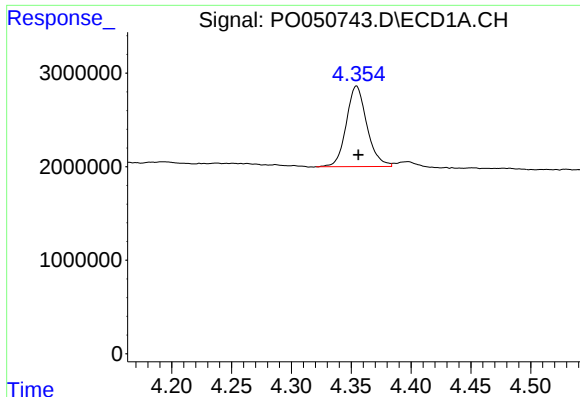

#1 Tetrachloro-m-xylene


R.T.: 4.354 min
Delta R.T.: -0.002 min
Response: 10299599
Conc: 20.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
DPC-91567-OD-01

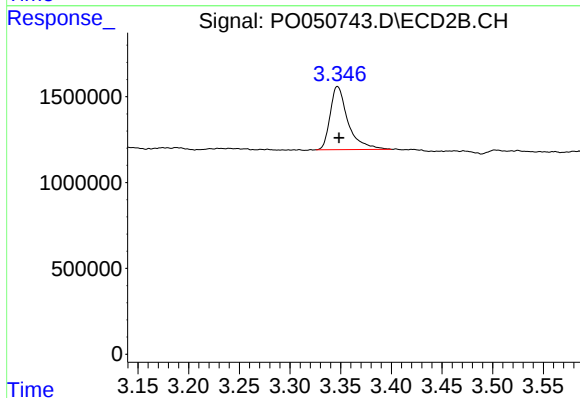


#1 Tetrachloro-m-xylene

R.T.: 3.347 min
Delta R.T.: -0.001 min
Response: 4501904
Conc: 20.71 ng/ml

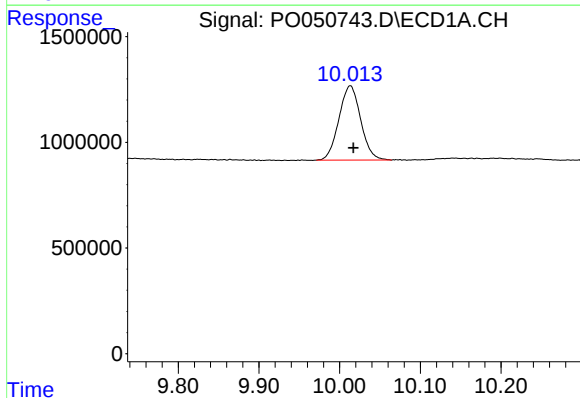

#2 Decachlorobiphenyl

R.T.: 10.013 min
Delta R.T.: -0.004 min
Response: 6588073
Conc: 21.20 ng/ml

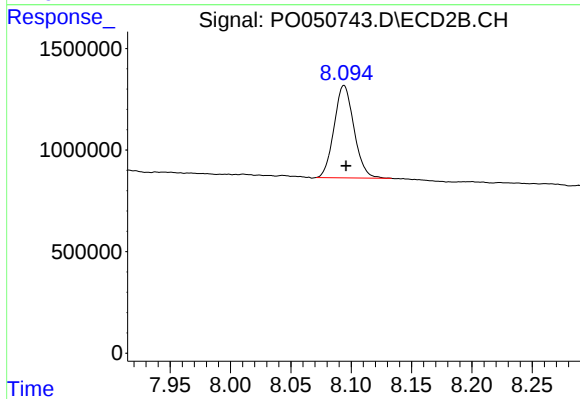

#2 Decachlorobiphenyl

R.T.: 8.094 min
Delta R.T.: -0.002 min
Response: 5231836
Conc: 20.45 ng/ml